

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060622\
 Data File : FF010699.D
 Signal(s) : FID2B.ch
 Acq On : 06 Jun 2022 15:33
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 03:29:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 03:28:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.824	2091090	18.499 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.876	100526	0.820 ug/ml
14) N-DOTRIACONTANE	18.709	154733	1.275 ug/ml
16) N-HEXATRIACONTANE	20.273	138003	1.605 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060622\
Data File : FF010699.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2022 15:33
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 03:29:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 03:28:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

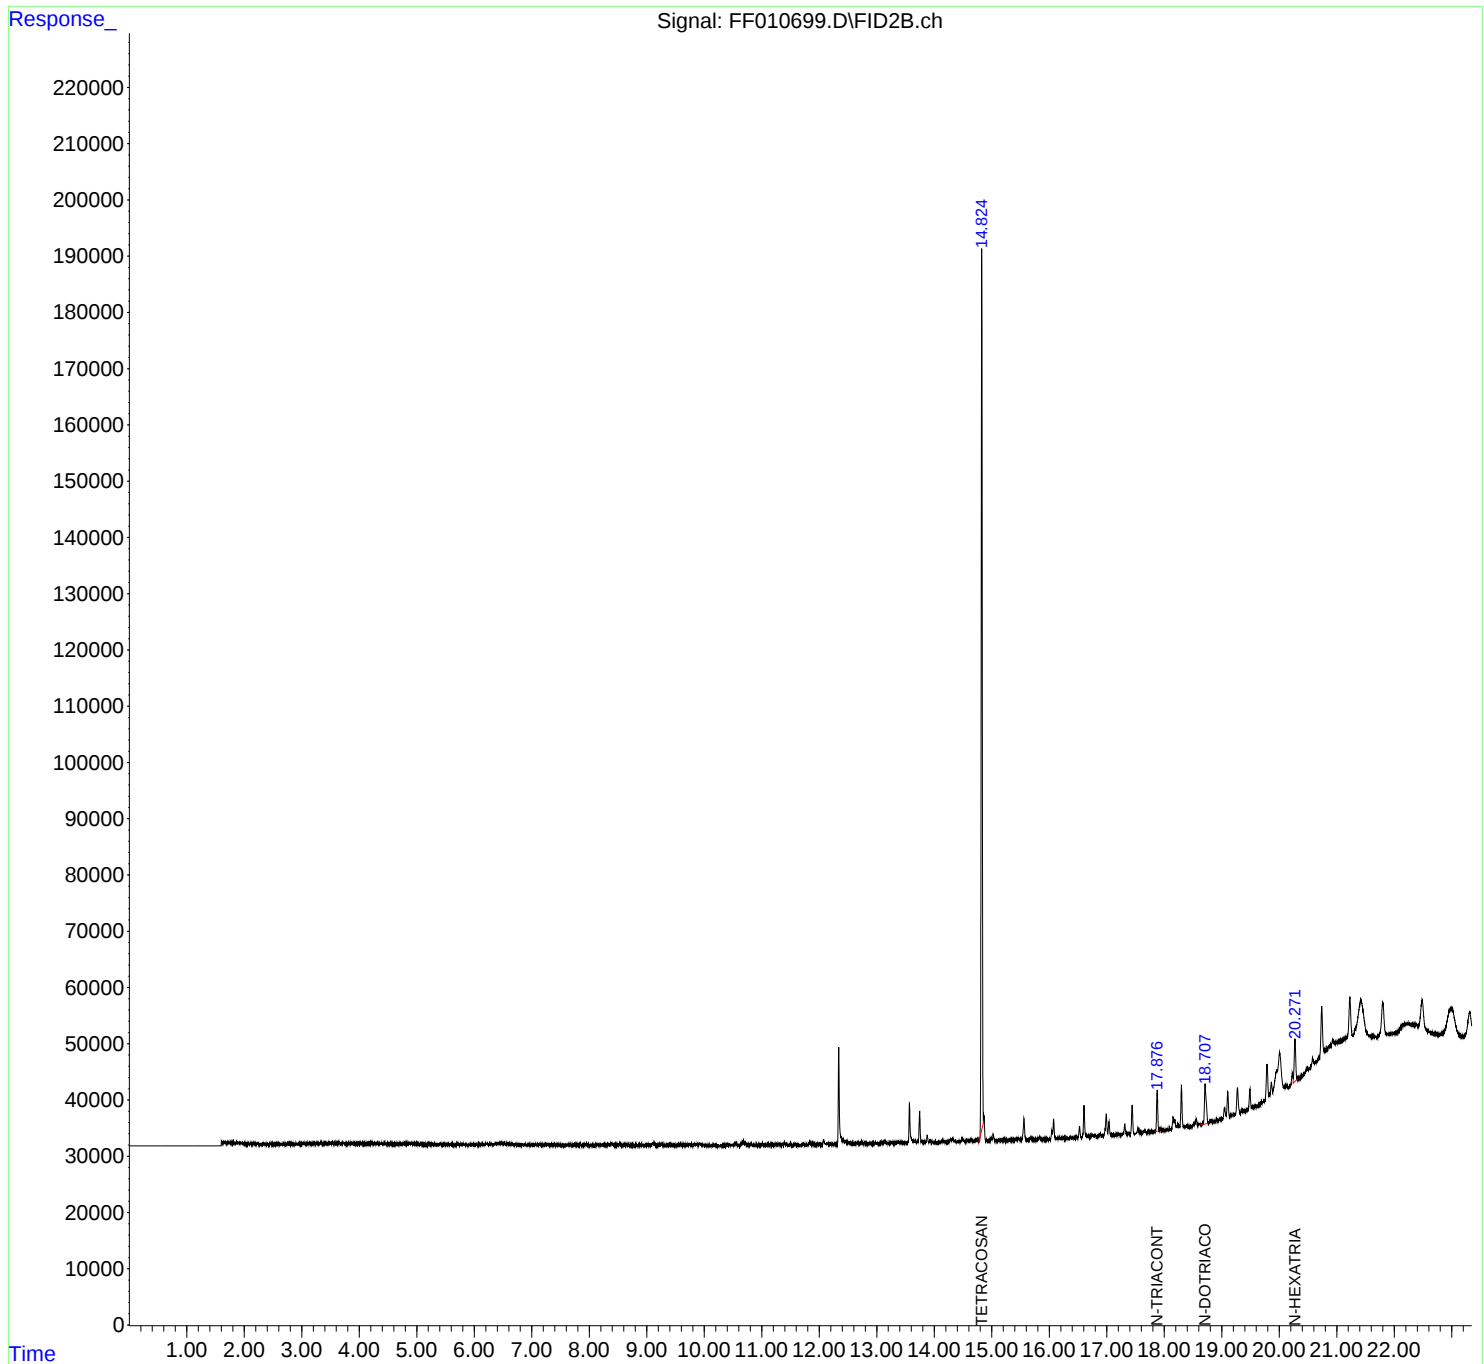


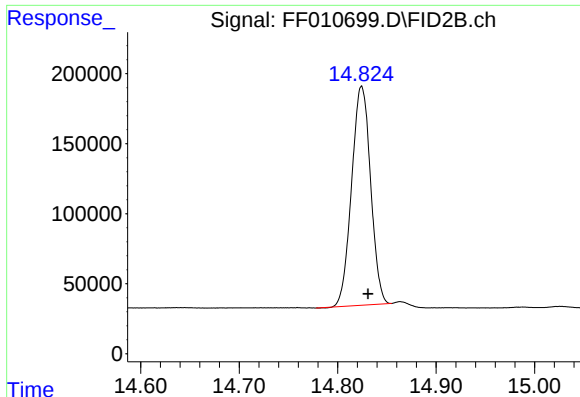

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.824 min
Delta R.T.: -0.007 min
Response: 2091090
Conc: 18.50 ug/ml

Instrument :
FID_F
ClientSampleId :

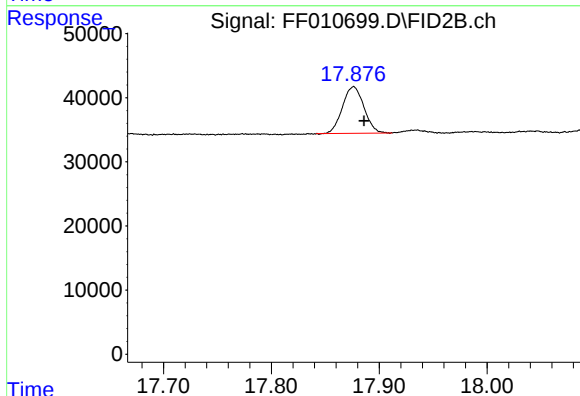


#13 N-TRIACONTANE

R.T.: 17.876 min
Delta R.T.: -0.010 min
Response: 100526
Conc: 0.82 ug/ml

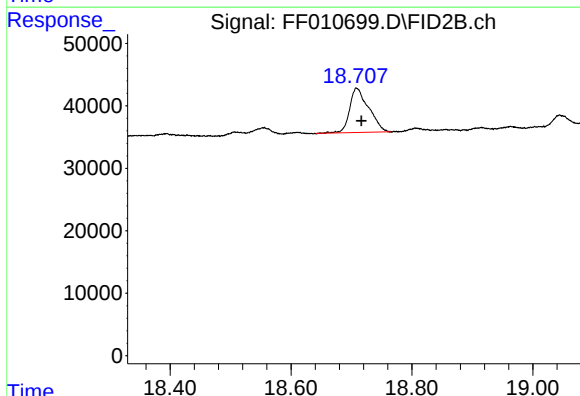

#14 N-DOTRIACONTANE

R.T.: 18.709 min
Delta R.T.: -0.007 min
Response: 154733
Conc: 1.28 ug/ml

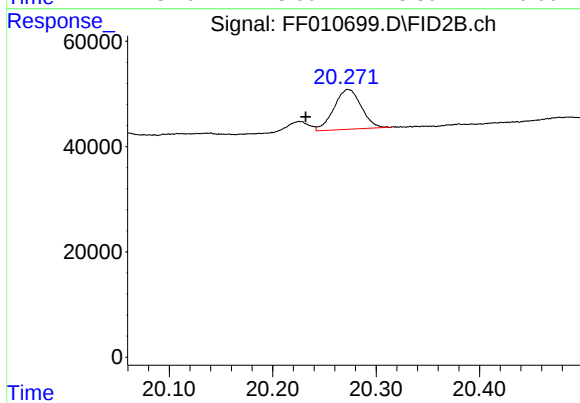

#16 N-HEXATRIACONTANE

R.T.: 20.273 min
Delta R.T.: 0.041 min
Response: 138003
Conc: 1.60 ug/ml