

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060623\
 Data File : FF012830.D
 Signal(s) : FID2B.ch
 Acq On : 06 Jun 2023 11:25
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 00:50:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Fri Jun 02 06:12:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.970	1859985	15.928 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.027	86416	0.670 ug/ml
14) N-DOTRIACONTANE	18.860	108779	0.861 ug/ml
15) N-TETRATRIACONTANE	19.642	83031	0.699 ug/ml
16) N-HEXATRIACONTANE	20.380	52929	0.441 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060623\
Data File : FF012830.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2023 11:25
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 00:50:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

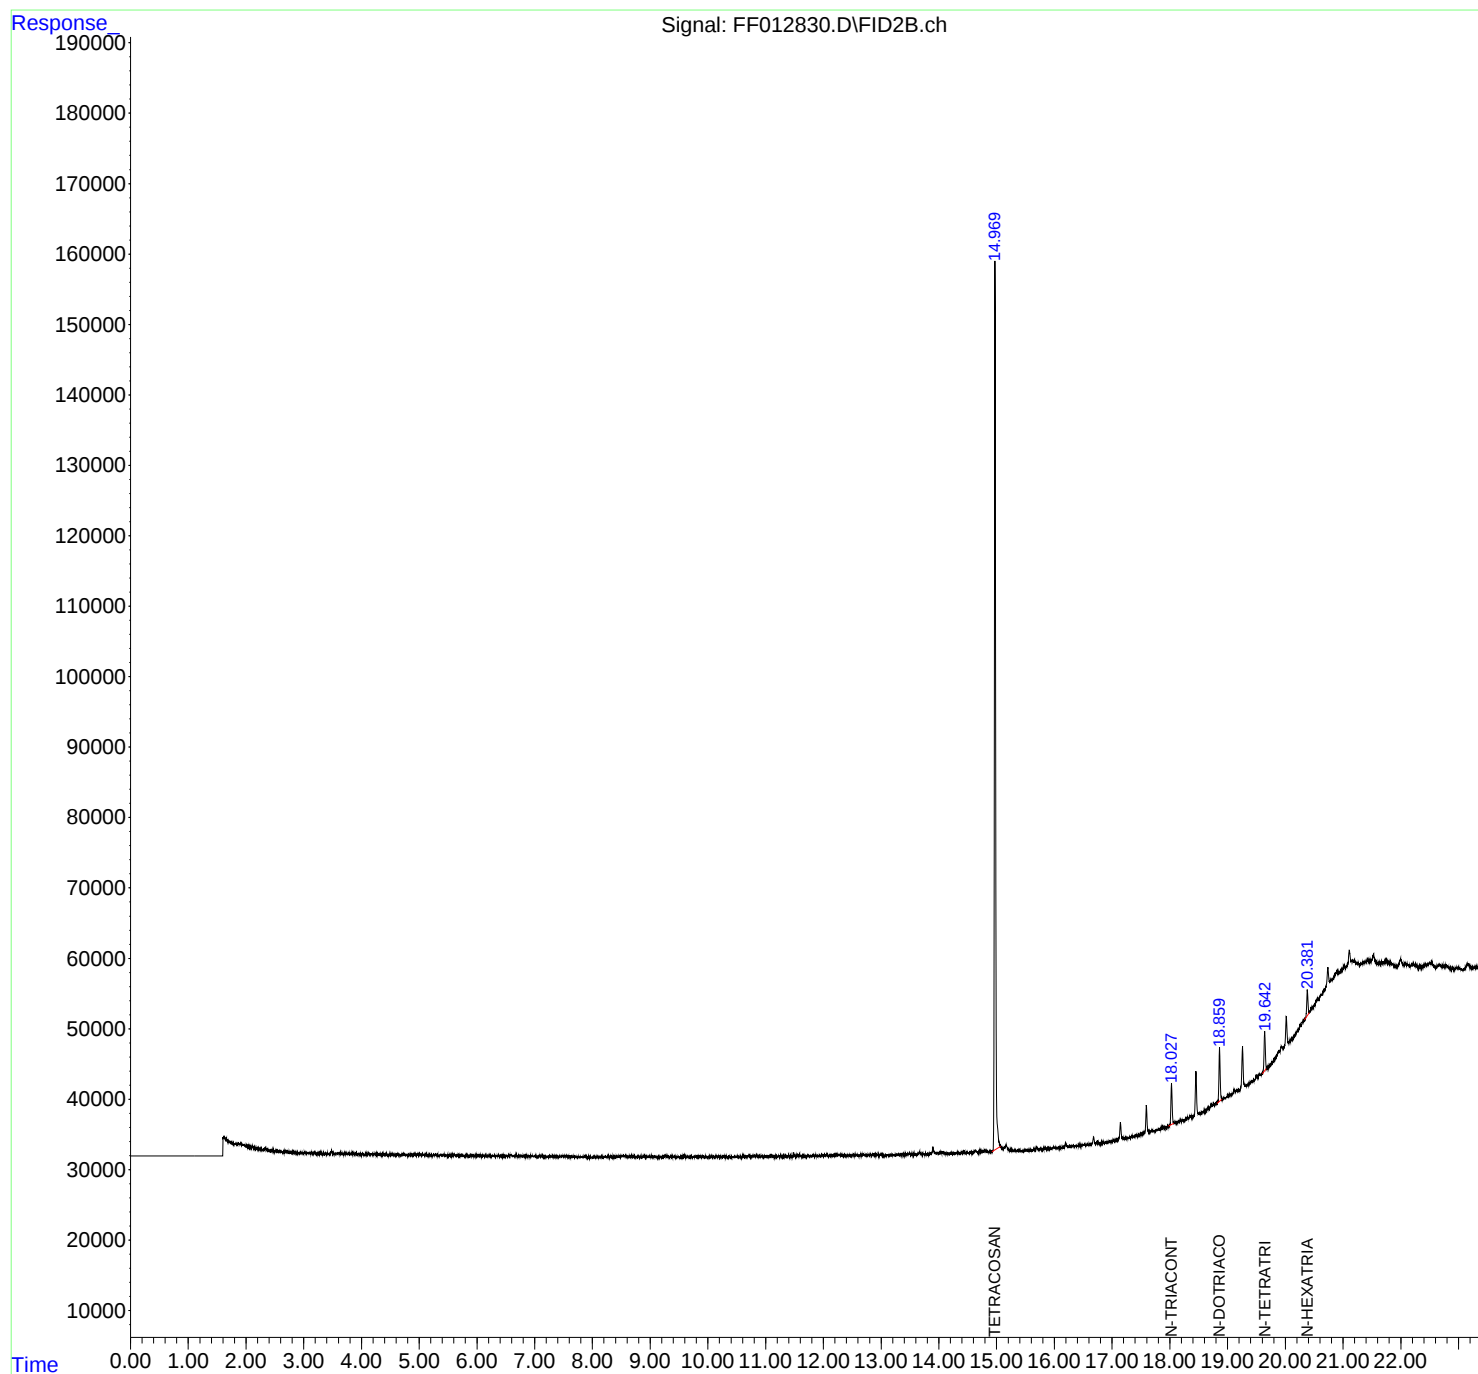


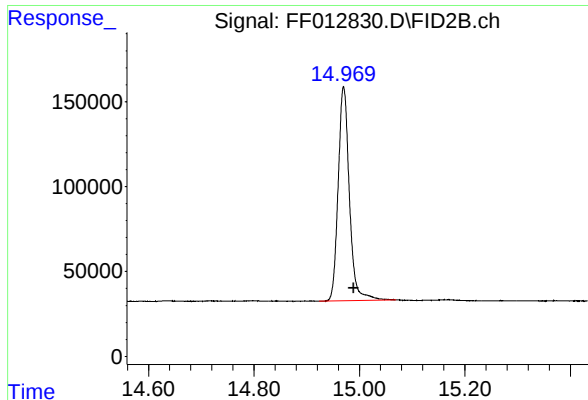

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.970 min
Delta R.T.: -0.019 min
Response: 1859985
Conc: 15.93 ug/ml

Instrument :
FID_F
ClientSampleId :

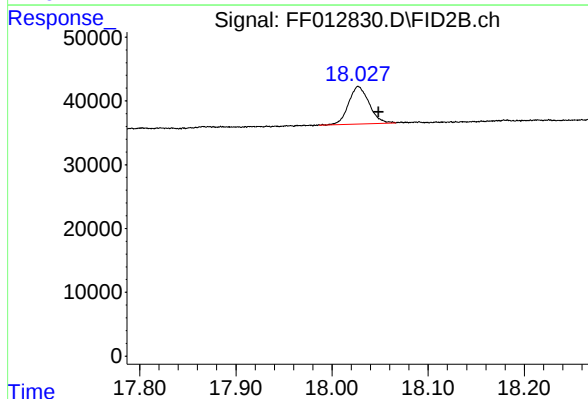


#13 N-TRIACONTANE

R.T.: 18.027 min
Delta R.T.: -0.021 min
Response: 86416
Conc: 0.67 ug/ml

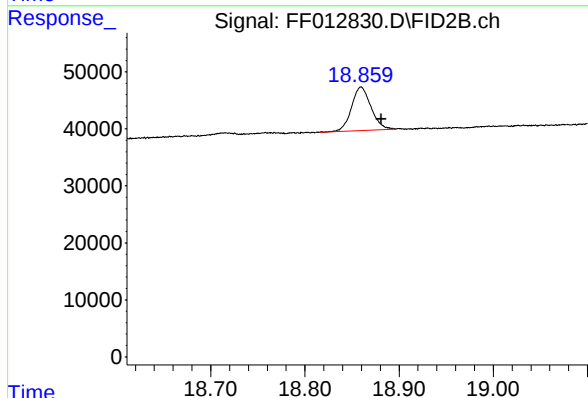


#14 N-DOTRIACONTANE

R.T.: 18.860 min
Delta R.T.: -0.022 min
Response: 108779
Conc: 0.86 ug/ml

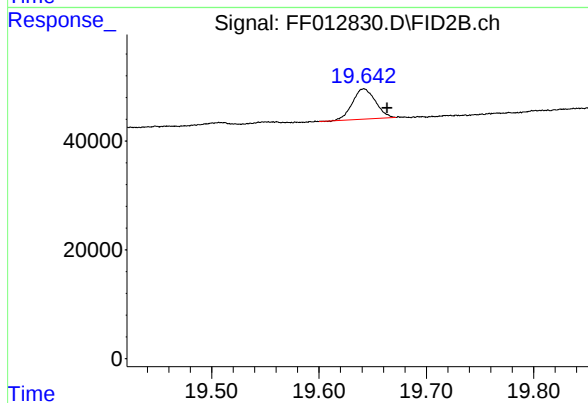

#15 N-TETRATRIACONTANE

R.T.: 19.642 min
Delta R.T.: -0.022 min
Response: 83031
Conc: 0.70 ug/ml

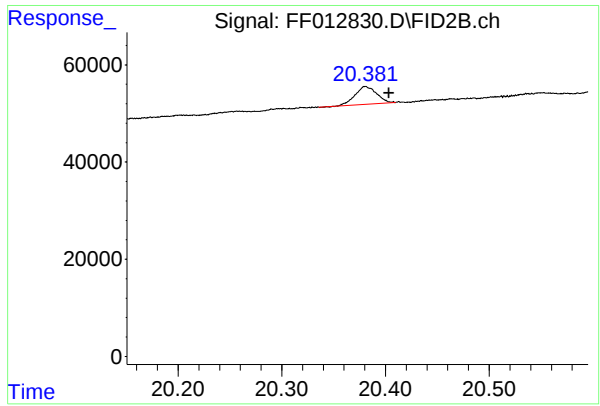

#16 N-HEXATRIACONTANE

R.T.: 20.380 min
Delta R.T.: -0.023 min
Response: 52929
Conc: 0.44 ug/ml

Instrument :

FID_F

ClientSampleId :