

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060623\
Data File : FF012832.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2023 13:35
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 00:50:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.700	1838129	14.104 ug/ml
12) N-OCTACOSANE	17.142	1888244	14.733 ug/ml
14) N-DOTRIACONTANE	18.860	56698	0.449 ug/ml
15) N-TETRATRIACONTANE	19.642	53883	0.454 ug/ml
16) N-HEXATRIACONTANE	20.382	45471	0.379 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060623\
Data File : FF012832.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2023 13:35
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 00:50:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

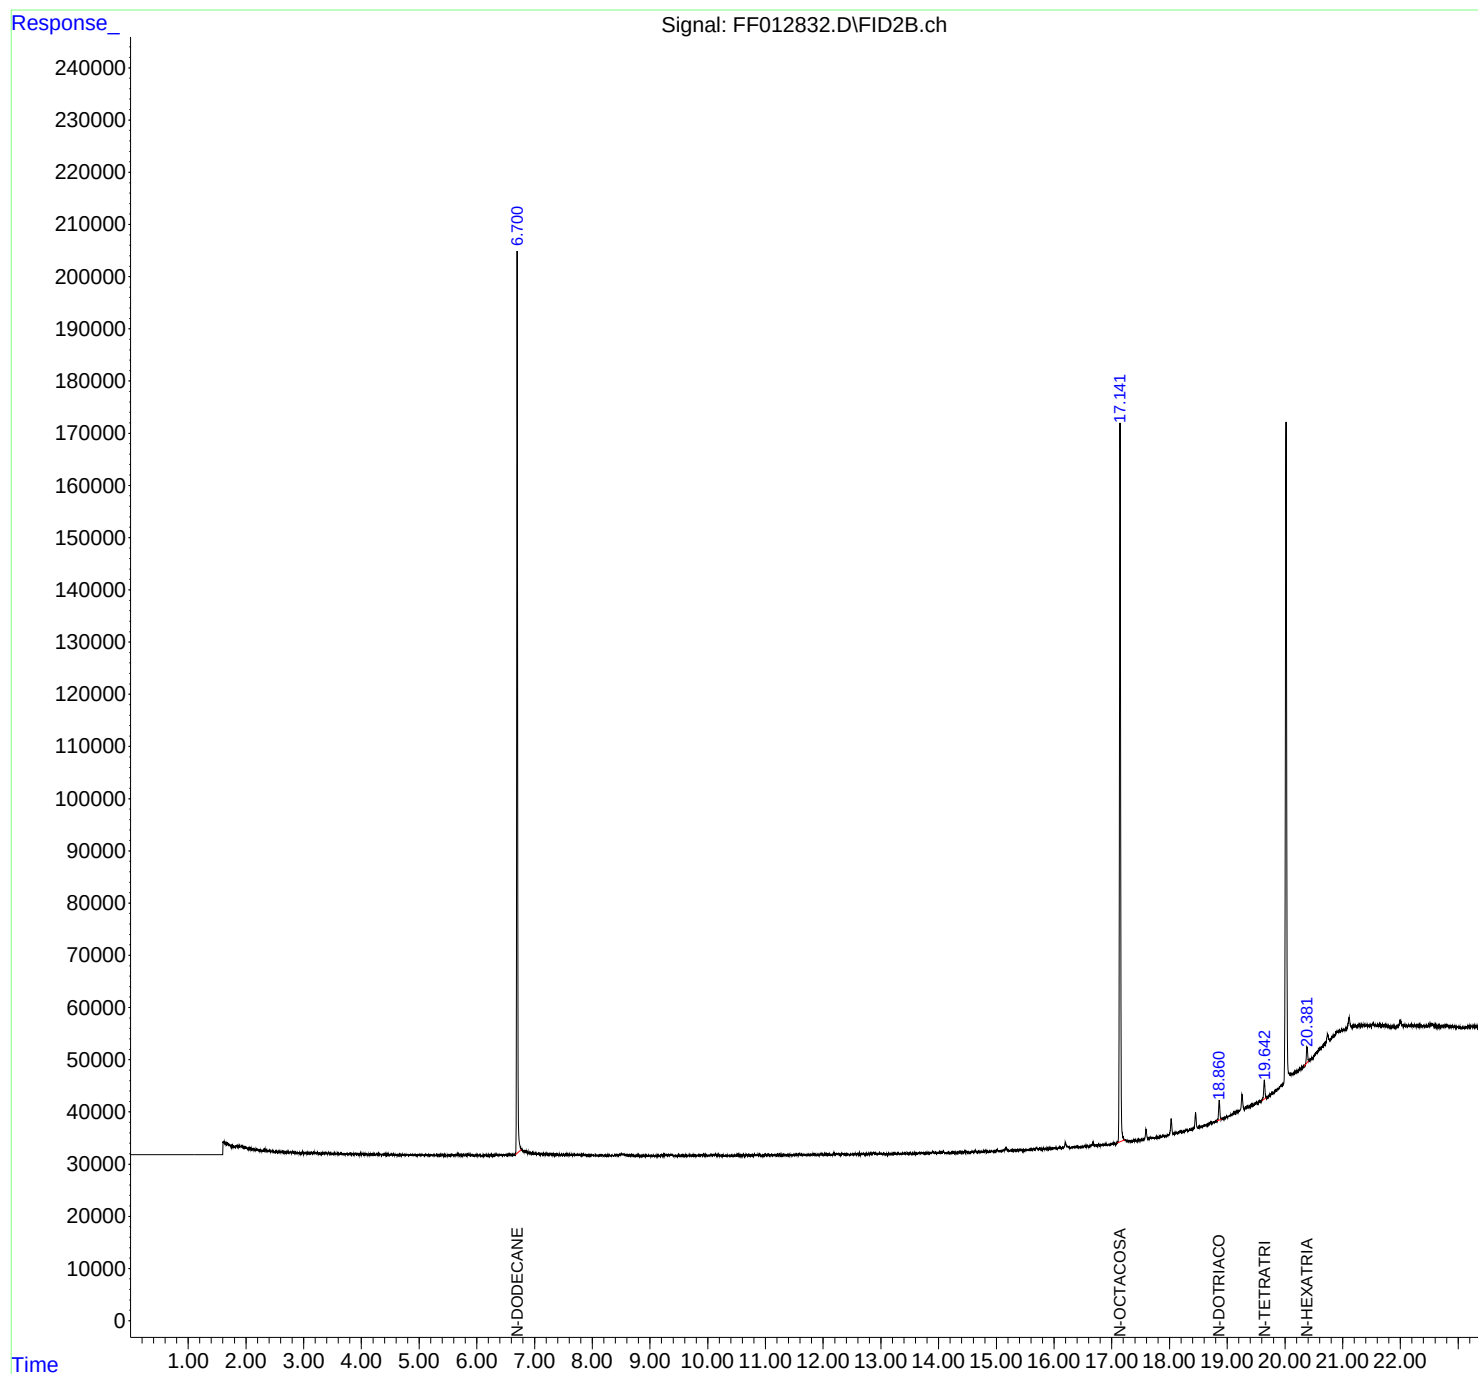


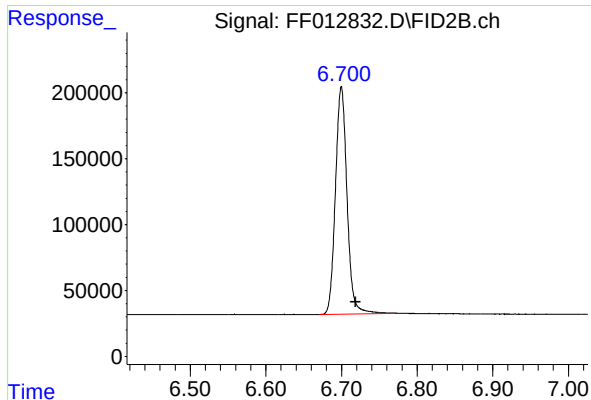

#3 N-DODECANE


R.T.: 6.700 min
Delta R.T.: -0.019 min
Response: 1838129
Conc: 14.10 ug/ml

Instrument :
FID_F
ClientSampleId :

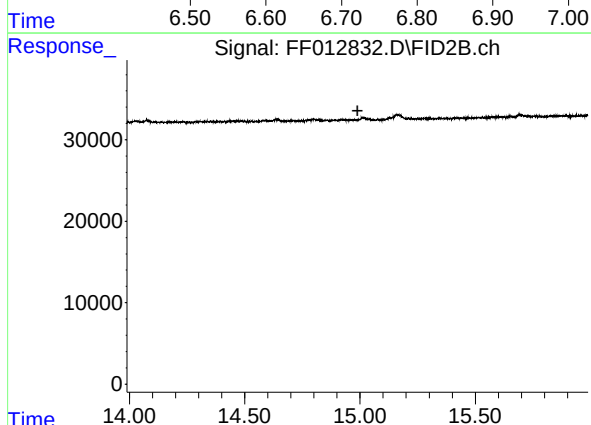


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.989 min
Response: 0
Conc: N.D.

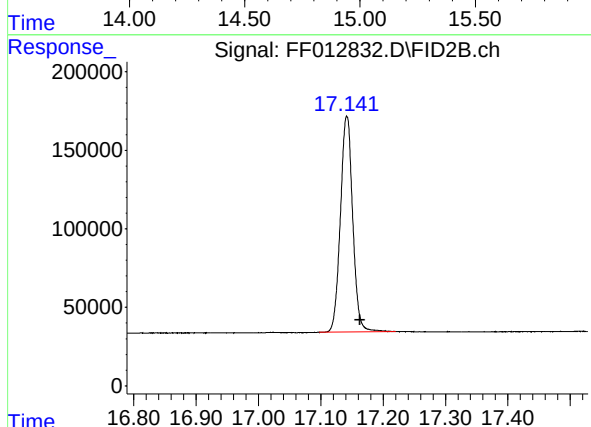


#12 N-OCTACOSANE

R.T.: 17.142 min
Delta R.T.: -0.021 min
Response: 1888244
Conc: 14.73 ug/ml

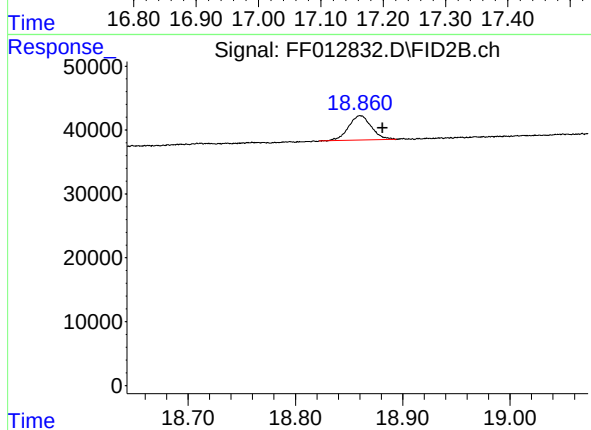

#14 N-DOTRIACONTANE


R.T.: 18.860 min
Delta R.T.: -0.021 min
Response: 56698
Conc: 0.45 ug/ml

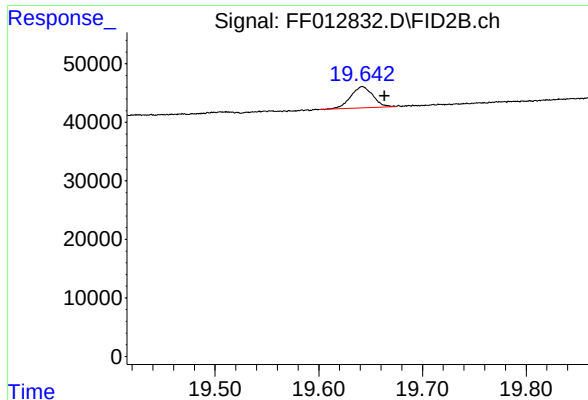

#15 N-TETRATRIACONTANE

R.T.: 19.642 min
Delta R.T.: -0.021 min
Response: 53883
Conc: 0.45 ug/ml

Instrument :
FID_F
ClientSampleId :

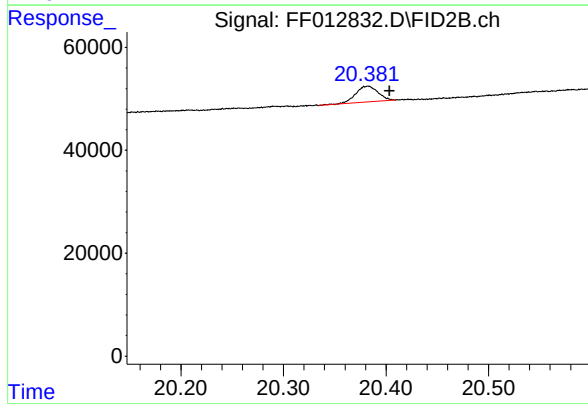

#16 N-HEXATRIACONTANE

R.T.: 20.382 min
Delta R.T.: -0.021 min
Response: 45471
Conc: 0.38 ug/ml