

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060623\
 Data File : FF012833.D
 Signal(s) : FID2B.ch
 Acq On : 06 Jun 2023 16:20
 Operator : YP\AJ
 Sample : PB153244BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 00:50:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Fri Jun 02 06:12:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.968	1798547	15.401 ug/ml
Target Compounds			
10) N-TETRACOSANE	15.153	103658	0.784 ug/ml
13) N-TRIACONTANE	18.025	50474	0.391 ug/ml
14) N-DOTRIACONTANE	18.858	84103	0.665 ug/ml
15) N-TETRATRIACONTANE	19.640	60448	0.509 ug/ml
16) N-HEXATRIACONTANE	20.380	58070	0.484 ug/ml
17) N-OCTATRIACONTANE	21.108	73064	0.628 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060623\
Data File : FF012833.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2023 16:20
Operator : YP\AJ
Sample : PB153244BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 00:50:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

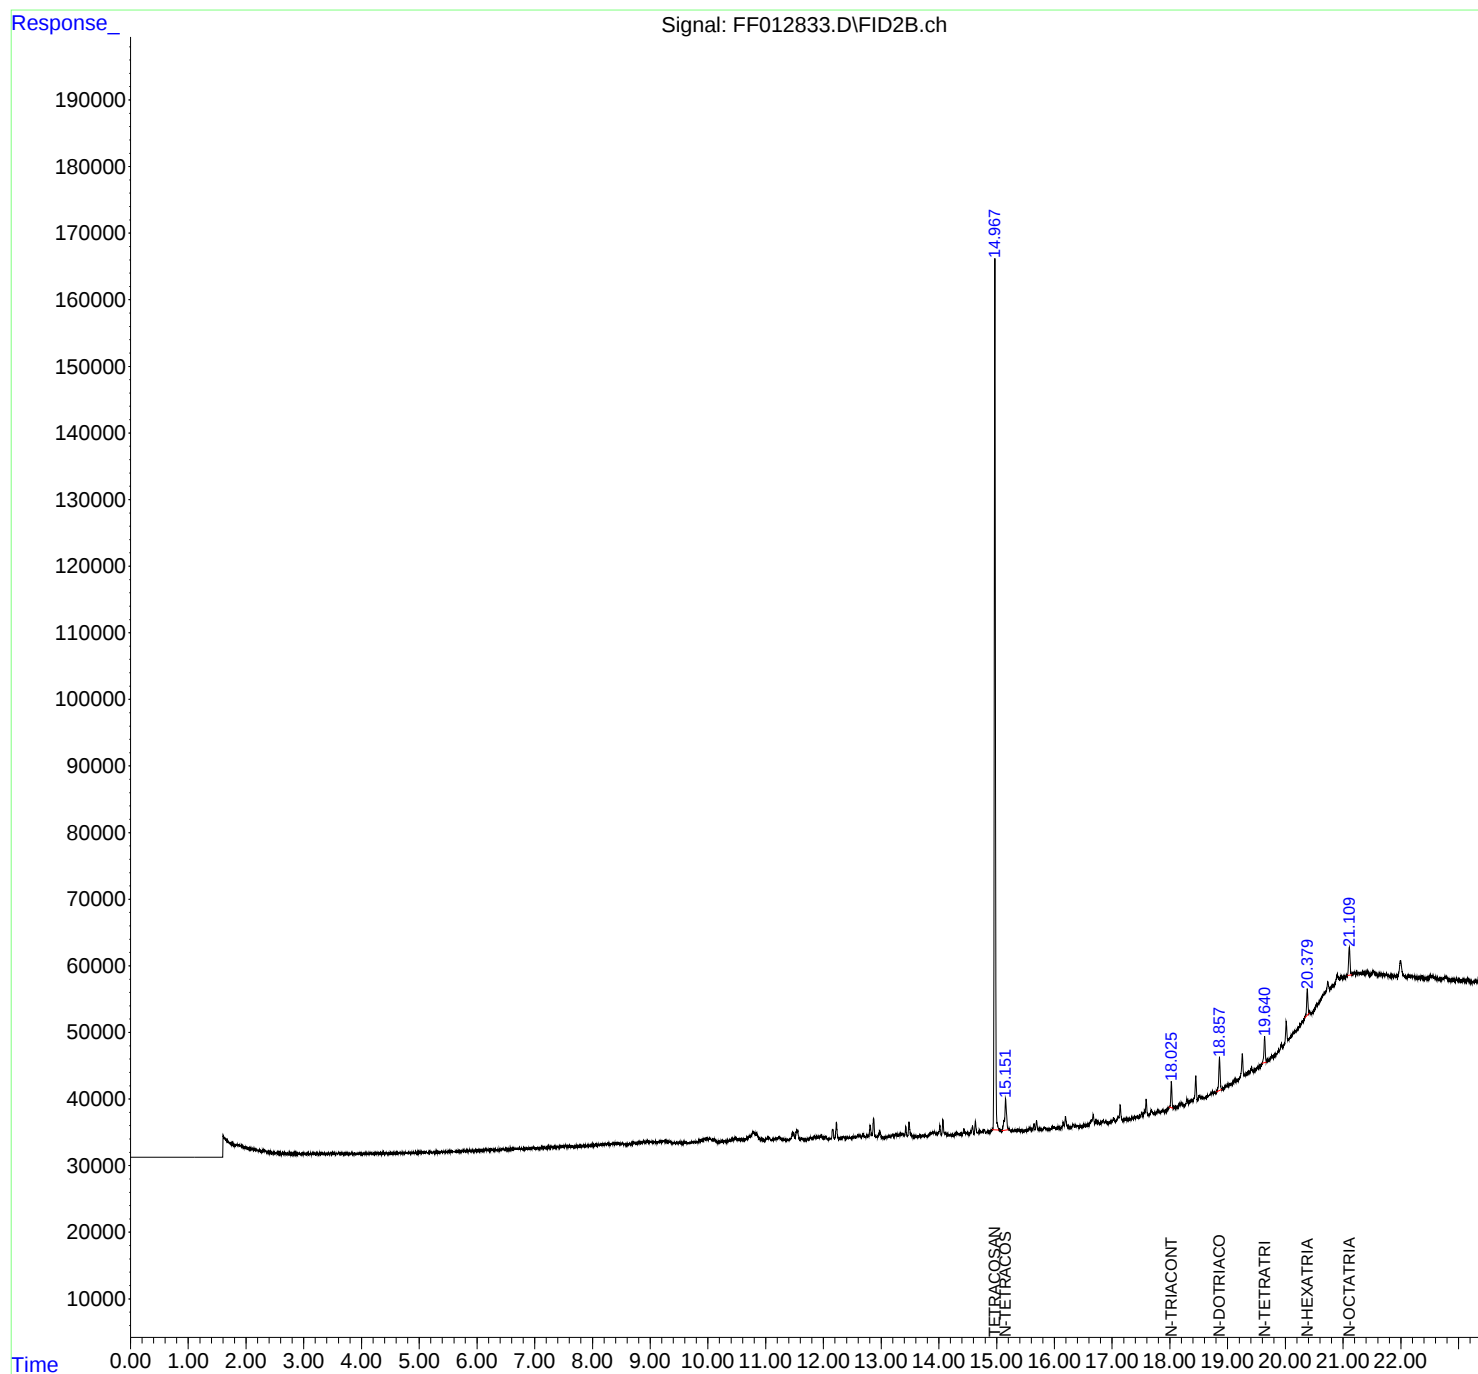


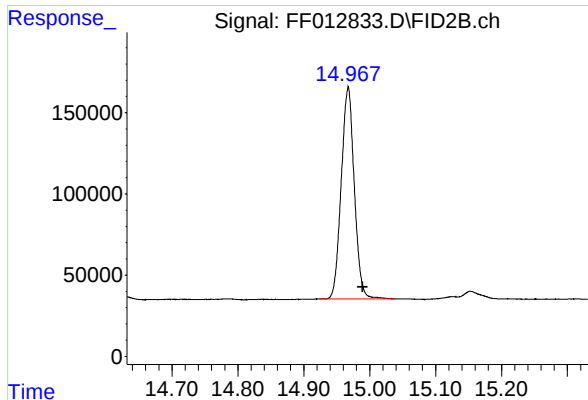

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.968 min
Delta R.T.: -0.022 min
Response: 1798547
Conc: 15.40 ug/ml

Instrument :
FID_F
ClientSampleId :

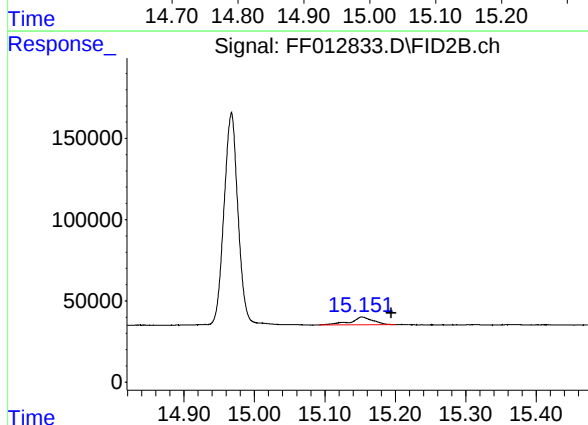


#10 N-TETRACOSANE

R.T.: 15.153 min
Delta R.T.: -0.042 min
Response: 103658
Conc: 0.78 ug/ml

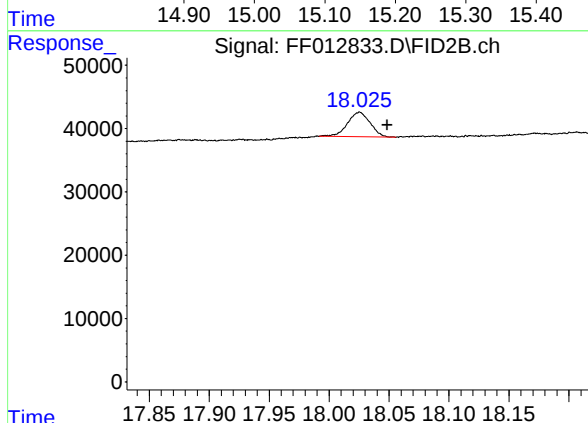


#13 N-TRIACONTANE

R.T.: 18.025 min
Delta R.T.: -0.023 min
Response: 50474
Conc: 0.39 ug/ml

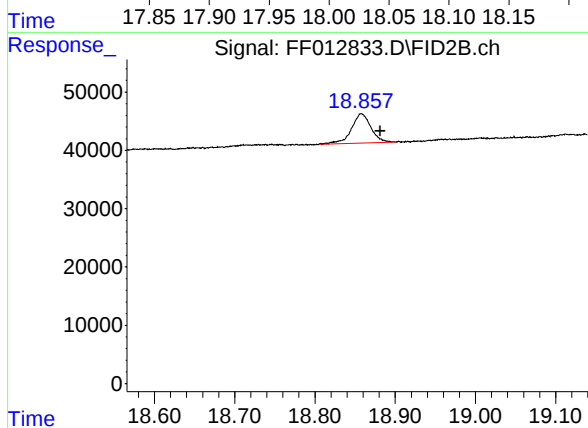

#14 N-DOTRIACONTANE


R.T.: 18.858 min
Delta R.T.: -0.024 min
Response: 84103
Conc: 0.67 ug/ml

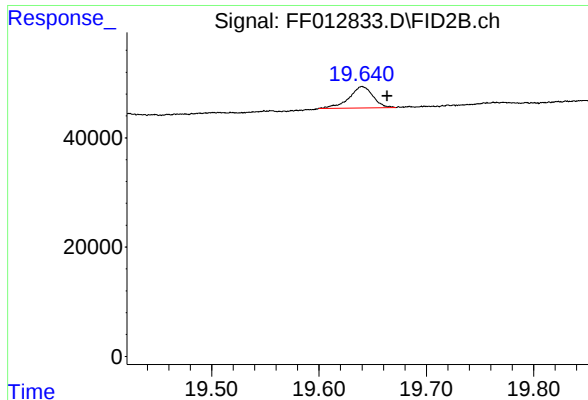

#15 N-TETRATRIACONTANE


R.T.: 19.640 min
Delta R.T.: -0.023 min
Response: 60448
Conc: 0.51 ug/ml

Instrument :
FID_F
ClientSampleId :

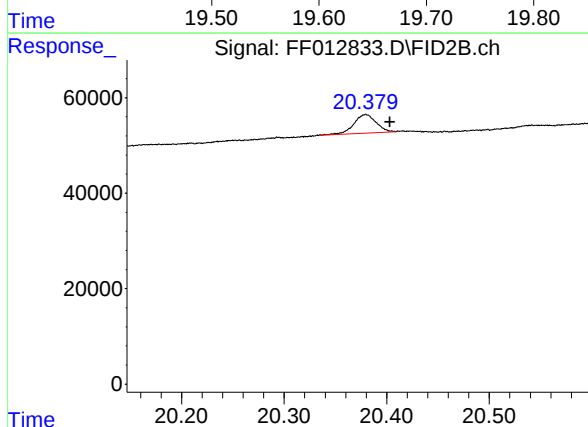

#16 N-HEXATRIACONTANE

R.T.: 20.380 min
Delta R.T.: -0.024 min
Response: 58070
Conc: 0.48 ug/ml

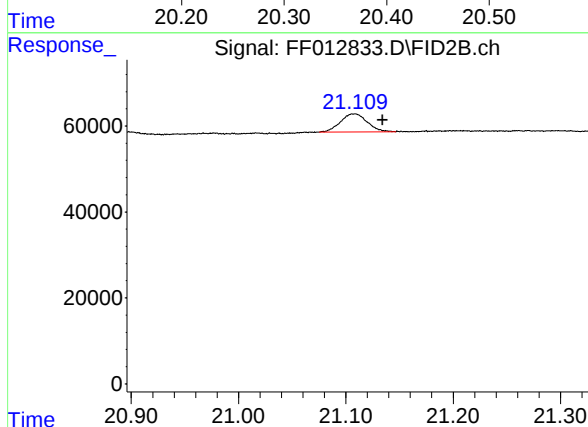

#17 N-OCTATRIACONTANE

R.T.: 21.108 min
Delta R.T.: -0.027 min
Response: 73064
Conc: 0.63 ug/ml