

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060623\
Data File : FF012838.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2023 18:48
Operator : YP\AJ
Sample : 03044-04
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-02-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

Integration File: autoint1.e
Quant Time: Jun 07 00:51:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.970	917921	7.860 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060623\
Data File : FF012838.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2023 18:48
Operator : YP\AJ
Sample : 03044-04
Misc :
ALS Vial : 66 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SB-02-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

Integration File: autoint1.e
Quant Time: Jun 07 00:51:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

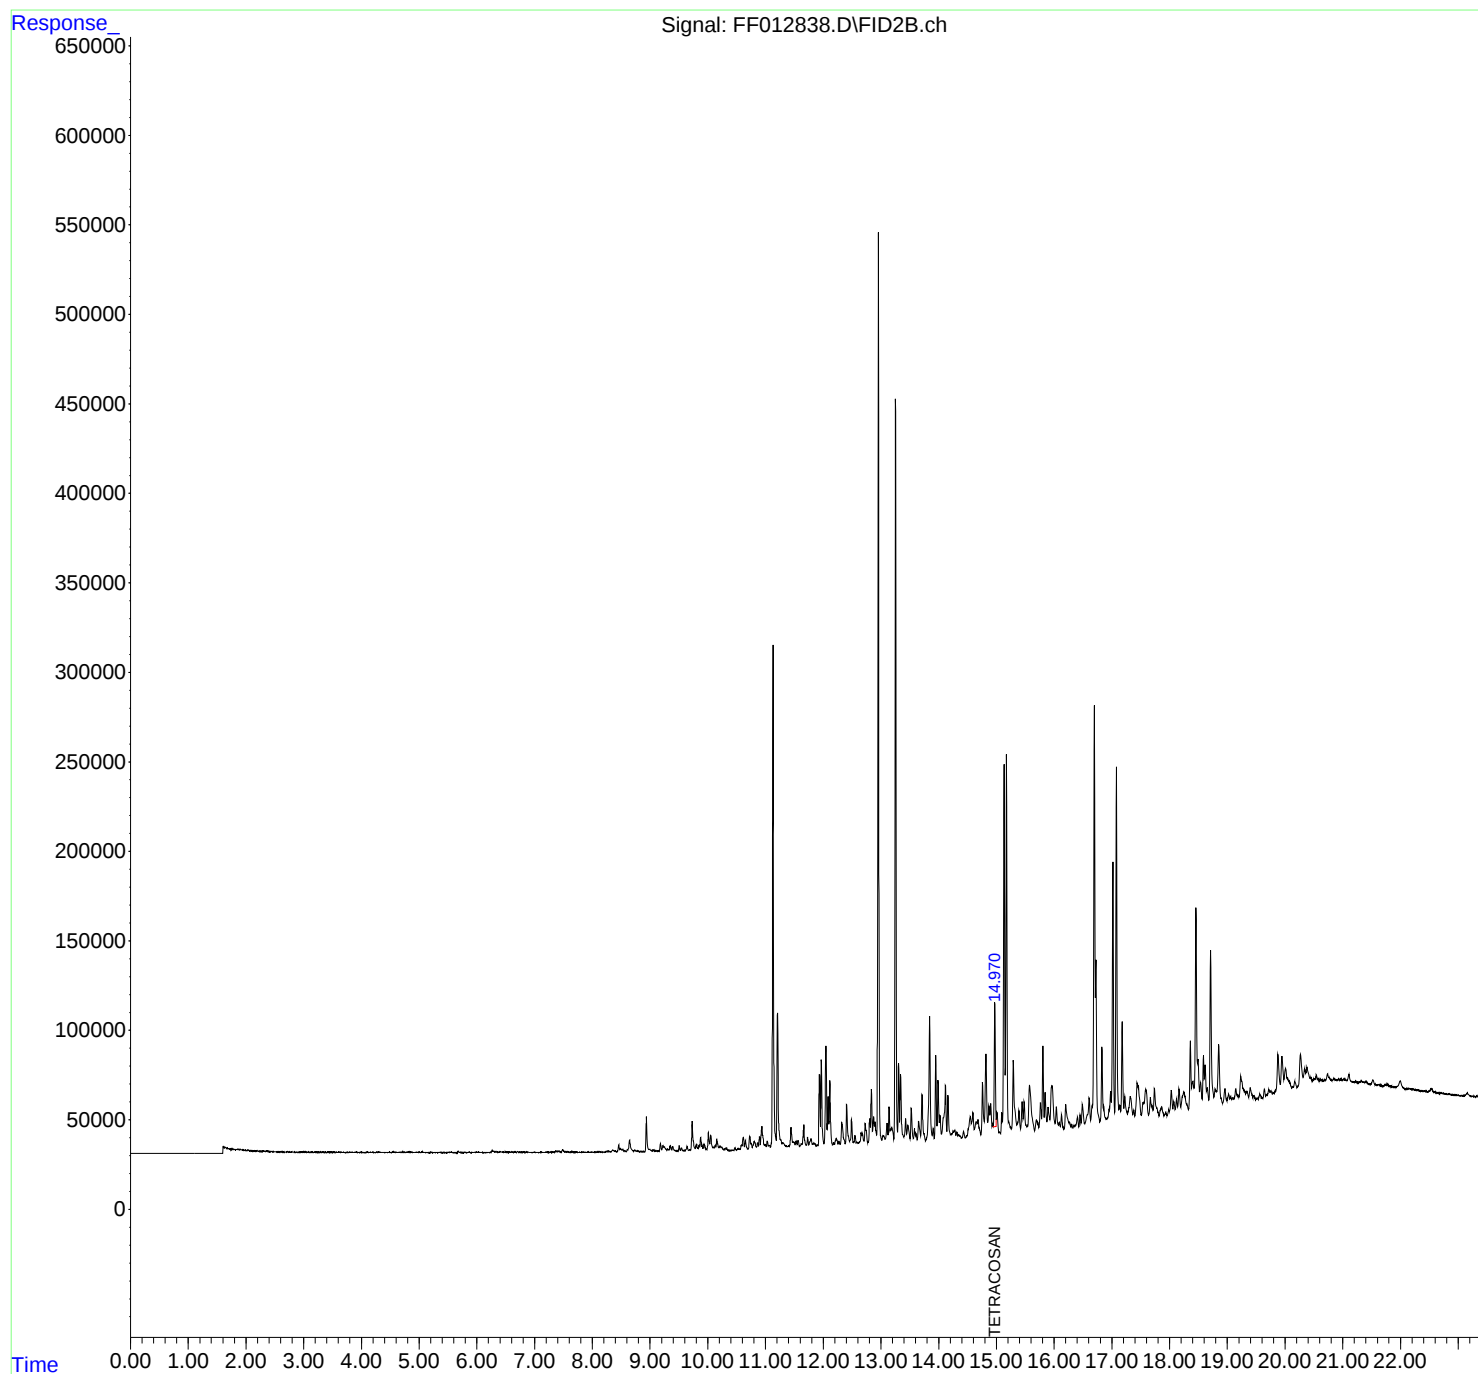

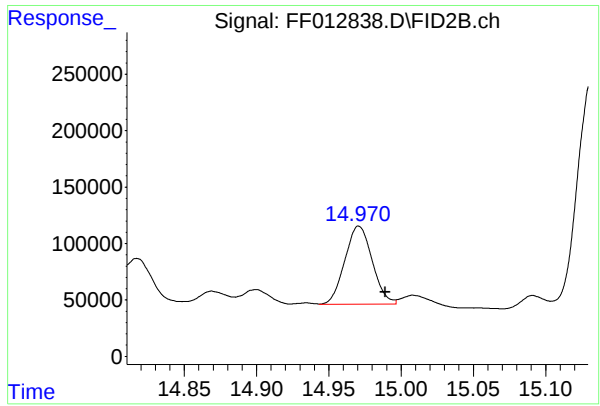

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.970 min
Delta R.T.: -0.019 min
Response: 917921
Conc: 7.86 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-02-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023