

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
 Data File : FF004735.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jun 2019 12:27
 Operator : DD\AJ
 Sample : K3192-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 13:52:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.707	2351687	19.259 ug/ml
Target Compounds			
4) N-TETRADECANE	8.293	740349	5.040 ug/ml
7) N-EICOSANE	12.657f	159861	1.104 ug/ml
10) N-TETRACOSANE	14.909	120158	0.867 ug/ml
11) N-HEXACOSANE	15.936	268646	1.972 ug/ml
12) N-OCTACOSANE	16.890	452370	3.327 ug/ml
13) N-TRIACONTANE	17.784	421010	3.045 ug/ml
14) N-DOTRIACONTANE	18.622	301557	2.180 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
Data File : FF004735.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2019 12:27
Operator : DD\AJ
Sample : K3192-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 13:52:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

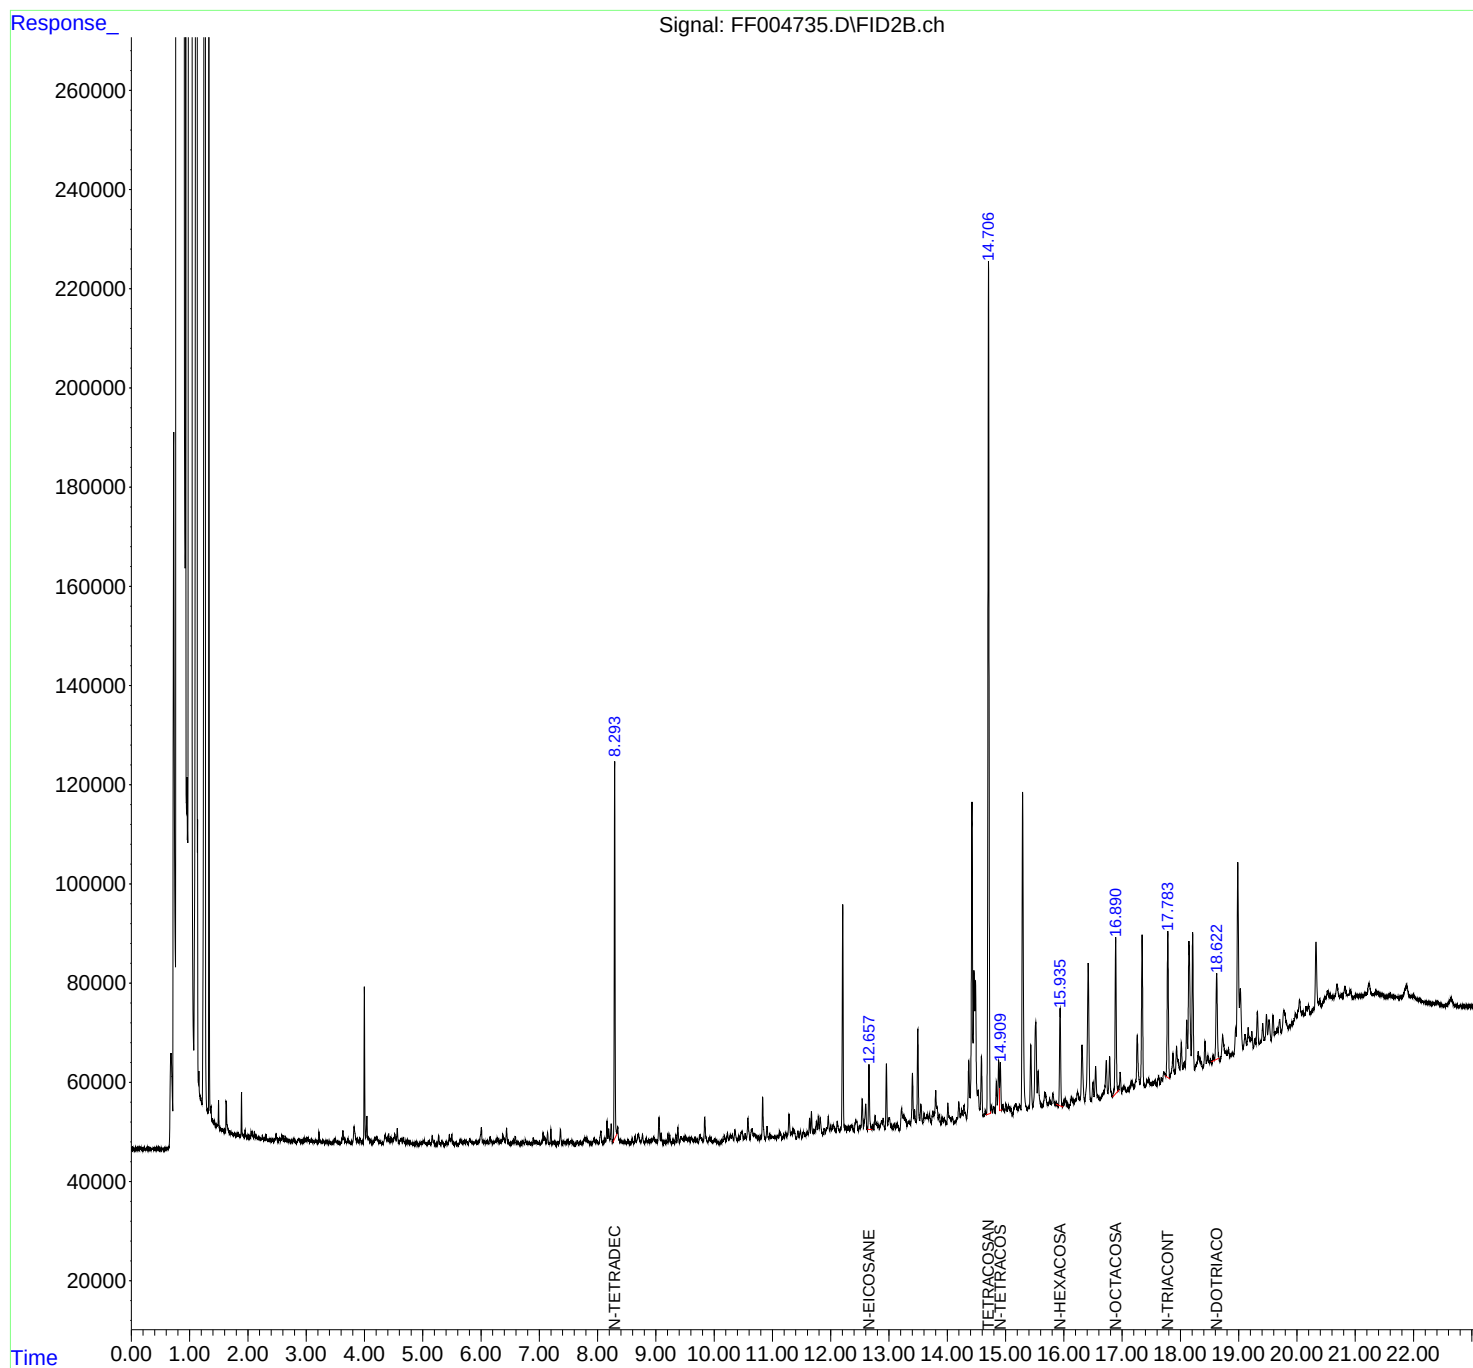


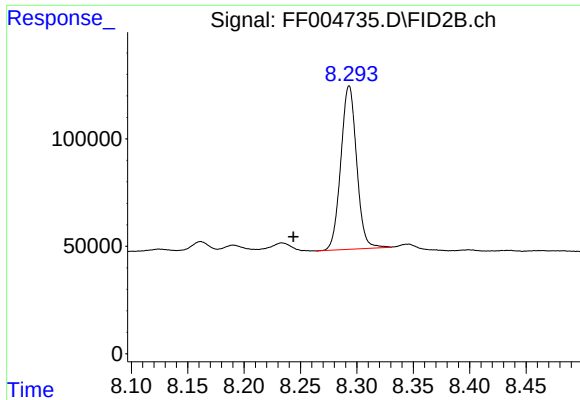

#4 N-TETRADECANE


R.T.: 8.293 min
Delta R.T.: 0.049 min
Response: 740349
Conc: 5.04 ug/ml

Instrument :
FID_F
ClientSampleId :

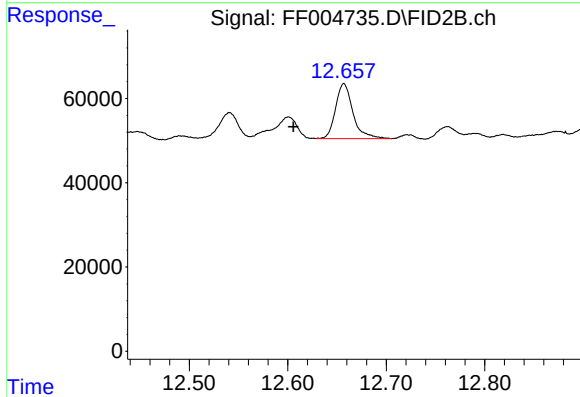


#7 N-EICOSANE

R.T.: 12.657 min
Delta R.T.: 0.051 min
Response: 159861
Conc: 1.10 ug/ml

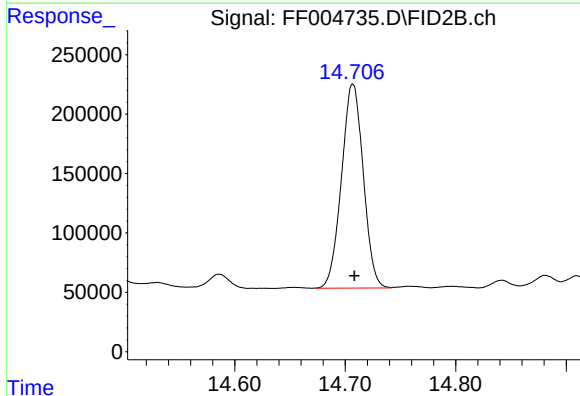


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.707 min
Delta R.T.: -0.001 min
Response: 2351687
Conc: 19.26 ug/ml

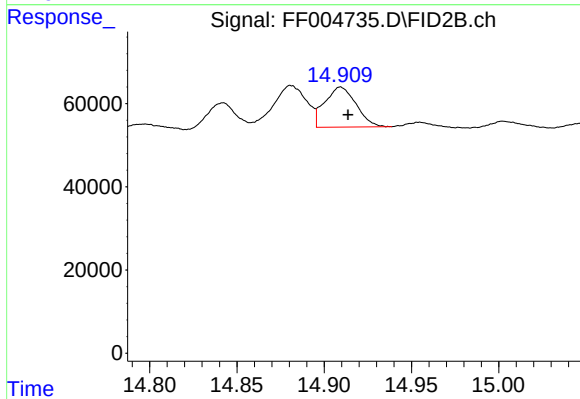

#10 N-TETRACOSANE


R.T.: 14.909 min
Delta R.T.: -0.004 min
Response: 120158
Conc: 0.87 ug/ml

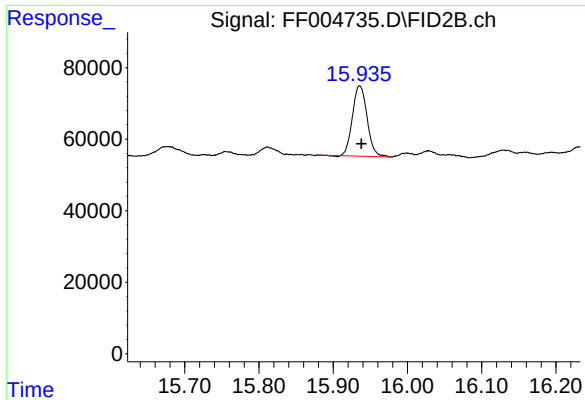

#11 N-HEXACOSANE


R.T.: 15.936 min
Delta R.T.: -0.002 min
Response: 268646
Conc: 1.97 ug/ml

Instrument :
FID_F
ClientSampleId :

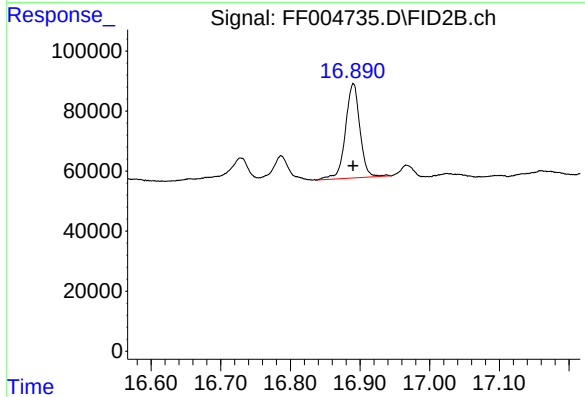


#12 N-OCTACOSANE

R.T.: 16.890 min
Delta R.T.: 0.000 min
Response: 452370
Conc: 3.33 ug/ml

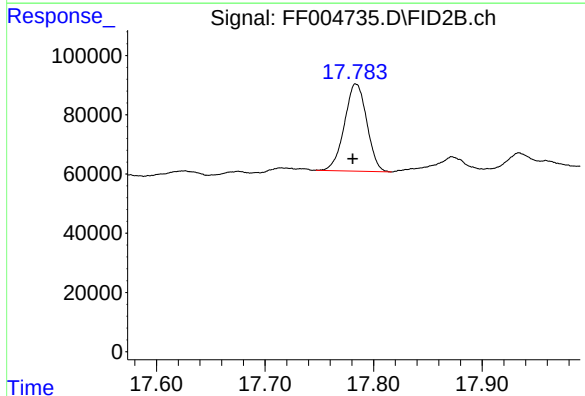

#13 N-TRIACONTANE

R.T.: 17.784 min
Delta R.T.: 0.003 min
Response: 421010
Conc: 3.04 ug/ml

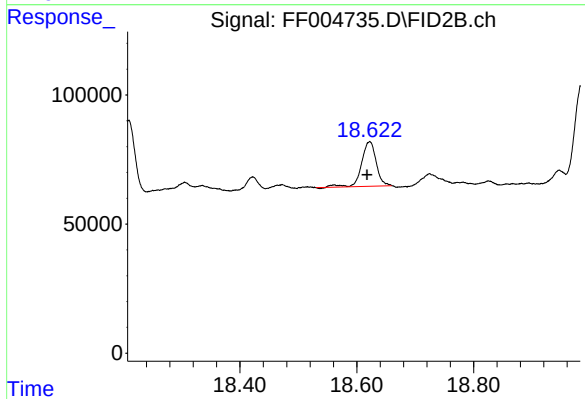

#14 N-DOTRIACONTANE

R.T.: 18.622 min
Delta R.T.: 0.005 min
Response: 301557
Conc: 2.18 ug/ml