

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
 Data File : FF004739.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jun 2019 14:24
 Operator : DD\AJ
 Sample : PB120408BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 21:40:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.706	2179459	17.848 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.632	174357	1.260 ug/ml
16) N-HEXATRIACONTANE	20.201f	364349	2.768 ug/ml
18) N-TETRACONTANE	21.884	468410	3.804 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
Data File : FF004739.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2019 14:24
Operator : DD\AJ
Sample : PB120408BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 21:40:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

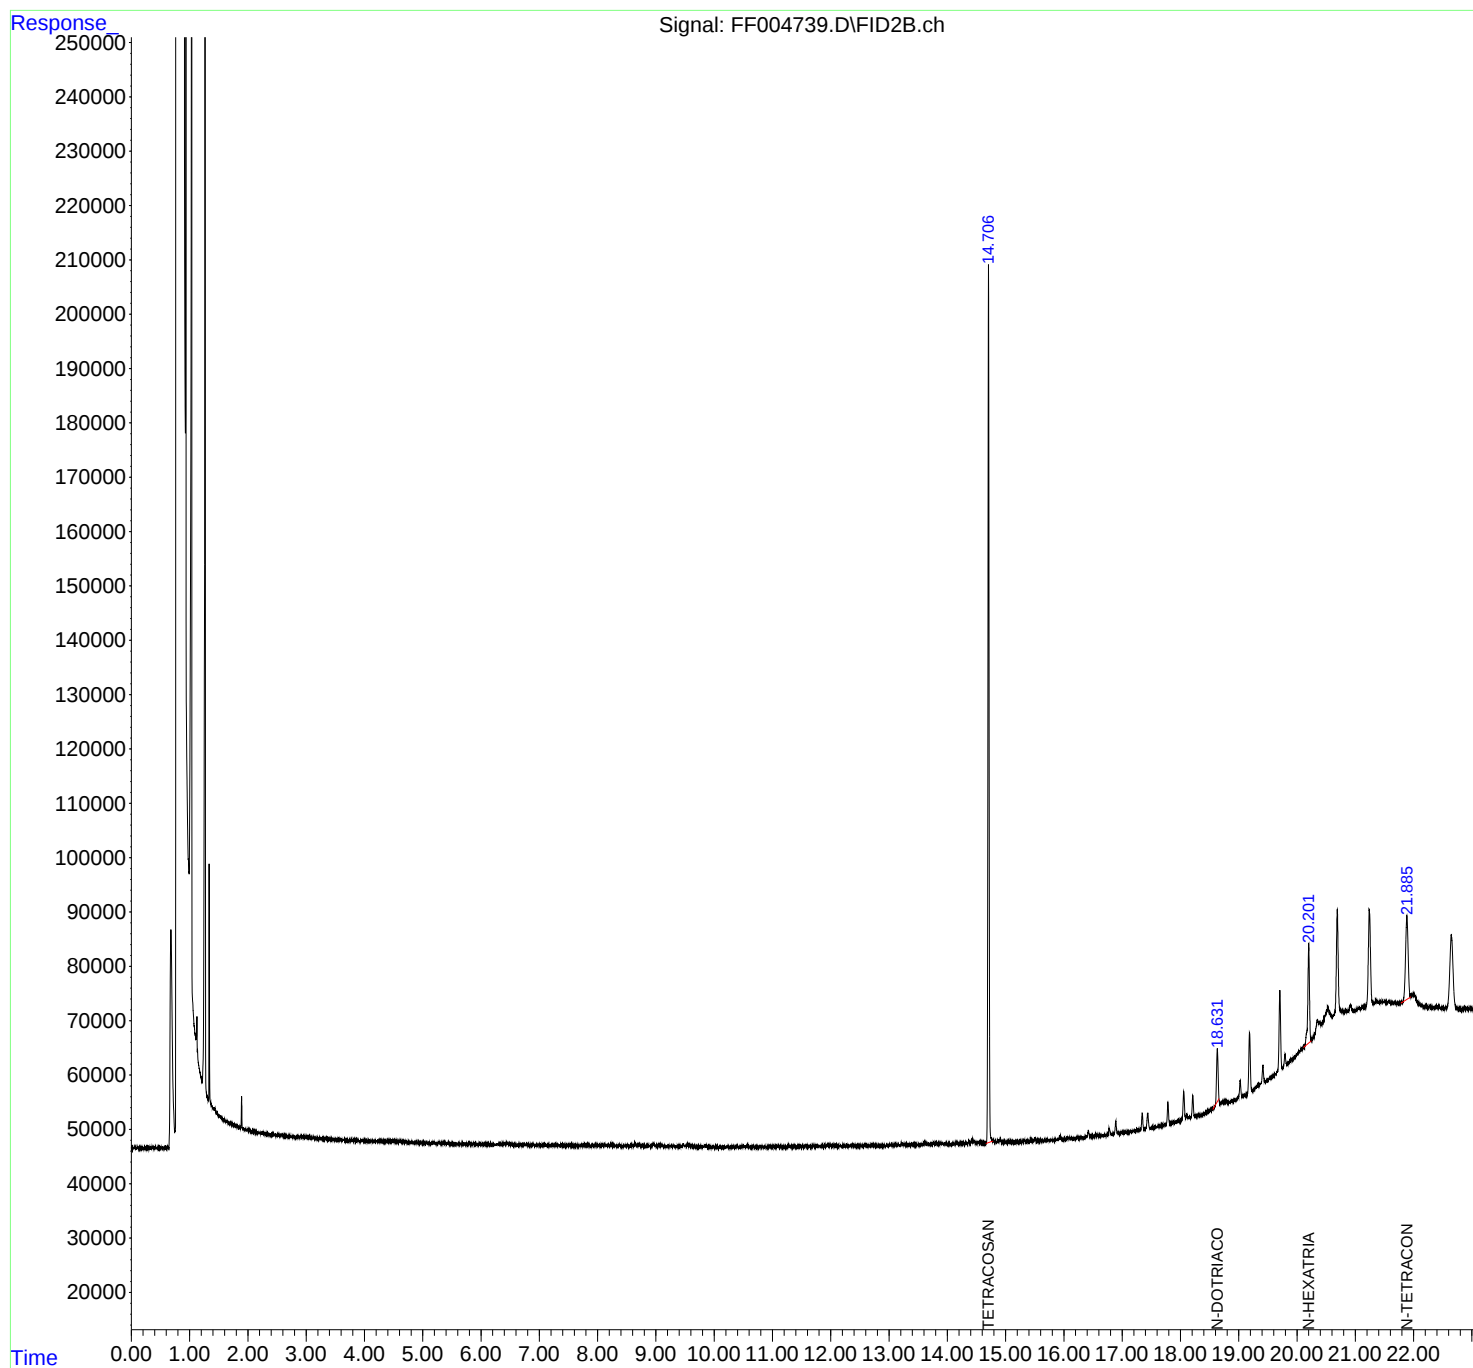


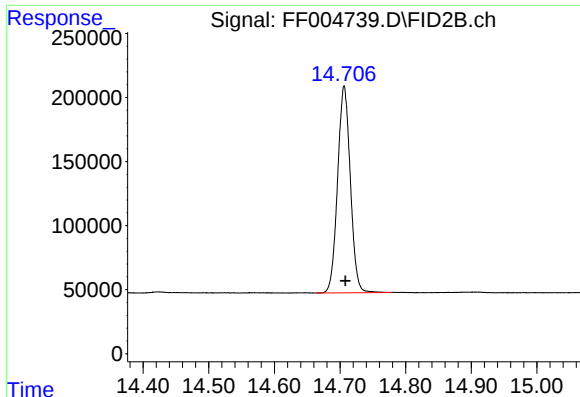

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.706 min
Delta R.T.: -0.002 min
Response: 2179459
Conc: 17.85 ug/ml

Instrument :
FID_F
ClientSampleId :

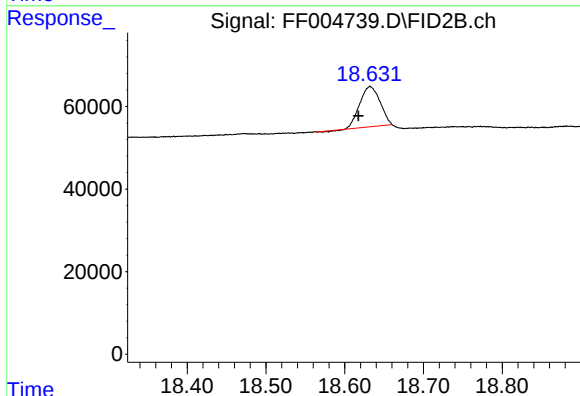


#14 N-DOTRIACONTANE

R.T.: 18.632 min
Delta R.T.: 0.015 min
Response: 174357
Conc: 1.26 ug/ml

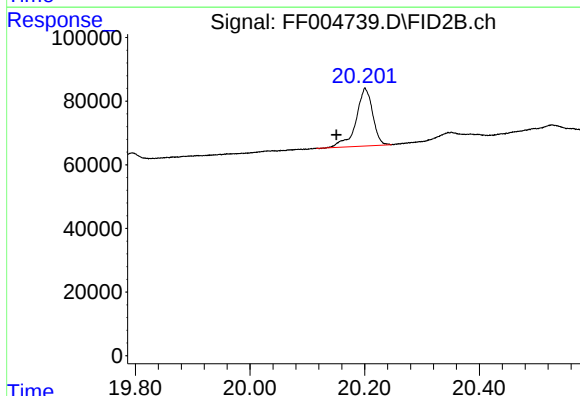

#16 N-HEXATRIACONTANE

R.T.: 20.201 min
Delta R.T.: 0.050 min
Response: 364349
Conc: 2.77 ug/ml

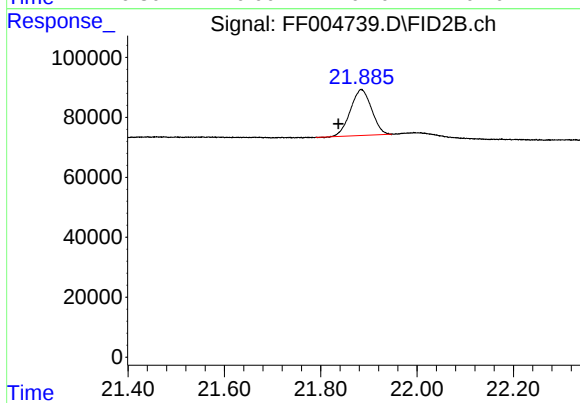

#18 N-TETRACONTANE

R.T.: 21.884 min
Delta R.T.: 0.047 min
Response: 468410
Conc: 3.80 ug/ml