

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
Data File : FF004742.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2019 15:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 21:40:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.706	2024772	16.581 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.783	136960	0.990 ug/ml
14) N-DOTRIACONTANE	18.624	171710	1.241 ug/ml
15) N-TETRATRIACONTANE	19.414	114720	0.839 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
Data File : FF004742.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2019 15:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 21:40:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

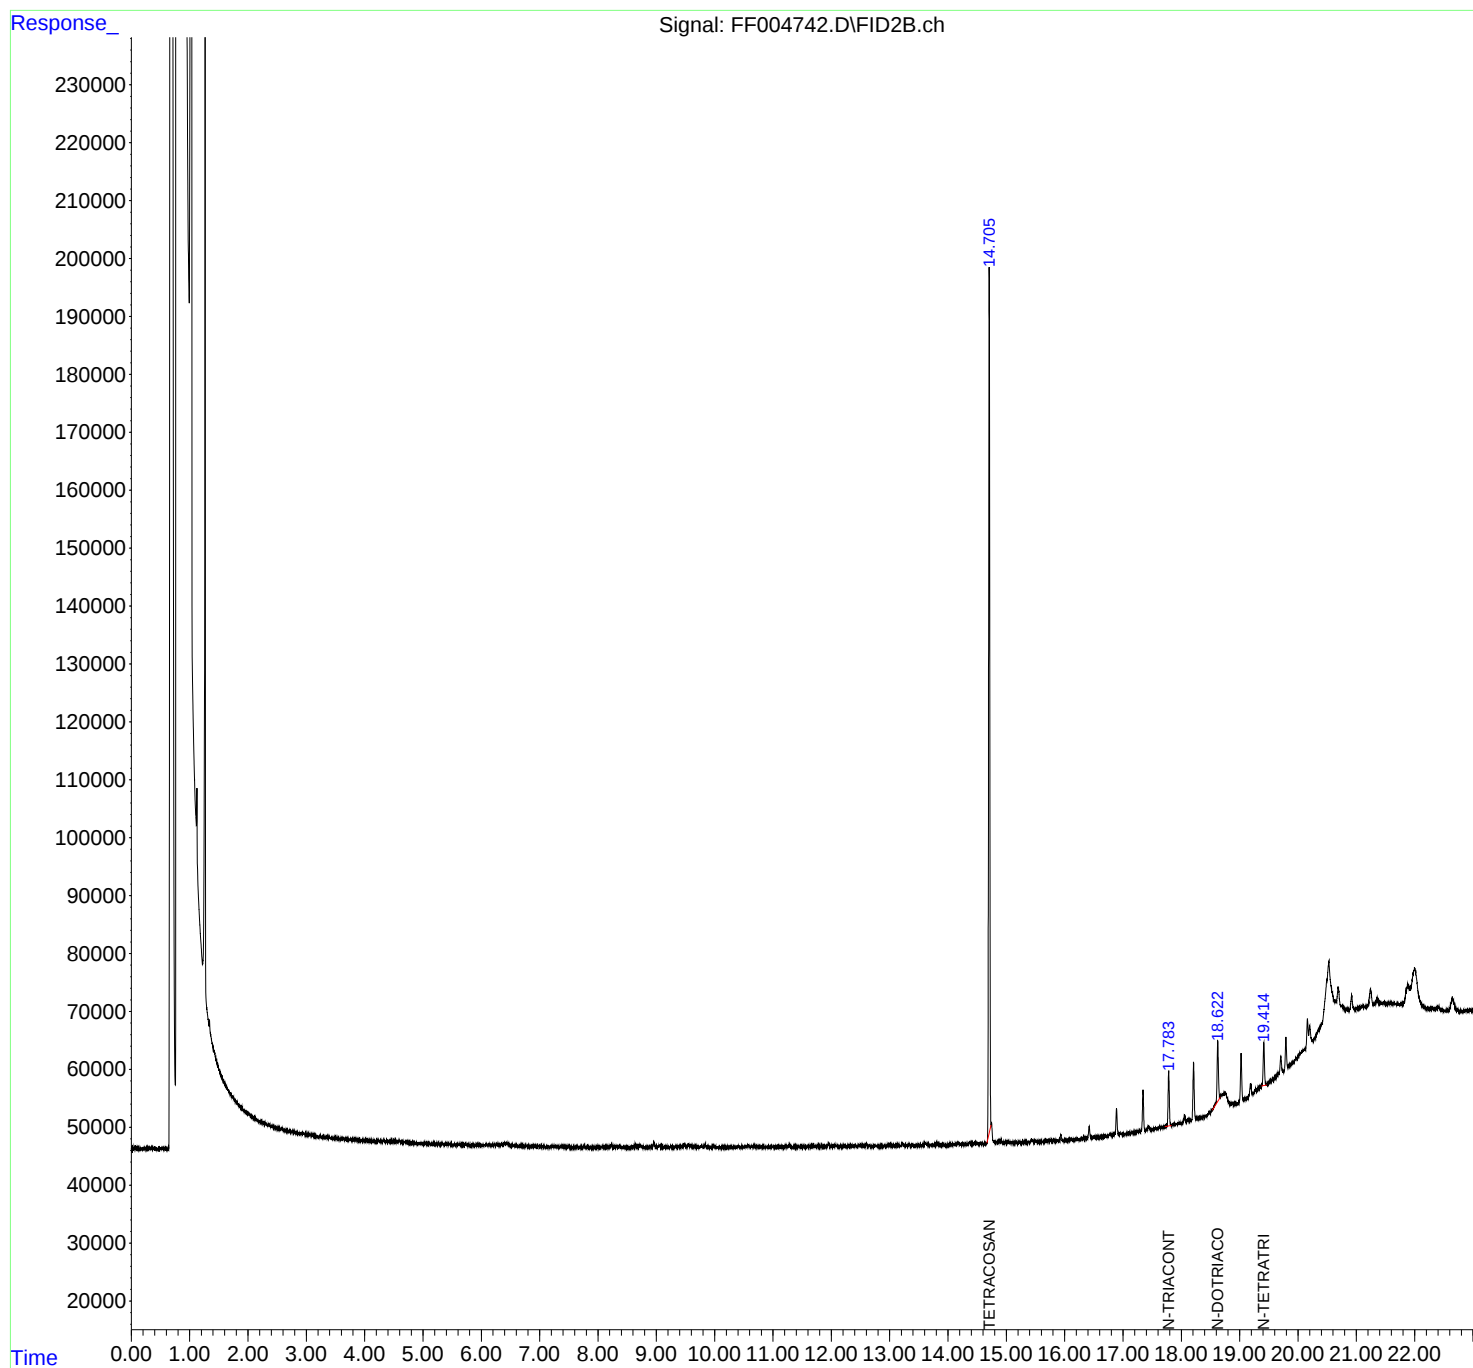


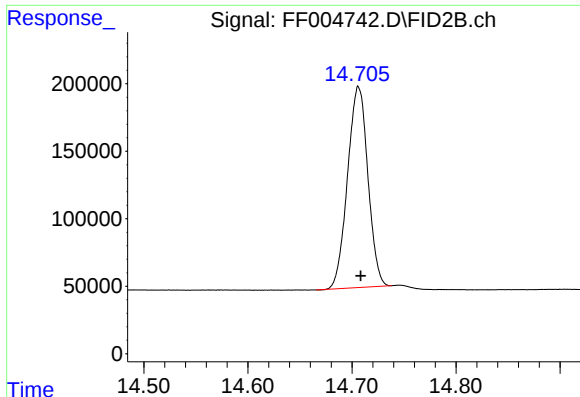

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.706 min
Delta R.T.: -0.002 min
Response: 2024772
Conc: 16.58 ug/ml

Instrument :
FID_F
ClientSampleId :

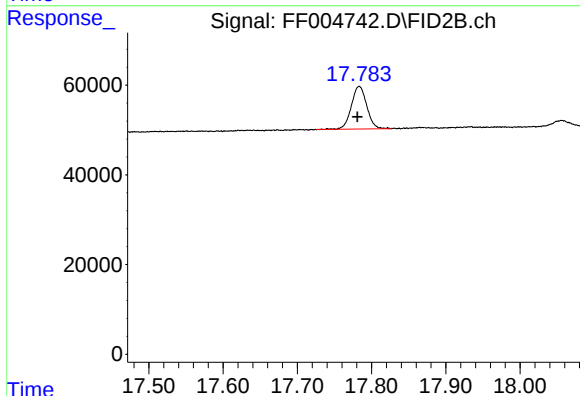


#13 N-TRIACONTANE

R.T.: 17.783 min
Delta R.T.: 0.002 min
Response: 136960
Conc: 0.99 ug/ml

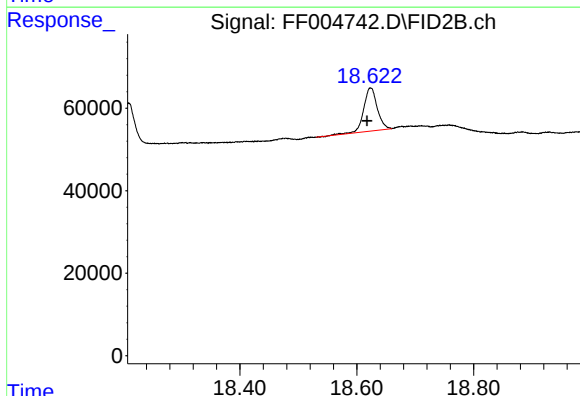

#14 N-DOTRIACONTANE

R.T.: 18.624 min
Delta R.T.: 0.006 min
Response: 171710
Conc: 1.24 ug/ml

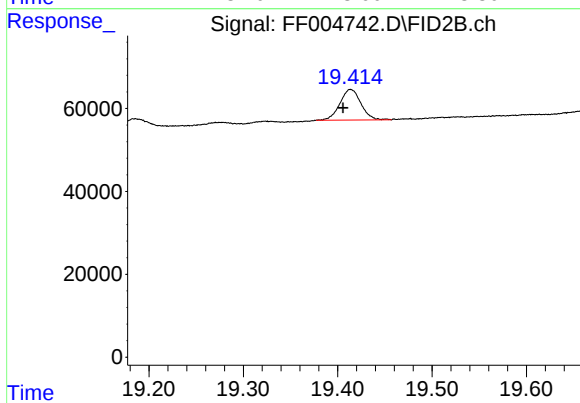

#15 N-TETRATRIACONTANE

R.T.: 19.414 min
Delta R.T.: 0.008 min
Response: 114720
Conc: 0.84 ug/ml