

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
Data File : FF004745.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2019 17:22
Operator : DD\AJ
Sample : PB120407BL
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 21:41:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.706	2101576	17.210 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.632	199188	1.440 ug/ml
16) N-HEXATRIACONTANE	20.200	433296	3.291 ug/ml
18) N-TETRACONTANE	21.883	584487	4.746 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
Data File : FF004745.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2019 17:22
Operator : DD\AJ
Sample : PB120407BL
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 21:41:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

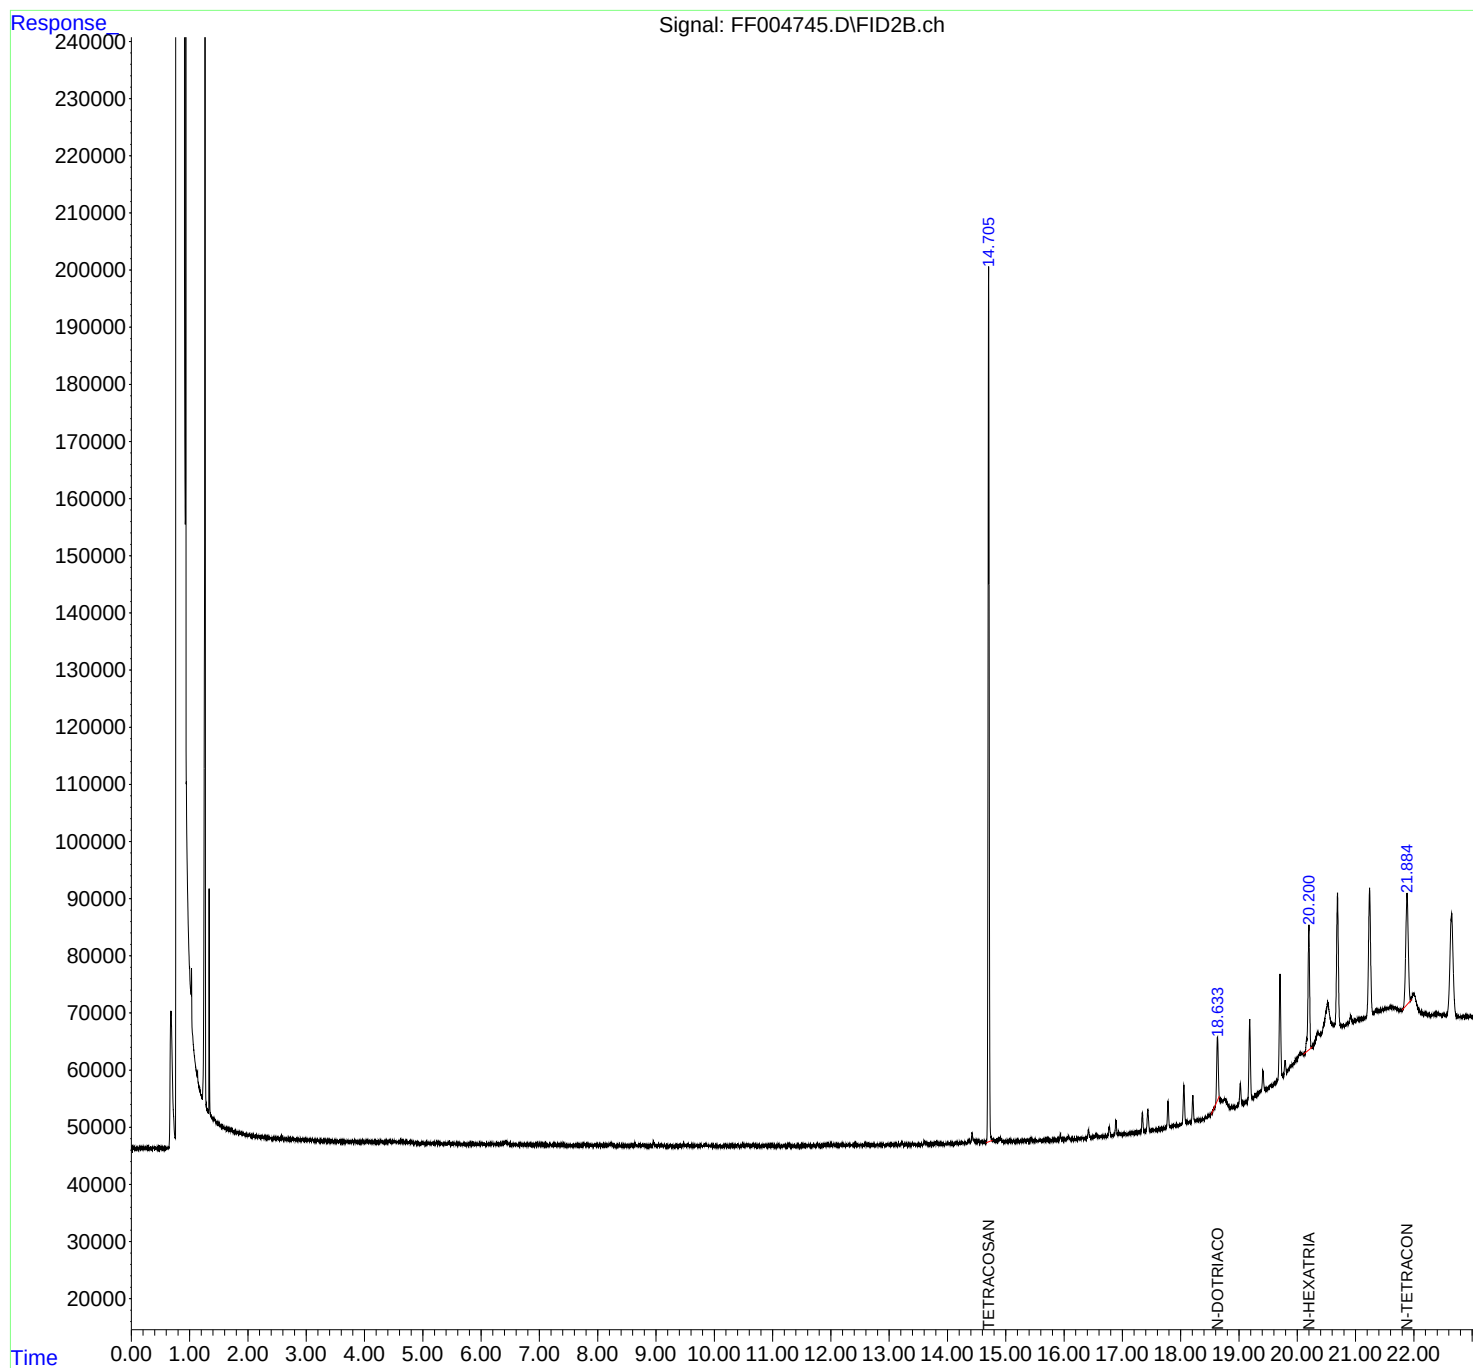


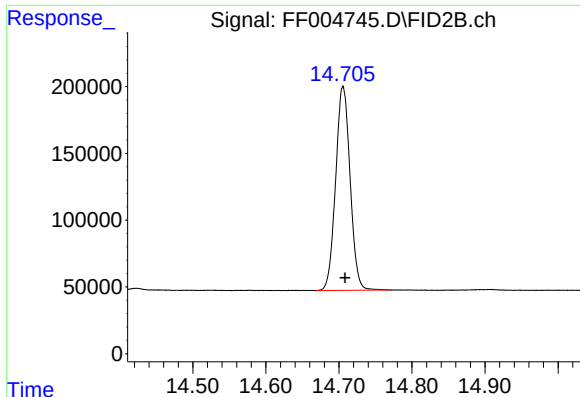

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.706 min
Delta R.T.: -0.003 min
Response: 2101576
Conc: 17.21 ug/ml

Instrument :
FID_F
ClientSampleId :

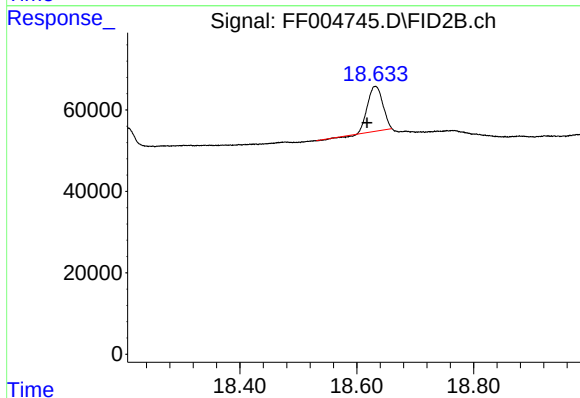


#14 N-DOTRIACONTANE

R.T.: 18.632 min
Delta R.T.: 0.014 min
Response: 199188
Conc: 1.44 ug/ml

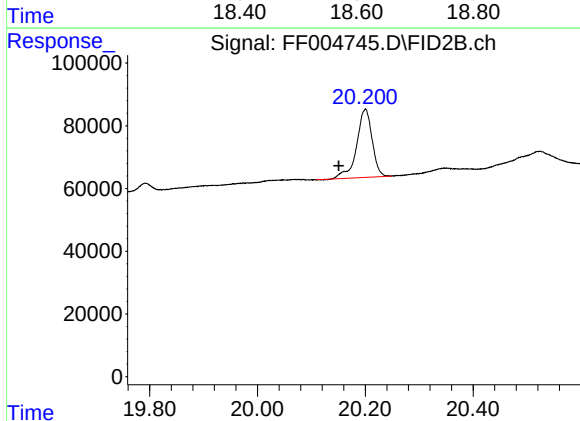

#16 N-HEXATRIACONTANE

R.T.: 20.200 min
Delta R.T.: 0.050 min
Response: 433296
Conc: 3.29 ug/ml

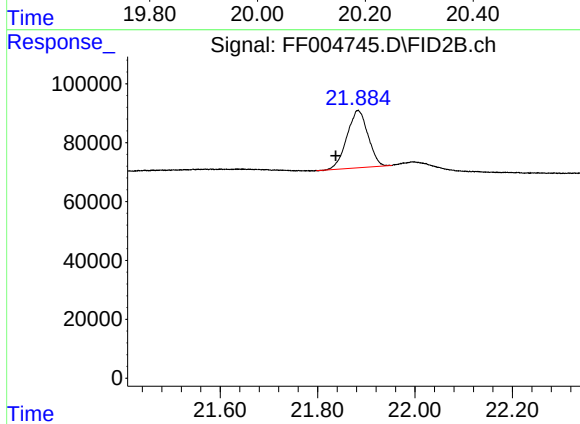

#18 N-TETRACONTANE

R.T.: 21.883 min
Delta R.T.: 0.046 min
Response: 584487
Conc: 4.75 ug/ml