

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
 Data File : FF004748.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jun 2019 18:51
 Operator : DD\AJ
 Sample : K3158-01 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 21:42:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.707	206829	1.694 ug/ml
Target Compounds			
7) N-EICOSANE	12.659f	947226	6.540 ug/ml
8) N-DOCOSANE	13.805	114752	0.812 ug/ml
10) N-TETRACOSANE	14.885	399430	2.882 ug/ml
11) N-HEXACOSANE	15.938	166355	1.221 ug/ml
12) N-OCTACOSANE	16.891	349865	2.573 ug/ml
13) N-TRIACONTANE	17.786	421800	3.050 ug/ml
14) N-DOTRIACONTANE	18.623	278795	2.015 ug/ml
15) N-TETRATRIACONTANE	19.417	127910	0.936 ug/ml
16) N-HEXATRIACONTANE	20.170	300841	2.285 ug/ml
17) N-OCTATRIACONTANE	20.919	631135	5.248 ug/ml
18) N-TETRACONTANE	21.889f	356784	2.897 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
Data File : FF004748.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2019 18:51
Operator : DD\AJ
Sample : K3158-01 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 07 21:42:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

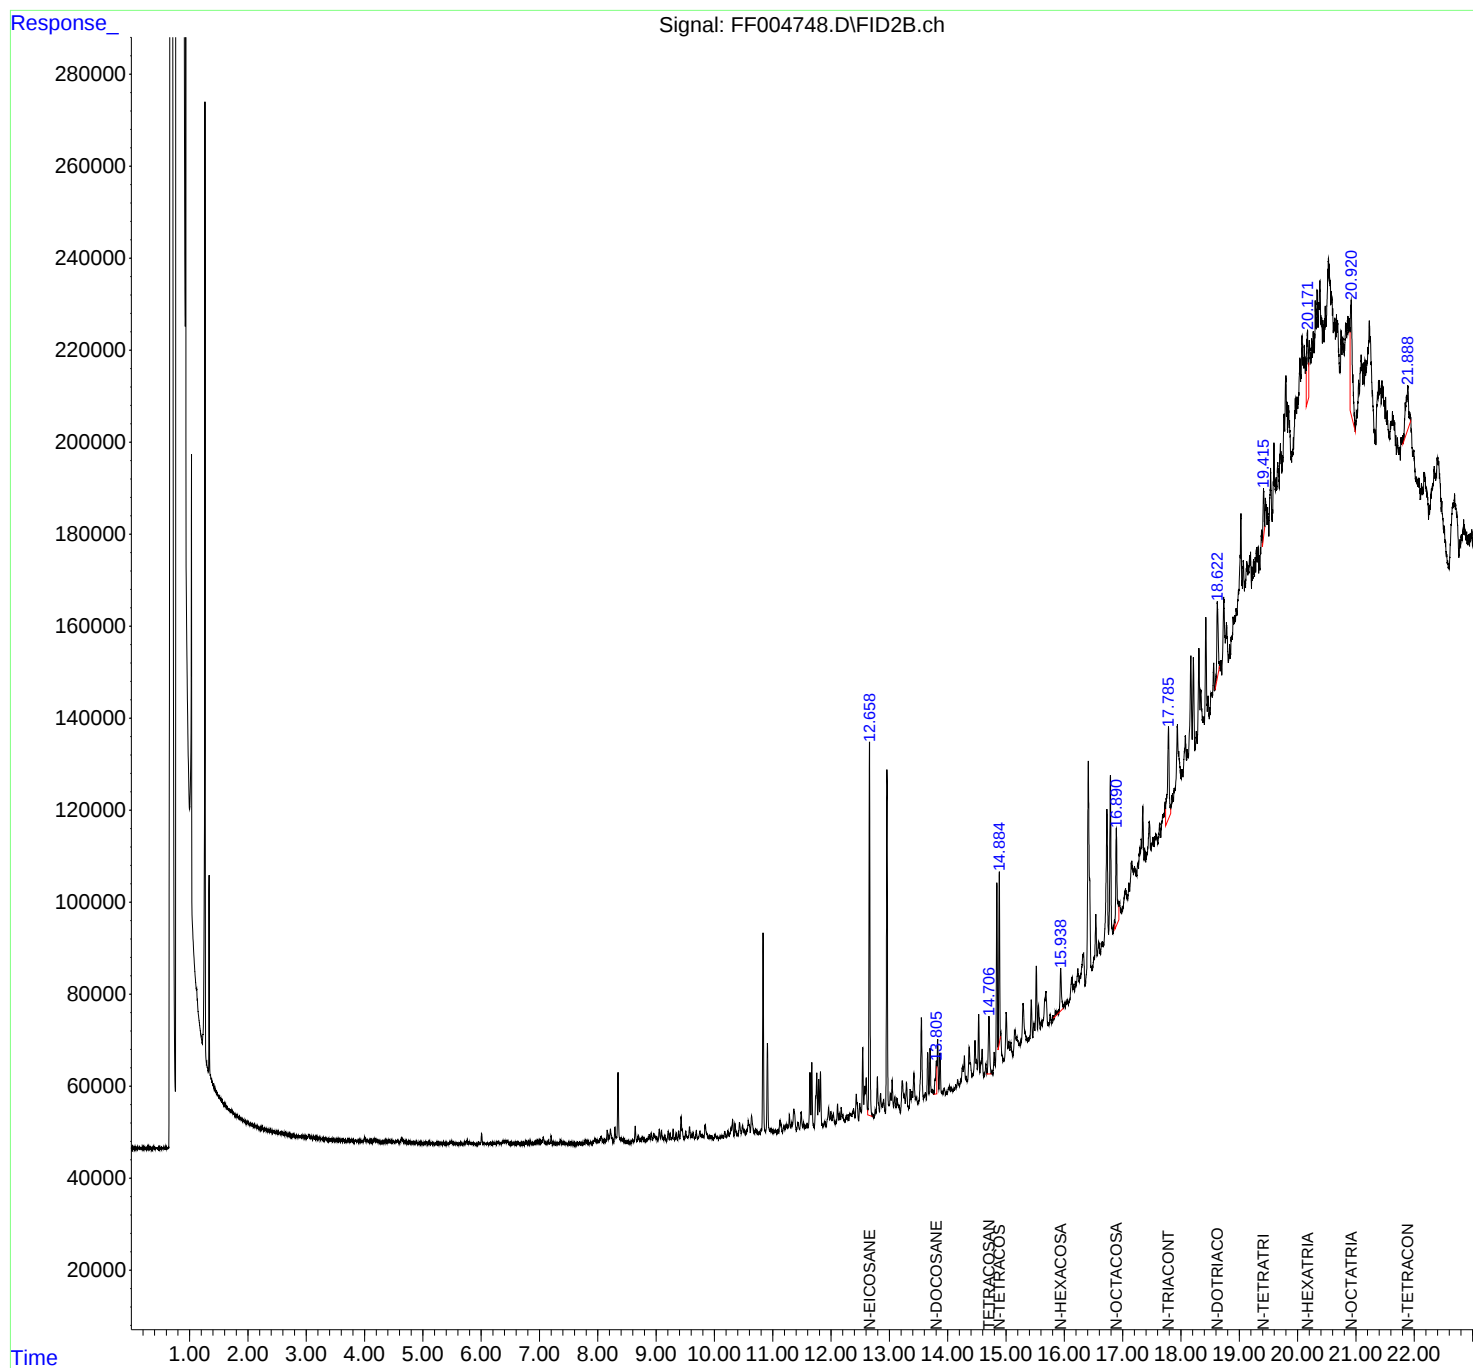


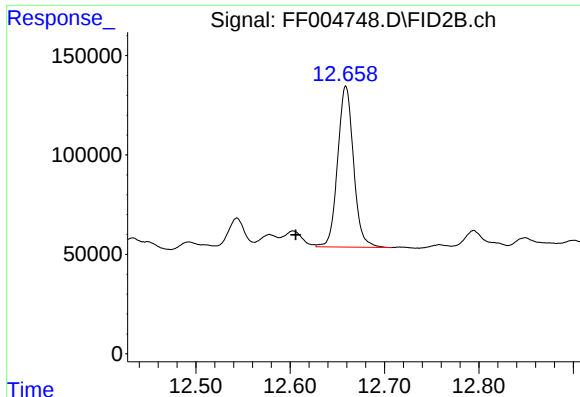

#7 N-EICOSANE


R.T.: 12.659 min
Delta R.T.: 0.053 min
Response: 947226
Conc: 6.54 ug/ml

Instrument :
FID_F
ClientSampleId :

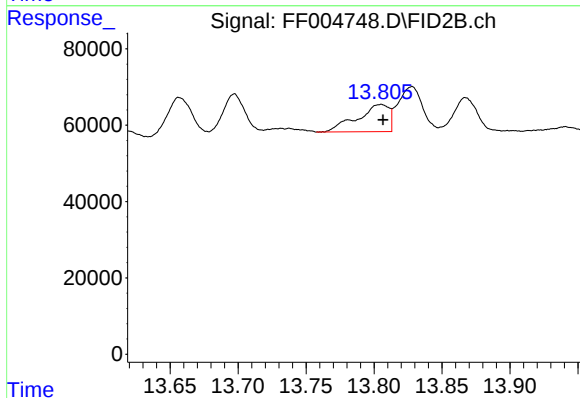


#8 N-DOCOSANE

R.T.: 13.805 min
Delta R.T.: -0.002 min
Response: 114752
Conc: 0.81 ug/ml

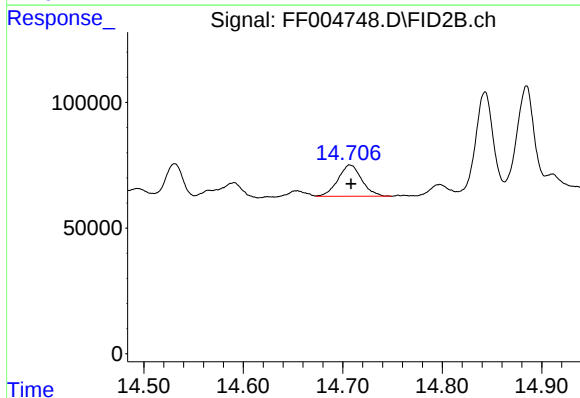


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.707 min
Delta R.T.: -0.001 min
Response: 206829
Conc: 1.69 ug/ml

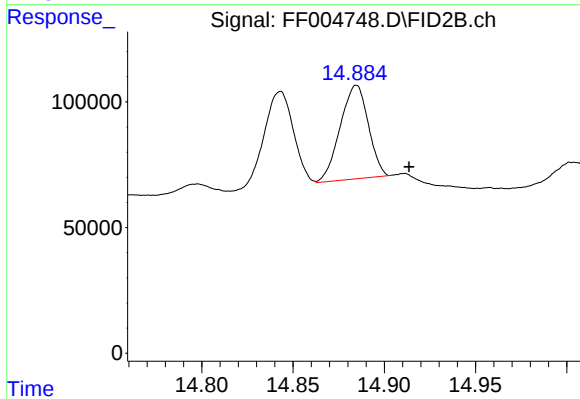

#10 N-TETRACOSANE


R.T.: 14.885 min
Delta R.T.: -0.029 min
Response: 399430
Conc: 2.88 ug/ml

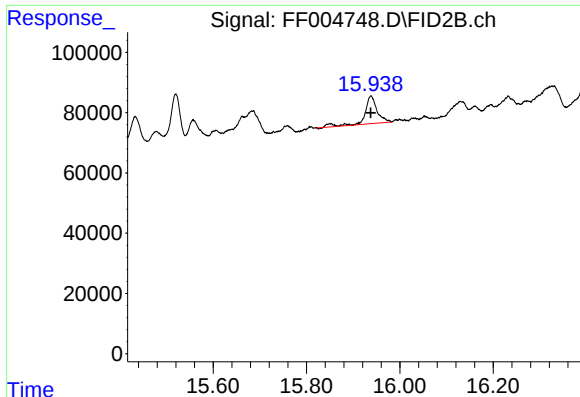

#11 N-HEXACOSANE


R.T.: 15.938 min
Delta R.T.: 0.000 min
Response: 166355
Conc: 1.22 ug/ml

Instrument :
FID_F
ClientSampleId :

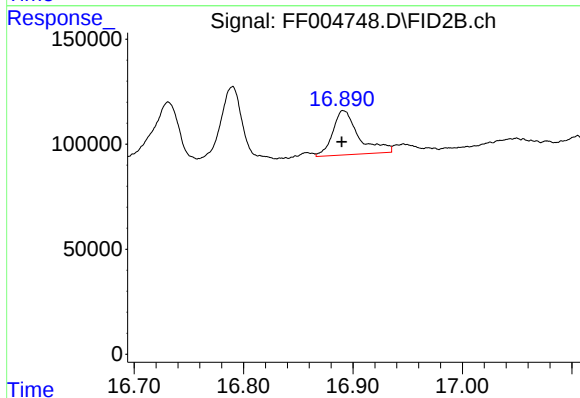


#12 N-OCTACOSANE

R.T.: 16.891 min
Delta R.T.: 0.002 min
Response: 349865
Conc: 2.57 ug/ml

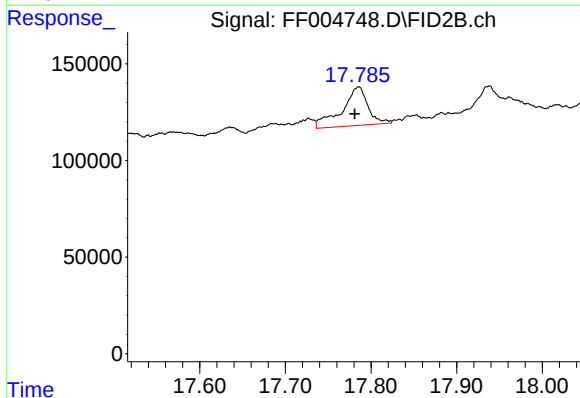


#13 N-TRIACONTANE

R.T.: 17.786 min
Delta R.T.: 0.005 min
Response: 421800
Conc: 3.05 ug/ml

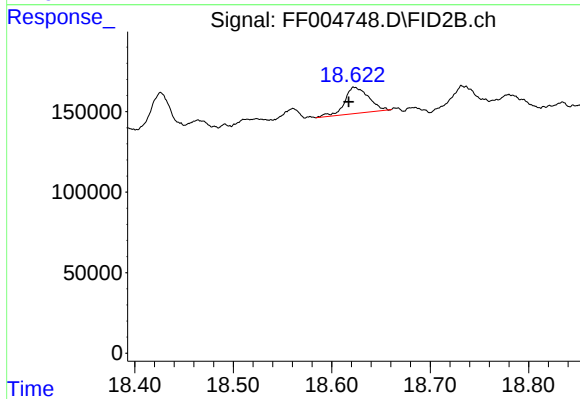

#14 N-DOTRIACONTANE


R.T.: 18.623 min
Delta R.T.: 0.006 min
Response: 278795
Conc: 2.02 ug/ml

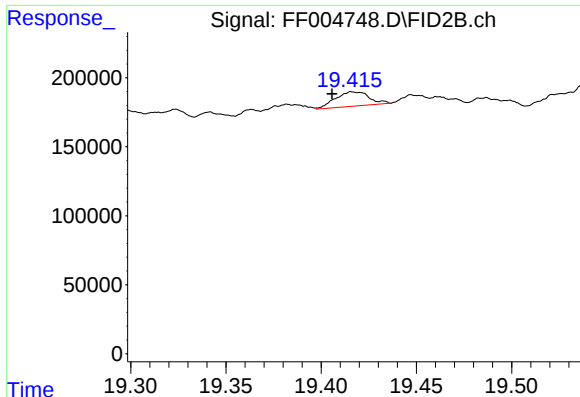

#15 N-TETRATRIACONTANE


R.T.: 19.417 min
Delta R.T.: 0.011 min
Response: 127910
Conc: 0.94 ug/ml

Instrument :
FID_F
ClientSampleId :

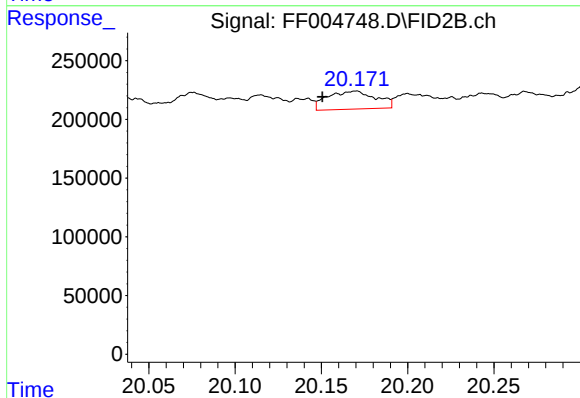


#16 N-HEXATRIACONTANE

R.T.: 20.170 min
Delta R.T.: 0.020 min
Response: 300841
Conc: 2.29 ug/ml

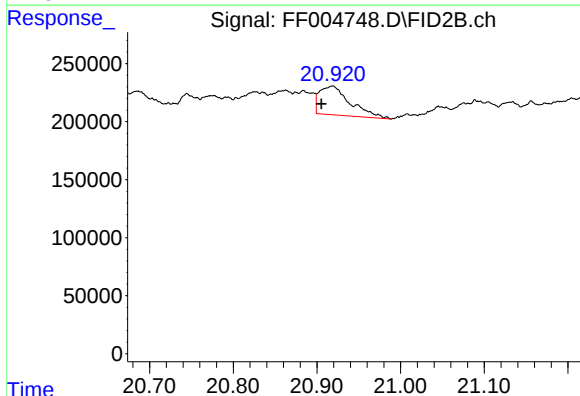

#17 N-OCTATRIACONTANE

R.T.: 20.919 min
Delta R.T.: 0.013 min
Response: 631135
Conc: 5.25 ug/ml

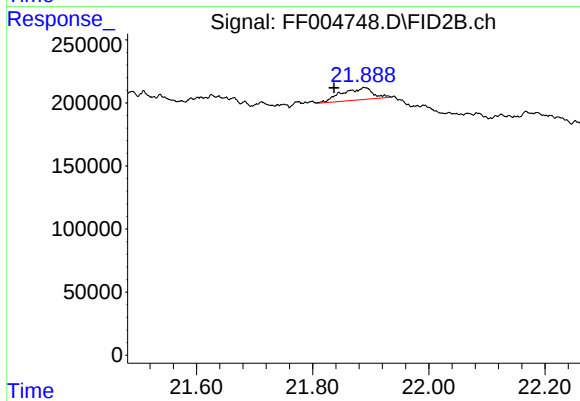

#18 N-TETRACONTANE

R.T.: 21.889 min
Delta R.T.: 0.052 min
Response: 356784
Conc: 2.90 ug/ml