

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
 Data File : FF004749.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jun 2019 19:21
 Operator : DD\AJ
 Sample : K3160-01 10X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 21:42:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.707	161078	1.319 ug/ml
Target Compounds			
7) N-EICOSANE	12.658f	89516	0.618 ug/ml
12) N-OCTACOSANE	16.892	109133	0.803 ug/ml
13) N-TRIACONTANE	17.786	358987	2.596 ug/ml
14) N-DOTRIACONTANE	18.626	339298	2.453 ug/ml
15) N-TETRATRIACONTANE	19.411	150368	1.100 ug/ml
16) N-HEXATRIACONTANE	20.159	293881	2.232 ug/ml
18) N-TETRACONTANE	21.880	290607	2.360 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
Data File : FF004749.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2019 19:21
Operator : DD\AJ
Sample : K3160-01 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 07 21:42:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

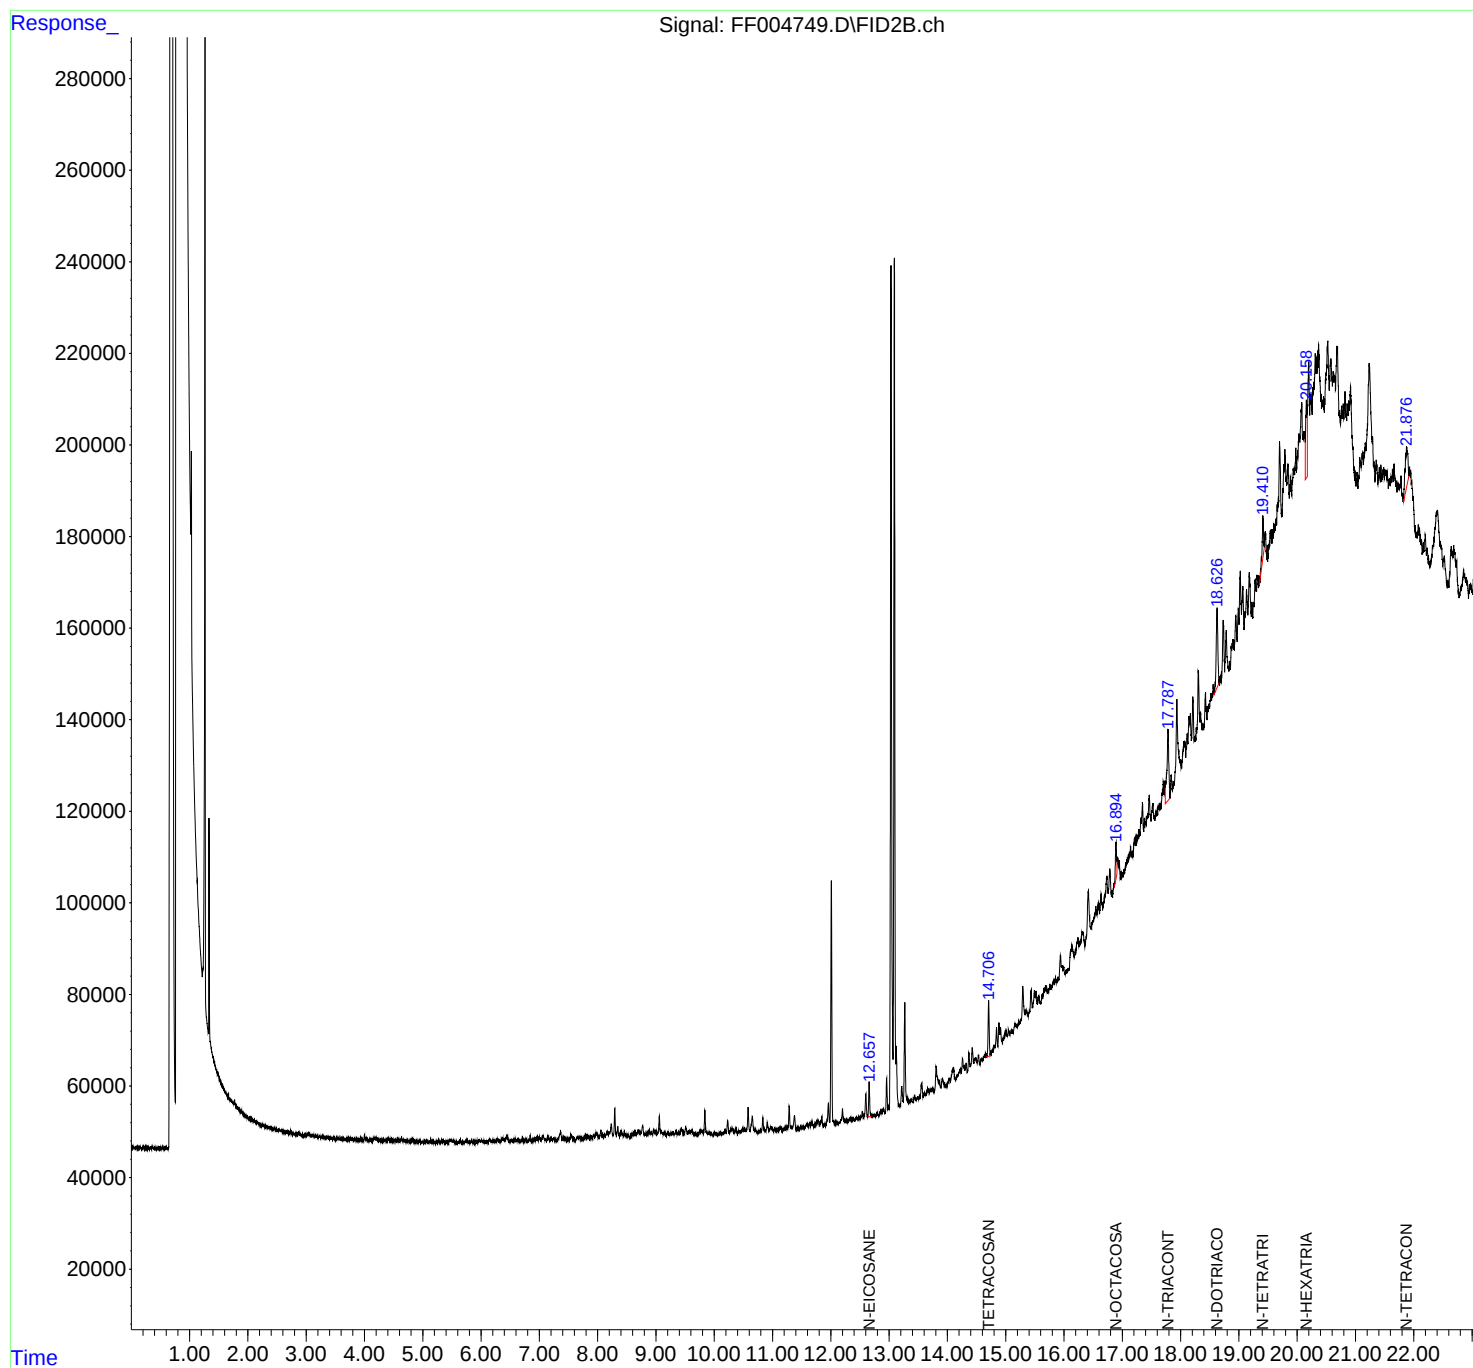


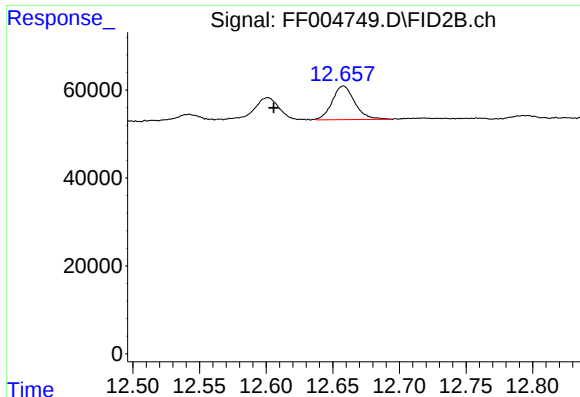

#7 N-EICOSANE


R.T.: 12.658 min
Delta R.T.: 0.052 min
Response: 89516
Conc: 0.62 ug/ml

Instrument :
FID_F
ClientSampleId :

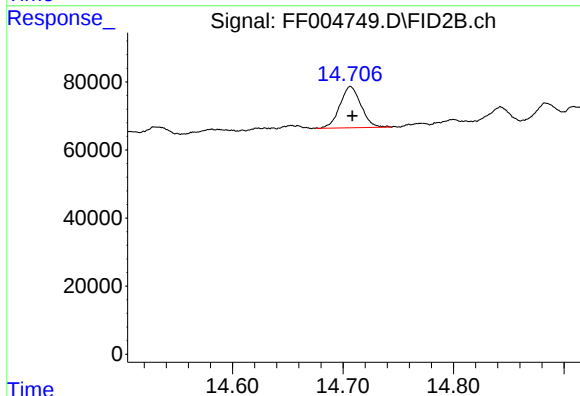


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.707 min
Delta R.T.: -0.002 min
Response: 161078
Conc: 1.32 ug/ml

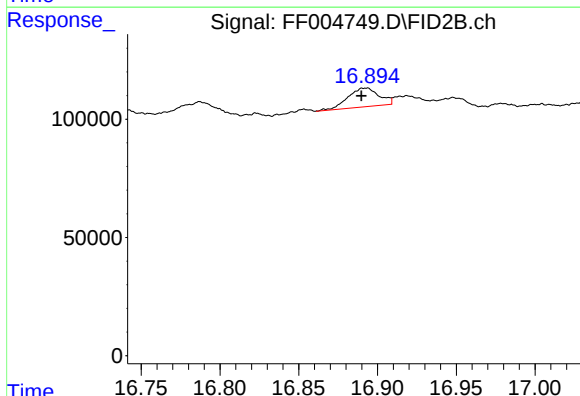


#12 N-OCTACOSANE

R.T.: 16.892 min
Delta R.T.: 0.003 min
Response: 109133
Conc: 0.80 ug/ml

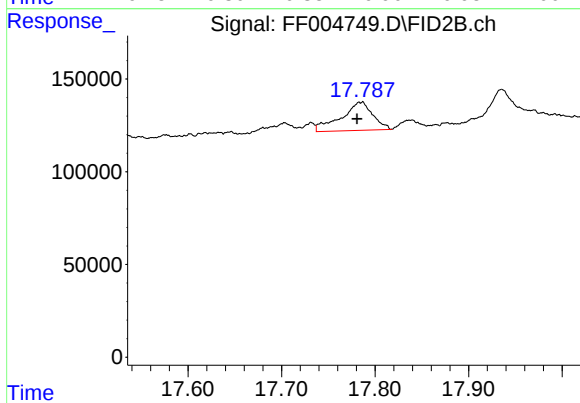

#13 N-TRIACONTANE


R.T.: 17.786 min
Delta R.T.: 0.005 min
Response: 358987
Conc: 2.60 ug/ml

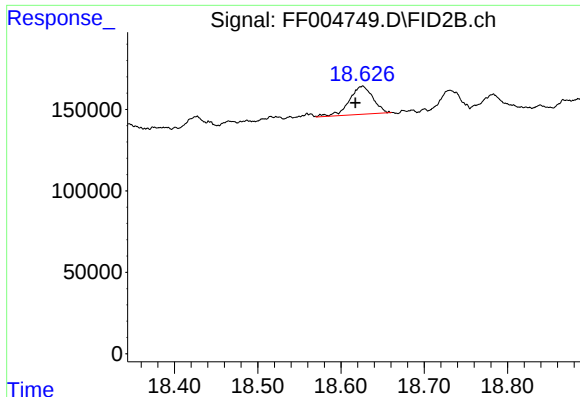

#14 N-DOTRIACONTANE


R.T.: 18.626 min
Delta R.T.: 0.008 min
Response: 339298
Conc: 2.45 ug/ml

Instrument :
FID_F
ClientSampleId :

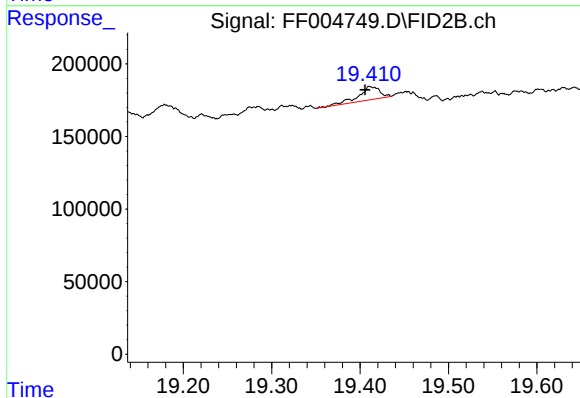


#15 N-TETRATRIACONTANE

R.T.: 19.411 min
Delta R.T.: 0.005 min
Response: 150368
Conc: 1.10 ug/ml

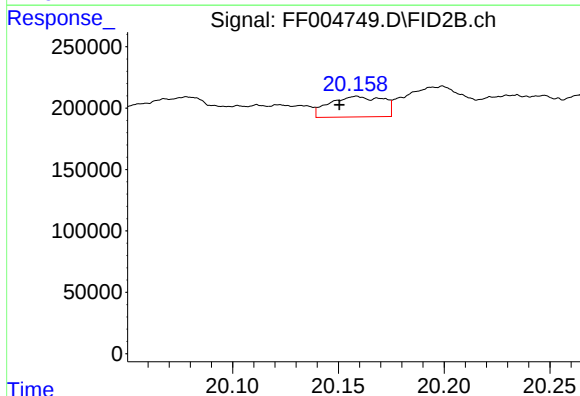

#16 N-HEXATRIACONTANE

R.T.: 20.159 min
Delta R.T.: 0.008 min
Response: 293881
Conc: 2.23 ug/ml

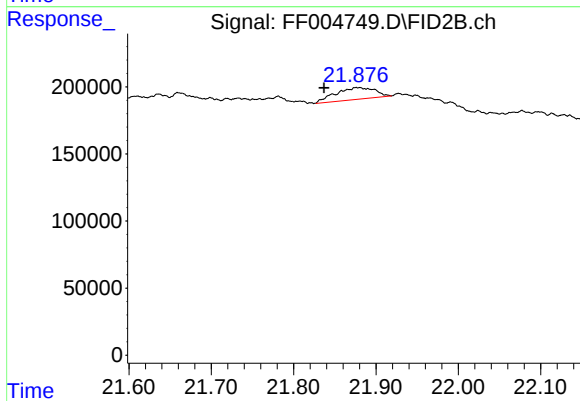

#18 N-TETRACONTANE

R.T.: 21.880 min
Delta R.T.: 0.043 min
Response: 290607
Conc: 2.36 ug/ml