

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
 Data File : FF004754.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jun 2019 21:49
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 23:09:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.709	2068157	16.937 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.893	82870	0.610 ug/ml
13) N-TRIACONTANE	17.783	178292	1.289 ug/ml
14) N-DOTRIACONTANE	18.621	248504	1.796 ug/ml
15) N-TETRATRIACONTANE	19.409	175181	1.281 ug/ml
16) N-HEXATRIACONTANE	20.153	137209	1.042 ug/ml
17) N-OCTATRIACONTANE	20.892	332828	2.768 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
Data File : FF004754.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2019 21:49
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 07 23:09:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

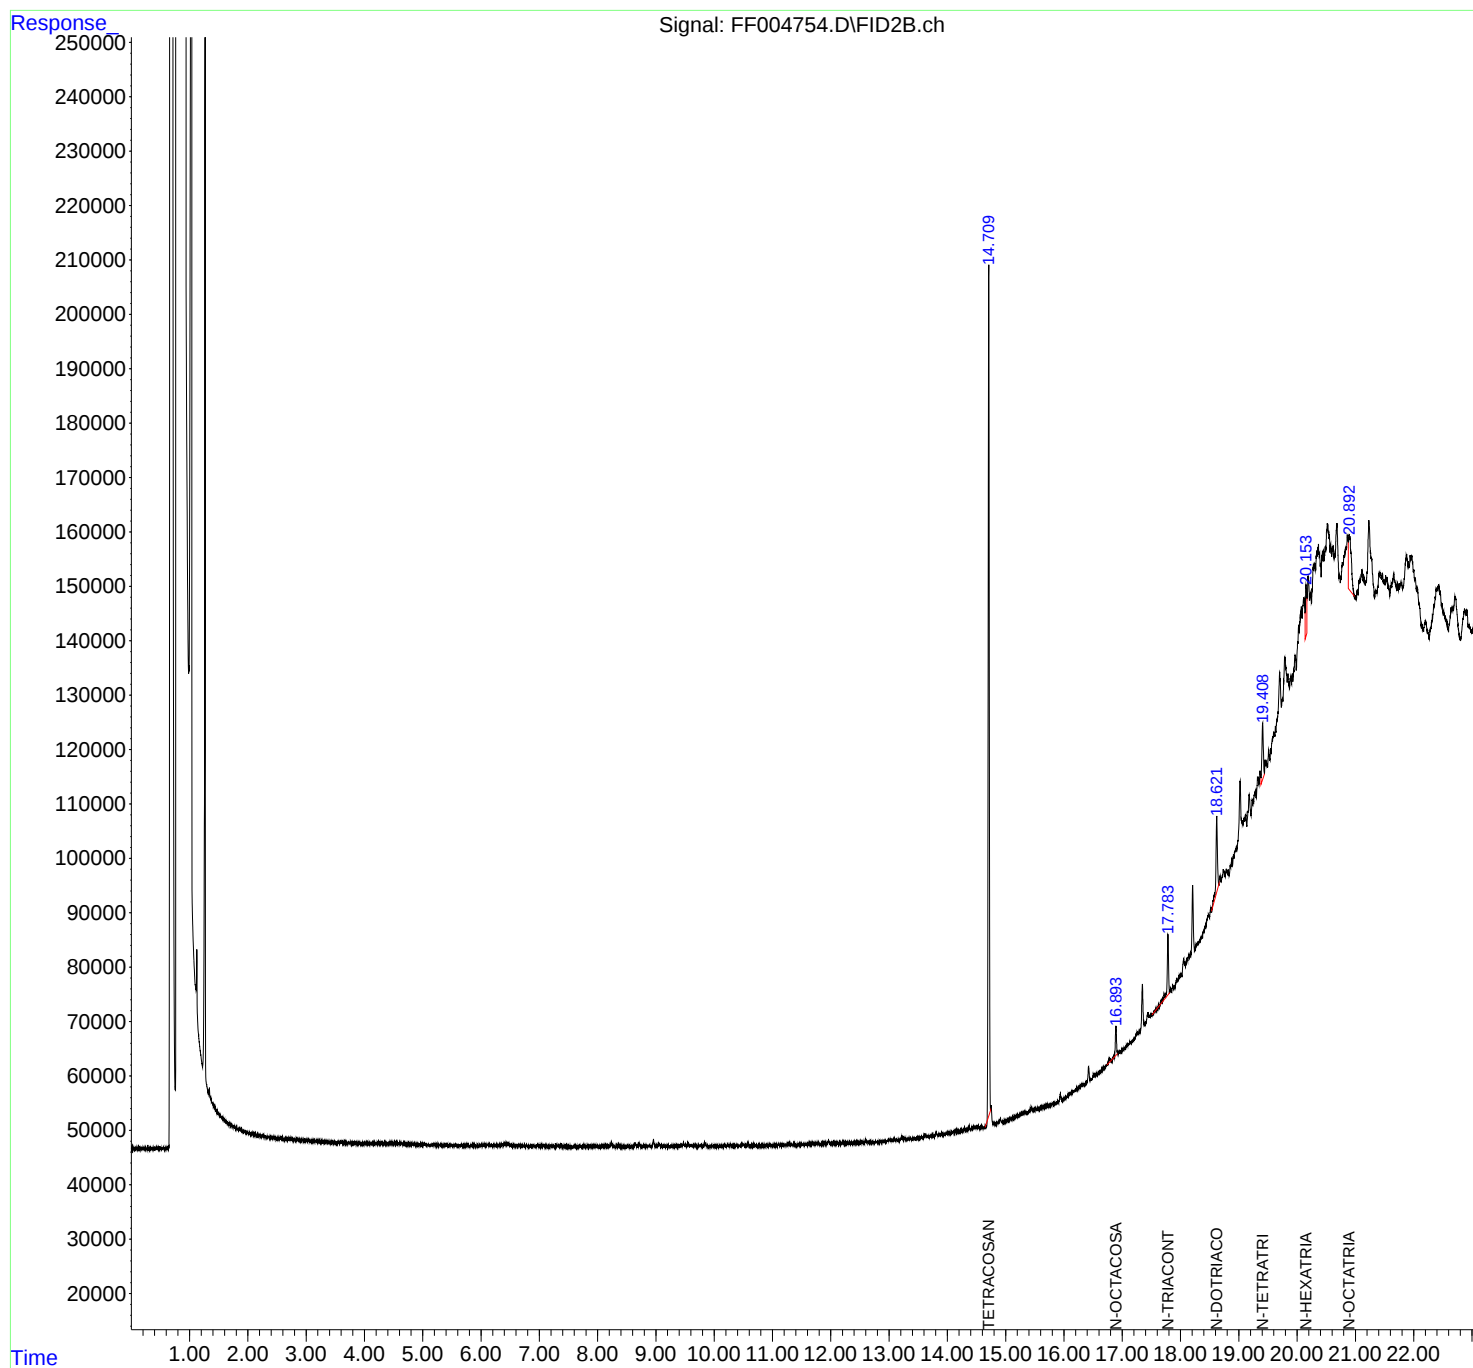


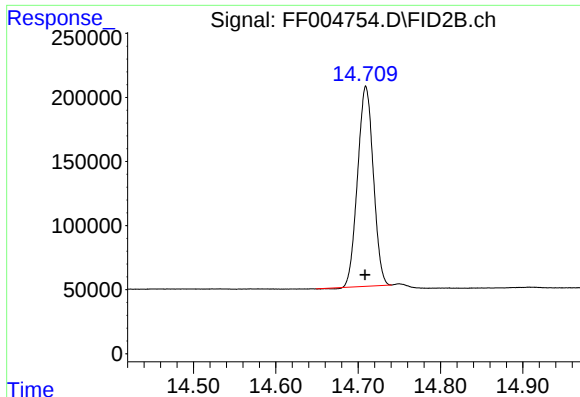

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.709 min
Delta R.T.: 0.001 min
Response: 2068157
Conc: 16.94 ug/ml

Instrument :
FID_F
ClientSampleId :

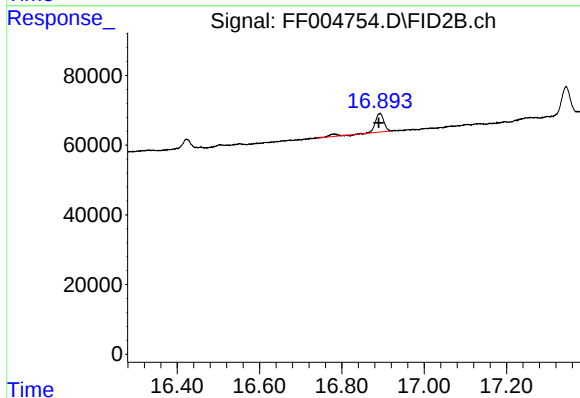


#12 N-OCTACOSANE

R.T.: 16.893 min
Delta R.T.: 0.003 min
Response: 82870
Conc: 0.61 ug/ml

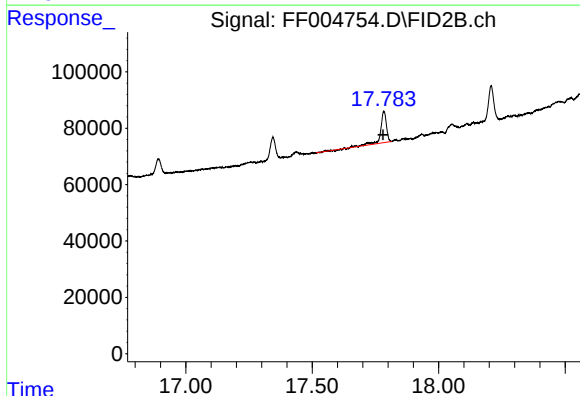


#13 N-TRIACONTANE

R.T.: 17.783 min
Delta R.T.: 0.002 min
Response: 178292
Conc: 1.29 ug/ml

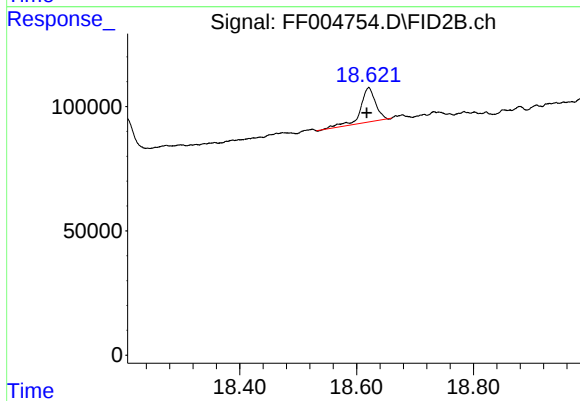

#14 N-DOTRIACONTANE


R.T.: 18.621 min
Delta R.T.: 0.004 min
Response: 248504
Conc: 1.80 ug/ml

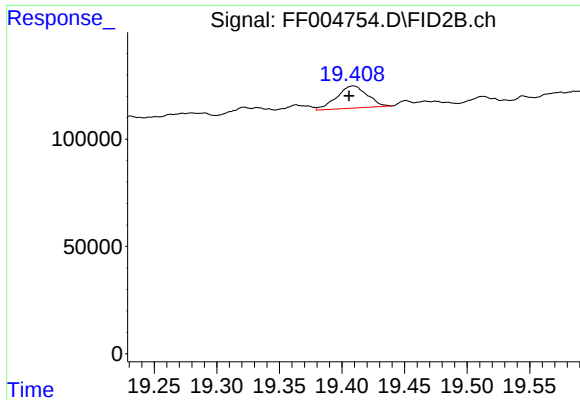

#15 N-TETRATRIACONTANE


R.T.: 19.409 min
Delta R.T.: 0.003 min
Response: 175181
Conc: 1.28 ug/ml

Instrument :
FID_F
ClientSampleId :

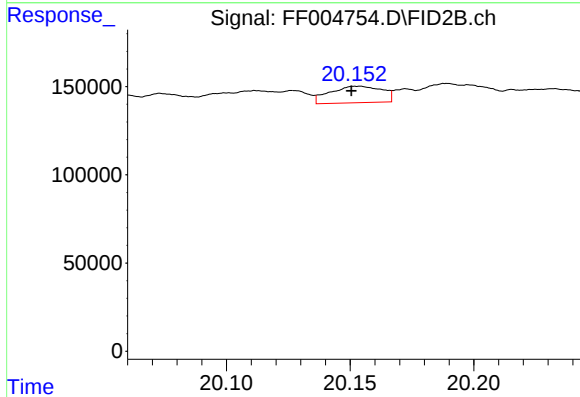

#16 N-HEXATRIACONTANE

R.T.: 20.153 min
Delta R.T.: 0.003 min
Response: 137209
Conc: 1.04 ug/ml

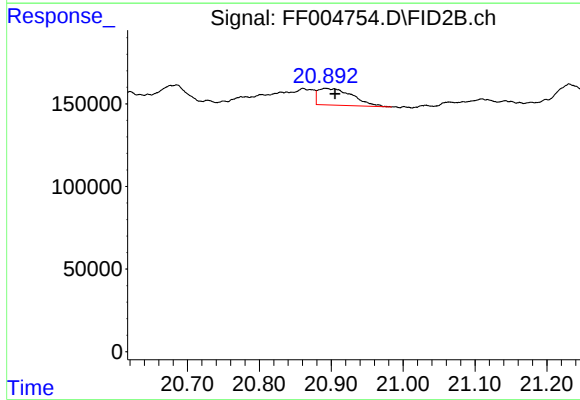

#17 N-OCTATRIACONTANE

R.T.: 20.892 min
Delta R.T.: -0.014 min
Response: 332828
Conc: 2.77 ug/ml