

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
 Data File : FF004736.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jun 2019 12:56
 Operator : DD\AJ
 Sample : K3192-01MS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CLVR-AVEX-WC1BMS

Integration File: autoint1.e
 Quant Time: Jun 07 13:52:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.707	2418748	19.808 ug/ml
Target Compounds			
1) N-OCTANE	2.310	2127976	14.750 ug/ml
2) N-DECANE	4.417	3177497	21.700 ug/ml
3) N-DODECANE	6.441	3299915	22.299 ug/ml
4) N-TETRADECANE	8.237	3281871	22.343 ug/ml
5) N-HEXADECANE	9.840	3255589	22.050 ug/ml
6) N-OCTADECANE	11.287	3172512	21.852 ug/ml
7) N-EICOSANE	12.602	3143923	21.708 ug/ml
8) N-DOCOSANE	13.804	3107018	21.988 ug/ml
10) N-TETRACOSANE	14.912	3221900	23.248 ug/ml
11) N-HEXACOSANE	15.937	3231383	23.716 ug/ml
12) N-OCTACOSANE	16.893	3517679	25.873 ug/ml
13) N-TRIACONTANE	17.785	3620404	26.181 ug/ml
14) N-DOTRIACONTANE	18.624	3430618	24.800 ug/ml
15) N-TETRATRIACONTANE	19.417	3040646	22.240 ug/ml
16) N-HEXATRIACONTANE	20.165	2835740	21.540 ug/ml
17) N-OCTATRIACONTANE	20.923	2630751	21.877 ug/ml
18) N-TETRACONTANE	21.853	2710363	22.010 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
Data File : FF004736.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2019 12:56
Operator : DD\AJ
Sample : K3192-01MS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CLVR-AVEX-WC1BMS

Integration File: autoint1.e
Quant Time: Jun 07 13:52:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

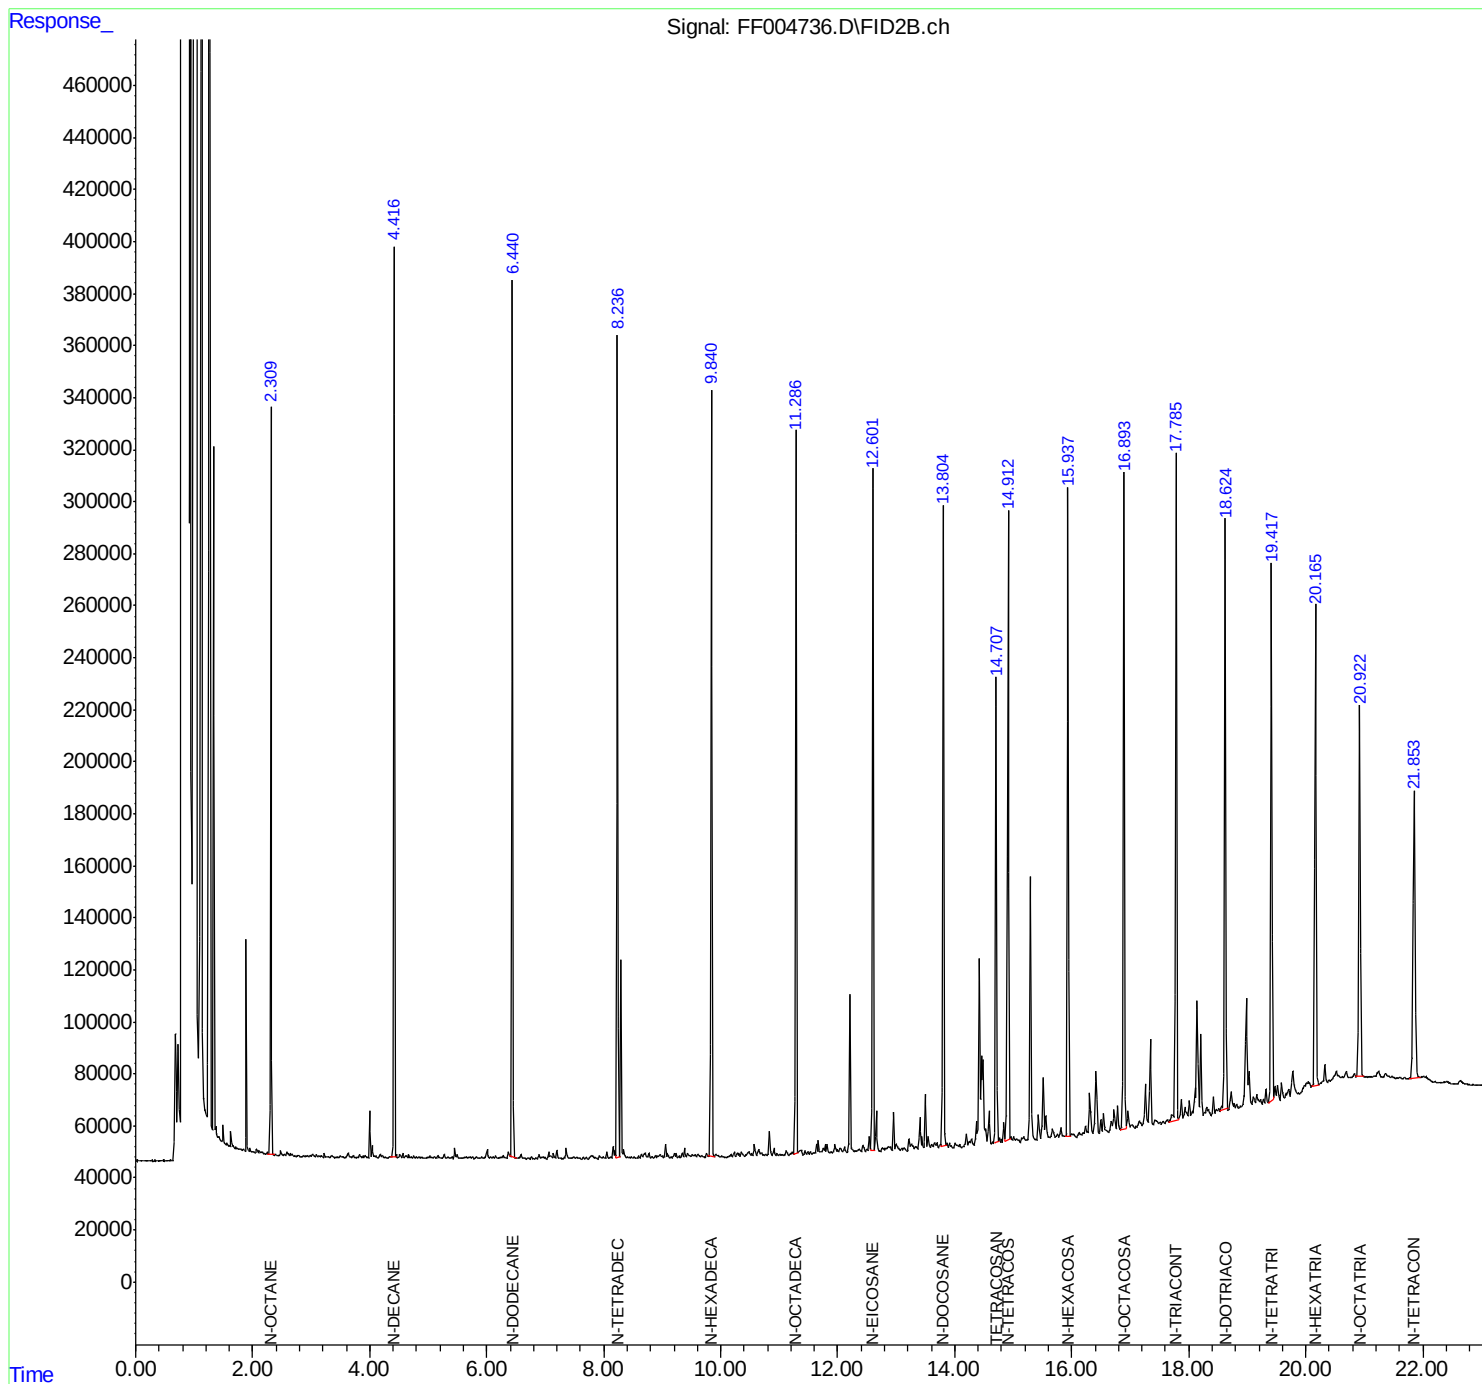


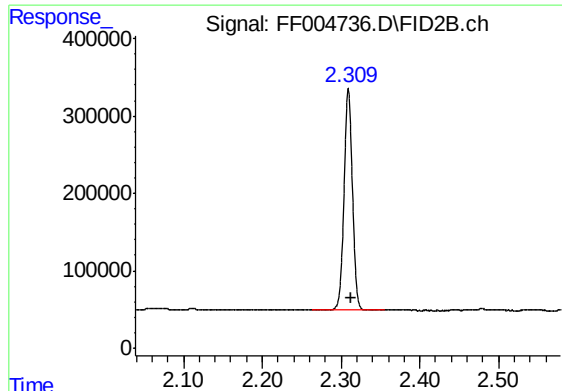

#1 N-OCTANE


R.T.: 2.310 min
Delta R.T.: -0.003 min
Response: 2127976
Conc: 14.75 ug/ml

Instrument :
FID_F
ClientSampleId :
CLVR-AVEX-WC1BMS

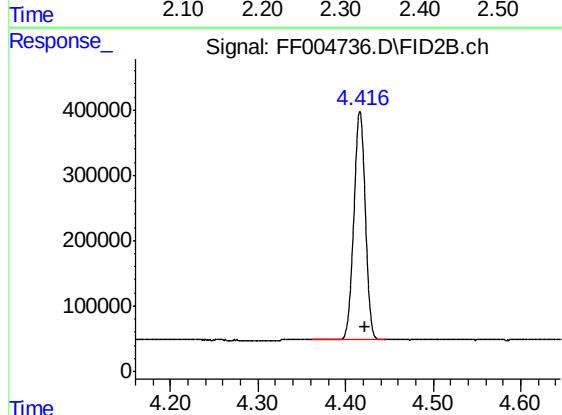


#2 N-DECANE

R.T.: 4.417 min
Delta R.T.: -0.006 min
Response: 3177497
Conc: 21.70 ug/ml

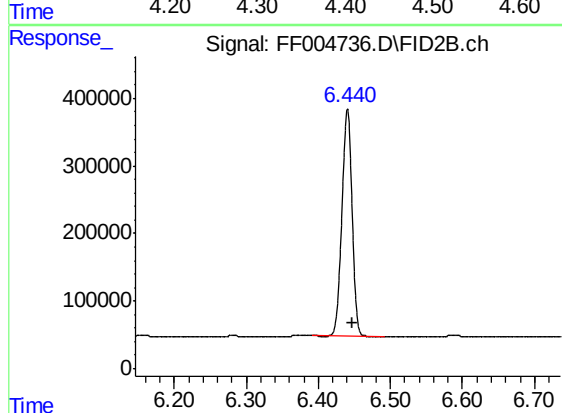


#3 N-DODECANE

R.T.: 6.441 min
Delta R.T.: -0.007 min
Response: 3299915
Conc: 22.30 ug/ml

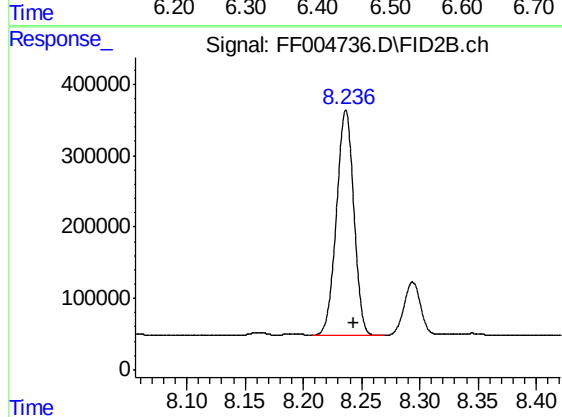

#4 N-TETRADECANE


R.T.: 8.237 min
Delta R.T.: -0.007 min
Response: 3281871
Conc: 22.34 ug/ml

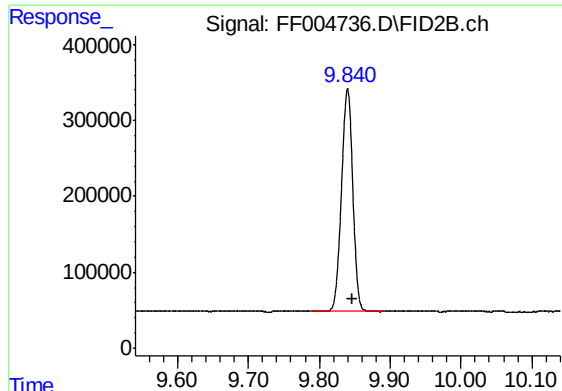

#5 N-HEXADECANE


R.T.: 9.840 min
Delta R.T.: -0.007 min
Response: 3255589
Conc: 22.05 ug/ml

Instrument :
FID_F
ClientSampleId :
CLVR-AVEX-WC1BMS

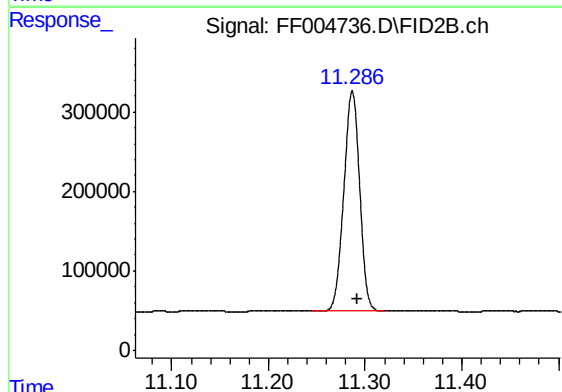


#6 N-OCTADECANE

R.T.: 11.287 min
Delta R.T.: -0.005 min
Response: 3172512
Conc: 21.85 ug/ml

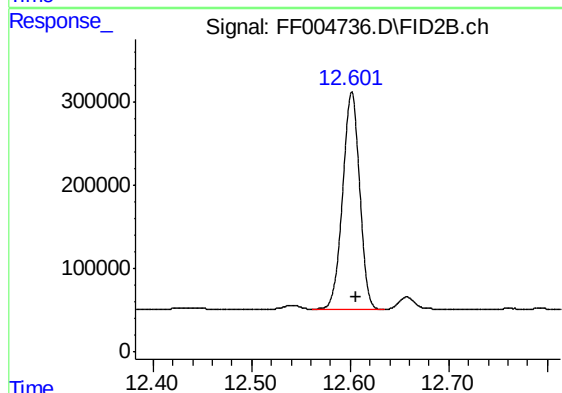


#7 N-EICOSANE

R.T.: 12.602 min
Delta R.T.: -0.004 min
Response: 3143923
Conc: 21.71 ug/ml

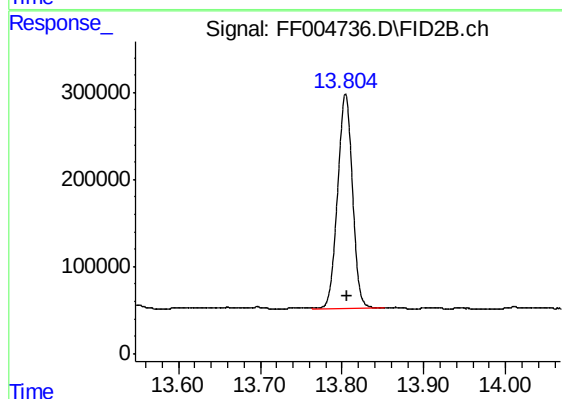

#8 N-DOCOSANE


R.T.: 13.804 min
Delta R.T.: -0.002 min
Response: 3107018
Conc: 21.99 ug/ml

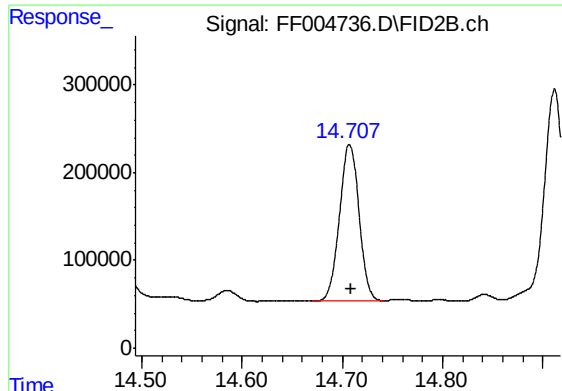

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.707 min
Delta R.T.: -0.001 min
Response: 2418748
Conc: 19.81 ug/ml

Instrument :
FID_F
ClientSampleId :
CLVR-AVEX-WC1BMS

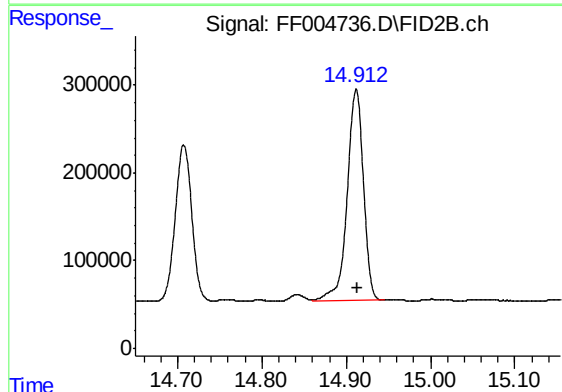


#10 N-TETRACOSANE

R.T.: 14.912 min
Delta R.T.: -0.002 min
Response: 3221900
Conc: 23.25 ug/ml

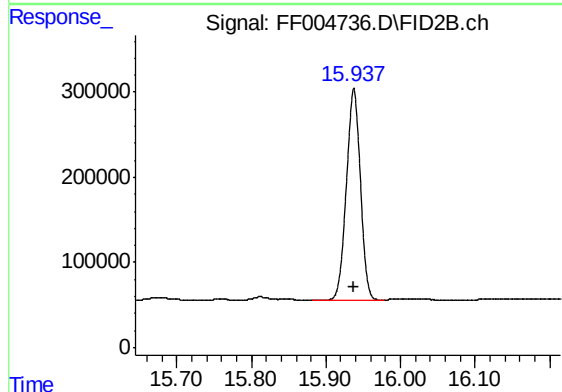


#11 N-HEXACOSANE

R.T.: 15.937 min
Delta R.T.: 0.000 min
Response: 3231383
Conc: 23.72 ug/ml

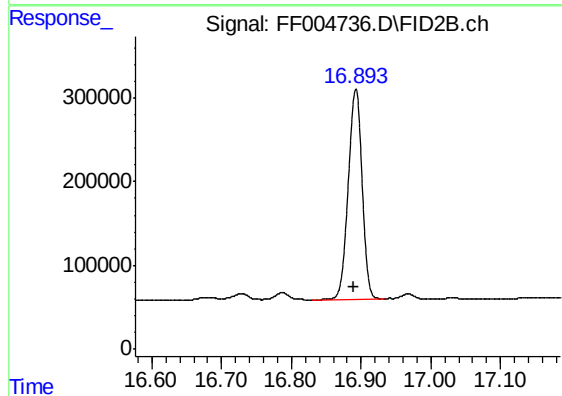

#12 N-OCTACOSANE


R.T.: 16.893 min
Delta R.T.: 0.003 min
Response: 3517679
Conc: 25.87 ug/ml

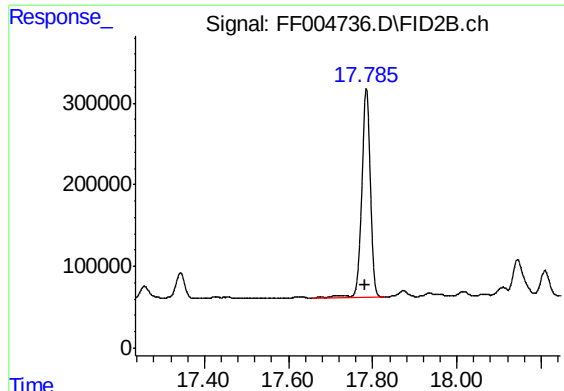

#13 N-TRIACONTANE


R.T.: 17.785 min
Delta R.T.: 0.004 min
Response: 3620404
Conc: 26.18 ug/ml

Instrument :
FID_F
ClientSampleId :
CLVR-AVEX-WC1BMS

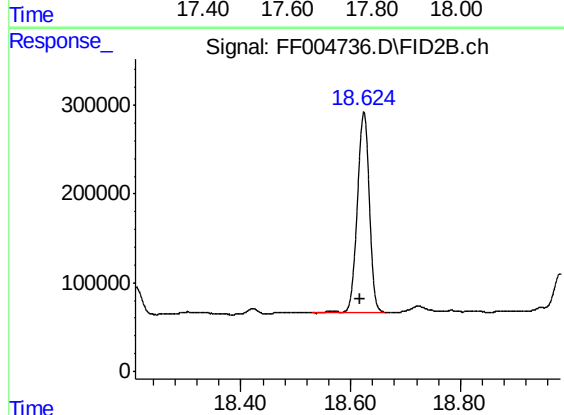


#14 N-DOTRIACONTANE

R.T.: 18.624 min
Delta R.T.: 0.007 min
Response: 3430618
Conc: 24.80 ug/ml

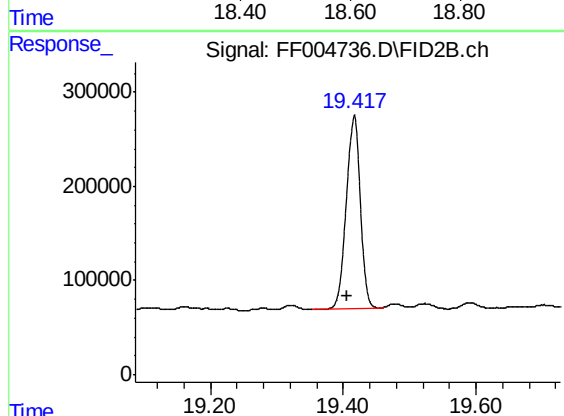


#15 N-TETRATRIACONTANE

R.T.: 19.417 min
Delta R.T.: 0.011 min
Response: 3040646
Conc: 22.24 ug/ml

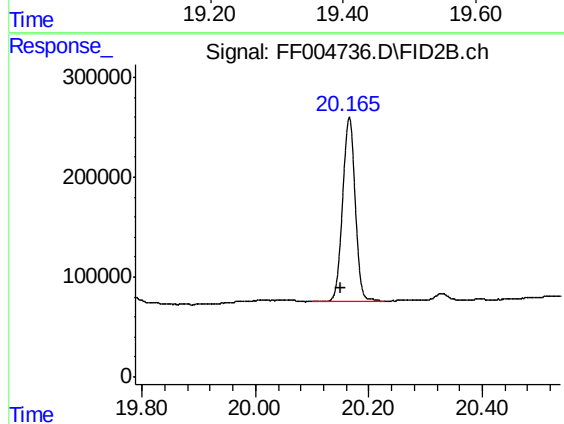

#16 N-HEXATRIACONTANE


R.T.: 20.165 min
Delta R.T.: 0.015 min
Response: 2835740
Conc: 21.54 ug/ml

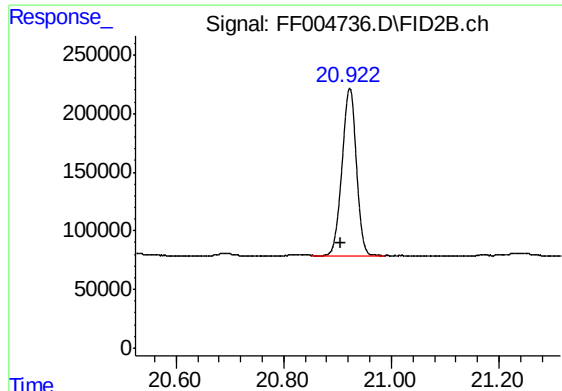

#17 N-OCTATRIACONTANE

R.T.: 20.923 min
Delta R.T.: 0.018 min
Response: 2630751
Conc: 21.88 ug/ml

Instrument :
FID_F
ClientSampleId :
CLVR-AVEX-WC1BMS

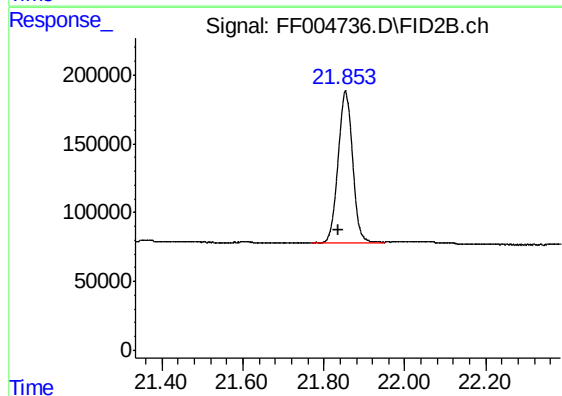

#18 N-TETRACONTANE

R.T.: 21.853 min
Delta R.T.: 0.016 min
Response: 2710363
Conc: 22.01 ug/ml