

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
 Data File : FF004743.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jun 2019 16:23
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 21:41:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.709	5593191	45.804 ug/ml
Target Compounds			
2) N-DECANE	4.417	7335009	50.092 ug/ml
3) N-DODECANE	6.441	7205203	48.690 ug/ml
4) N-TETRADECANE	8.238	6980956	47.525 ug/ml
5) N-HEXADECANE	9.842	6844370	46.357 ug/ml
6) N-OCTADECANE	11.289	6603605	45.485 ug/ml
7) N-EICOSANE	12.603	6519069	45.013 ug/ml
8) N-DOCOSANE	13.806	6386971	45.200 ug/ml
10) N-TETRACOSANE	14.914	6369077	45.957 ug/ml
11) N-HEXACOSANE	15.940	6382472	46.843 ug/ml
12) N-OCTACOSANE	16.895	6469511	47.584 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060719\
Data File : FF004743.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2019 16:23
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 21:41:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

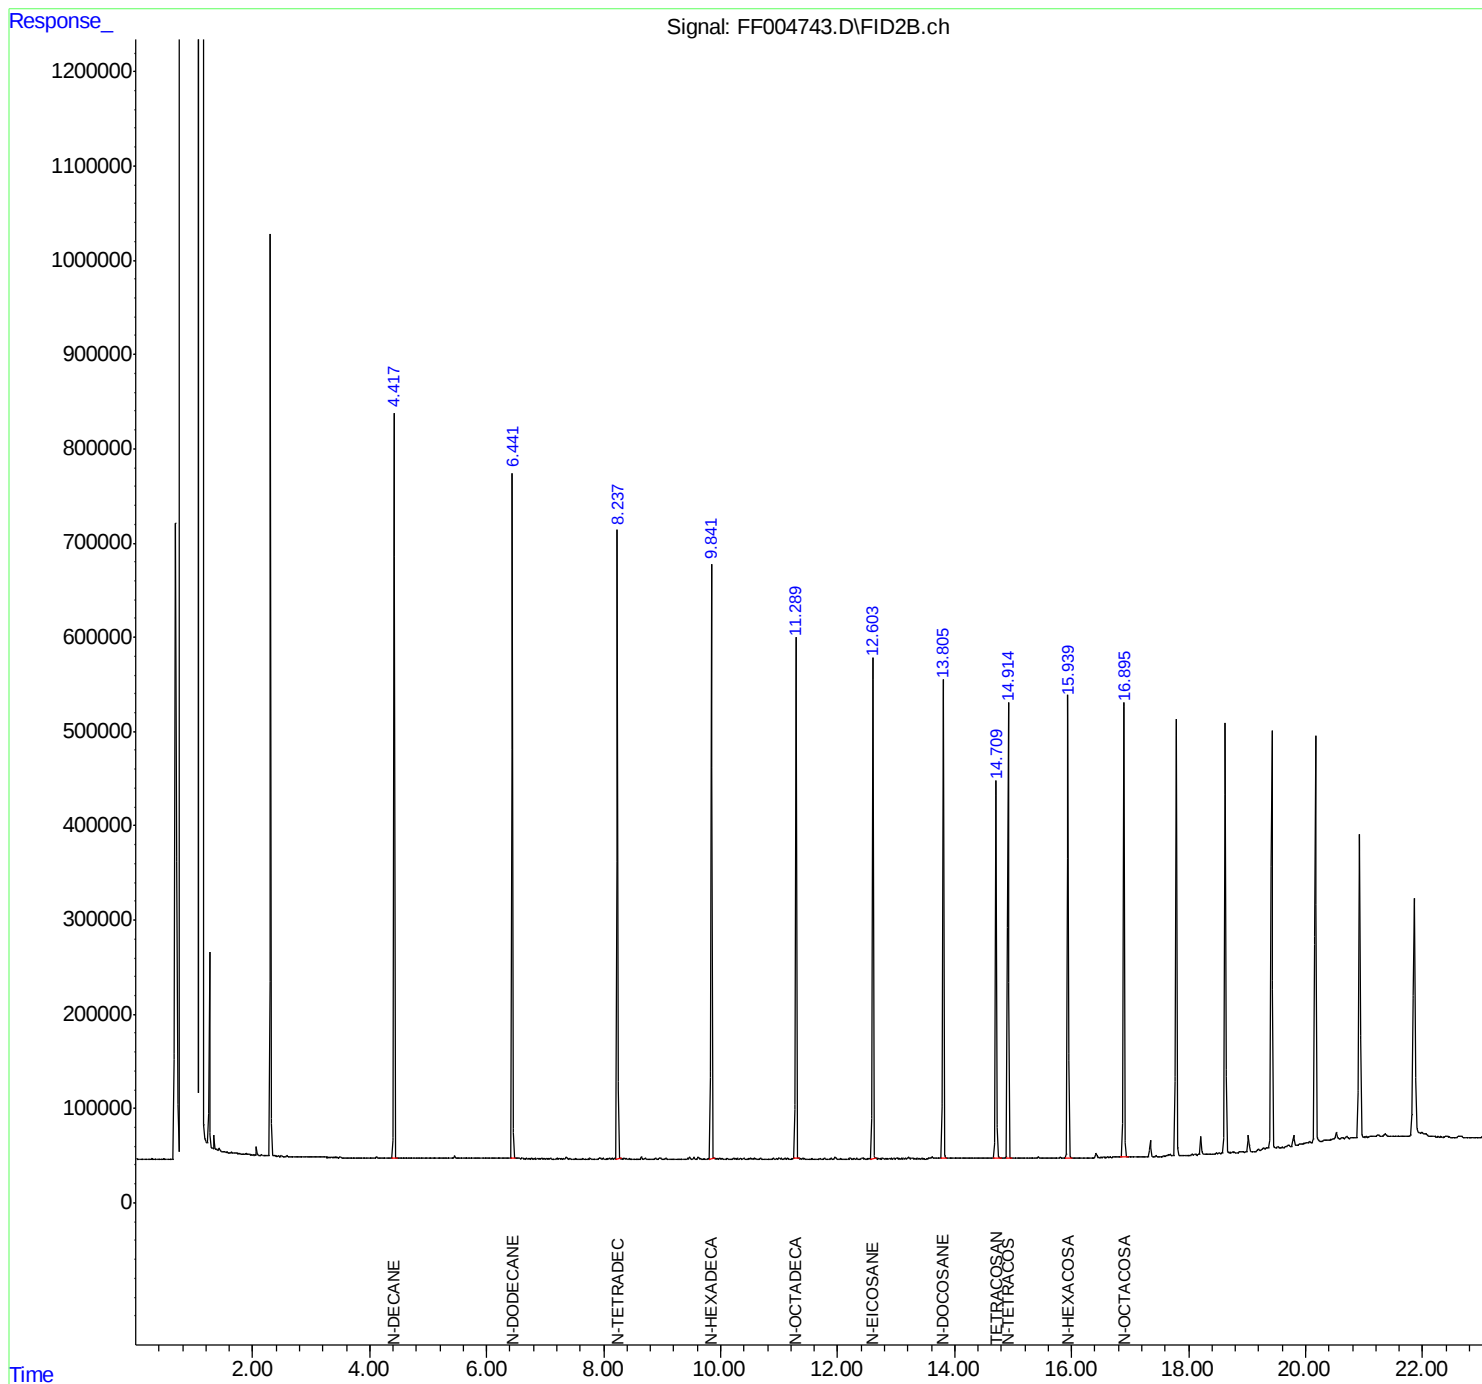


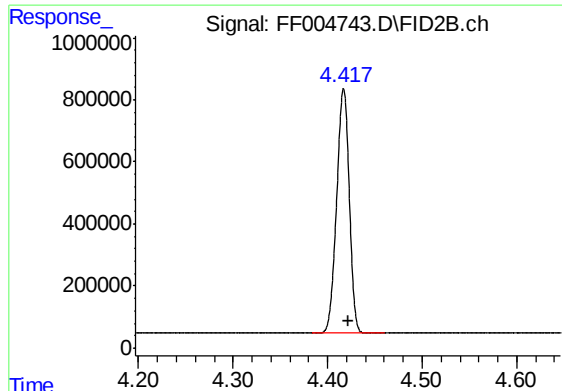

#2 N-DECANE


R.T.: 4.417 min
Delta R.T.: -0.005 min
Response: 7335009
Conc: 50.09 ug/ml

Instrument :
FID_F
ClientSampleId :

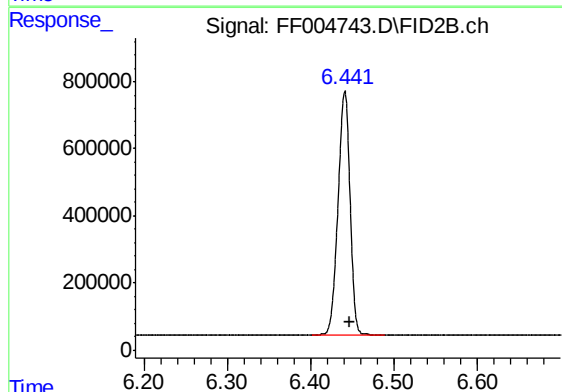


#3 N-DODECANE

R.T.: 6.441 min
Delta R.T.: -0.007 min
Response: 7205203
Conc: 48.69 ug/ml

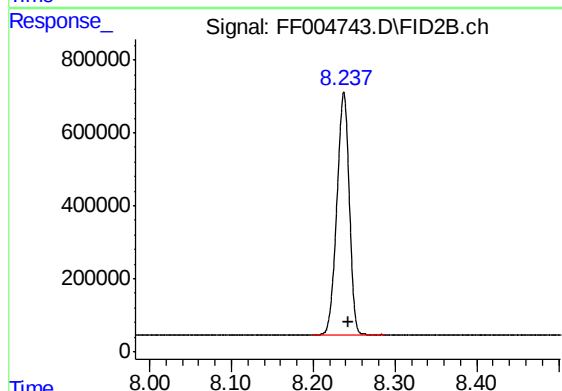


#4 N-TETRADECANE

R.T.: 8.238 min
Delta R.T.: -0.006 min
Response: 6980956
Conc: 47.53 ug/ml

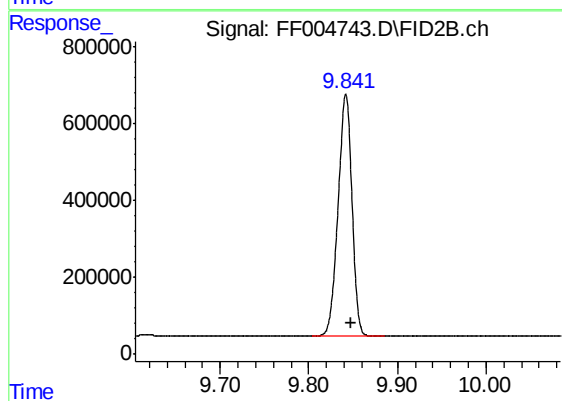

#5 N-HEXADECANE


R.T.: 9.842 min
Delta R.T.: -0.006 min
Response: 6844370
Conc: 46.36 ug/ml

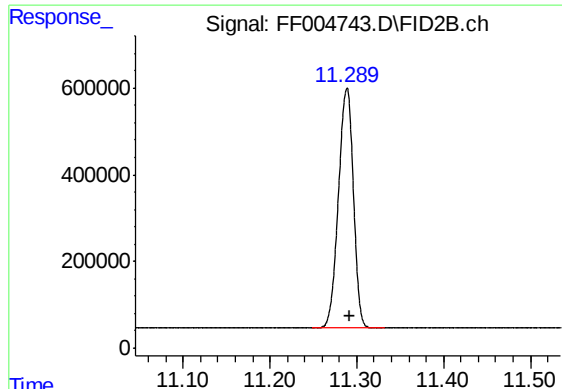

#6 N-OCTADECANE


R.T.: 11.289 min
Delta R.T.: -0.003 min
Response: 6603605
Conc: 45.48 ug/ml

Instrument :
FID_F
ClientSampleId :

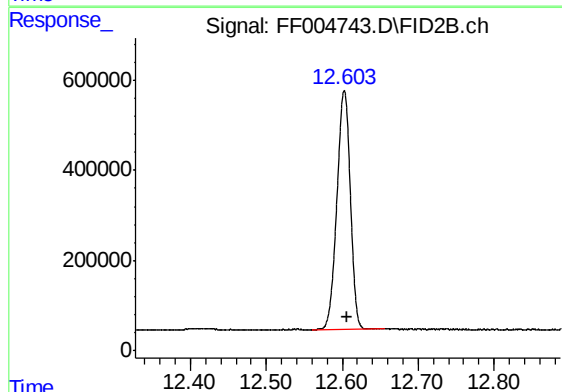


#7 N-EICOSANE

R.T.: 12.603 min
Delta R.T.: -0.003 min
Response: 6519069
Conc: 45.01 ug/ml

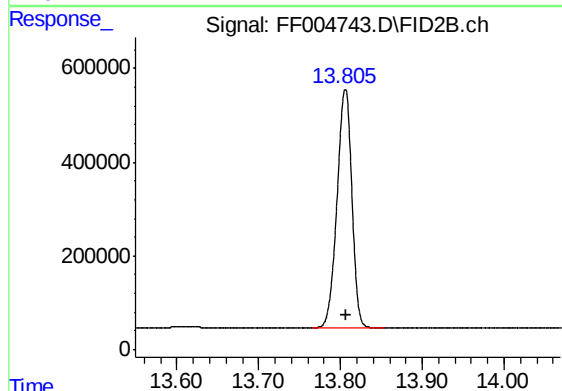


#8 N-DOCOSANE

R.T.: 13.806 min
Delta R.T.: 0.000 min
Response: 6386971
Conc: 45.20 ug/ml

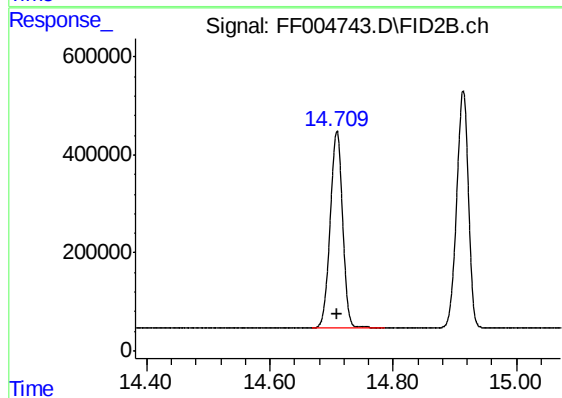

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.709 min
Delta R.T.: 0.000 min
Response: 5593191
Conc: 45.80 ug/ml

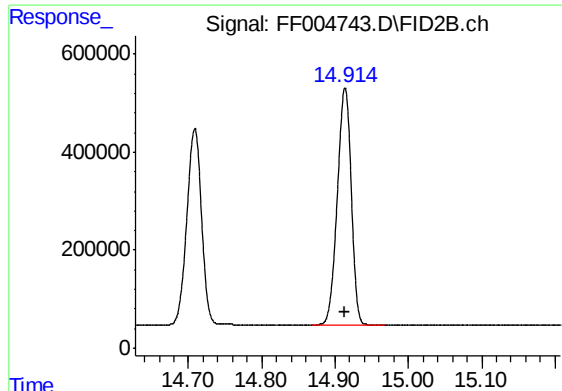

#10 N-TETRACOSANE


R.T.: 14.914 min
Delta R.T.: 0.000 min
Response: 6369077
Conc: 45.96 ug/ml

Instrument :
FID_F
ClientSampleId :

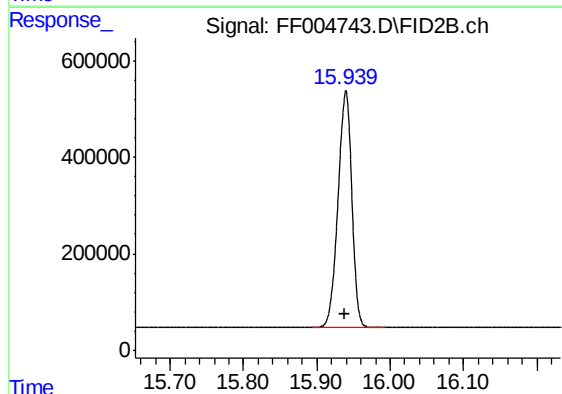

#11 N-HEXACOSANE

R.T.: 15.940 min
Delta R.T.: 0.002 min
Response: 6382472
Conc: 46.84 ug/ml

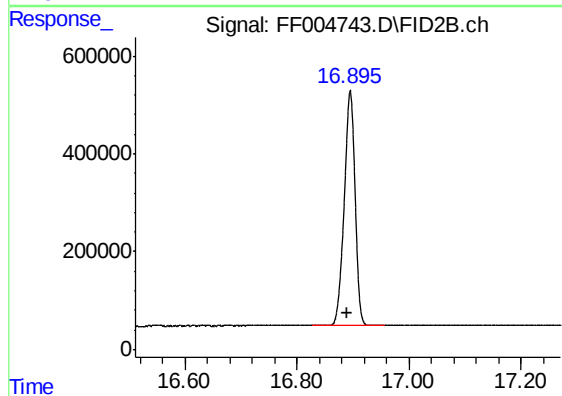

#12 N-OCTACOSANE

R.T.: 16.895 min
Delta R.T.: 0.005 min
Response: 6469511
Conc: 47.58 ug/ml