

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
Data File : FF008540.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2021 08:16
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:28:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.770	2084105	19.780 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.657	112182	0.932 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
Data File : FF008540.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2021 08:16
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:28:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

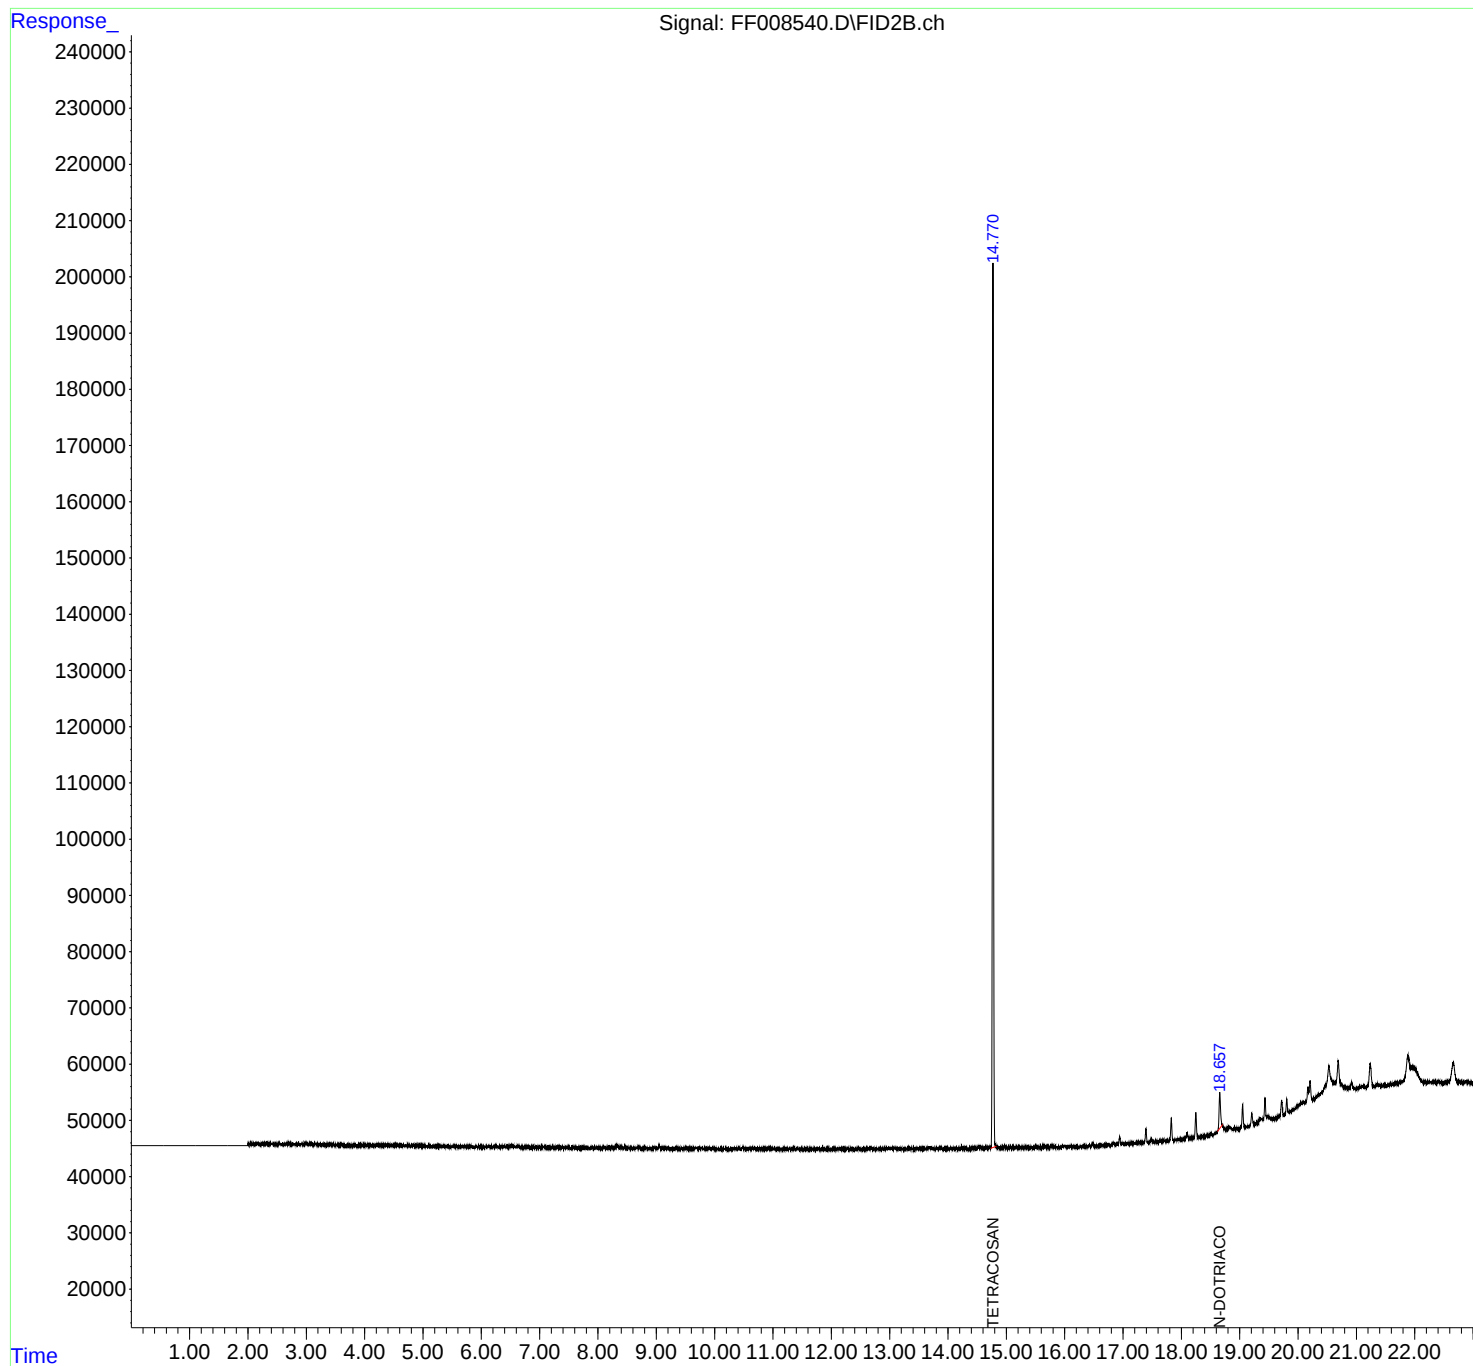


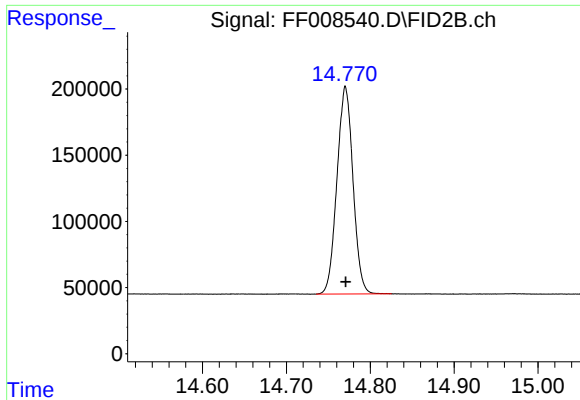

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.770 min
Delta R.T.: 0.000 min
Response: 2084105
Conc: 19.78 ug/ml

Instrument :
FID_F
ClientSampleId :

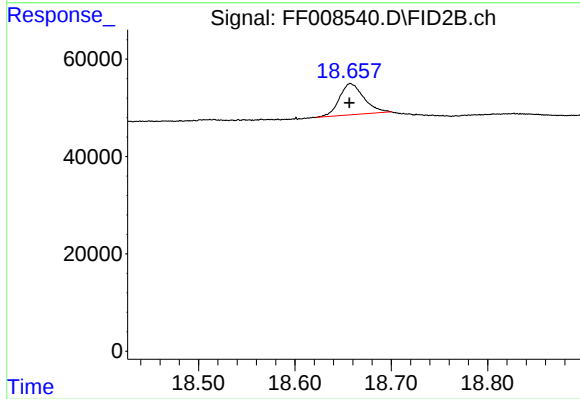

#14 N-DOTRIACONTANE

R.T.: 18.657 min
Delta R.T.: 0.000 min
Response: 112182
Conc: 0.93 ug/ml