

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
Data File : FF008547.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2021 11:58
Operator : DD\AJ
Sample : M2612-06
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:29:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.771	1980085	18.792 ug/ml
Target Compounds			
4) N-TETRADECANE	8.395f	772336	6.069 ug/ml
14) N-DOTRIACONTANE	18.654	183253	1.523 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
Data File : FF008547.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2021 11:58
Operator : DD\AJ
Sample : M2612-06
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:29:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

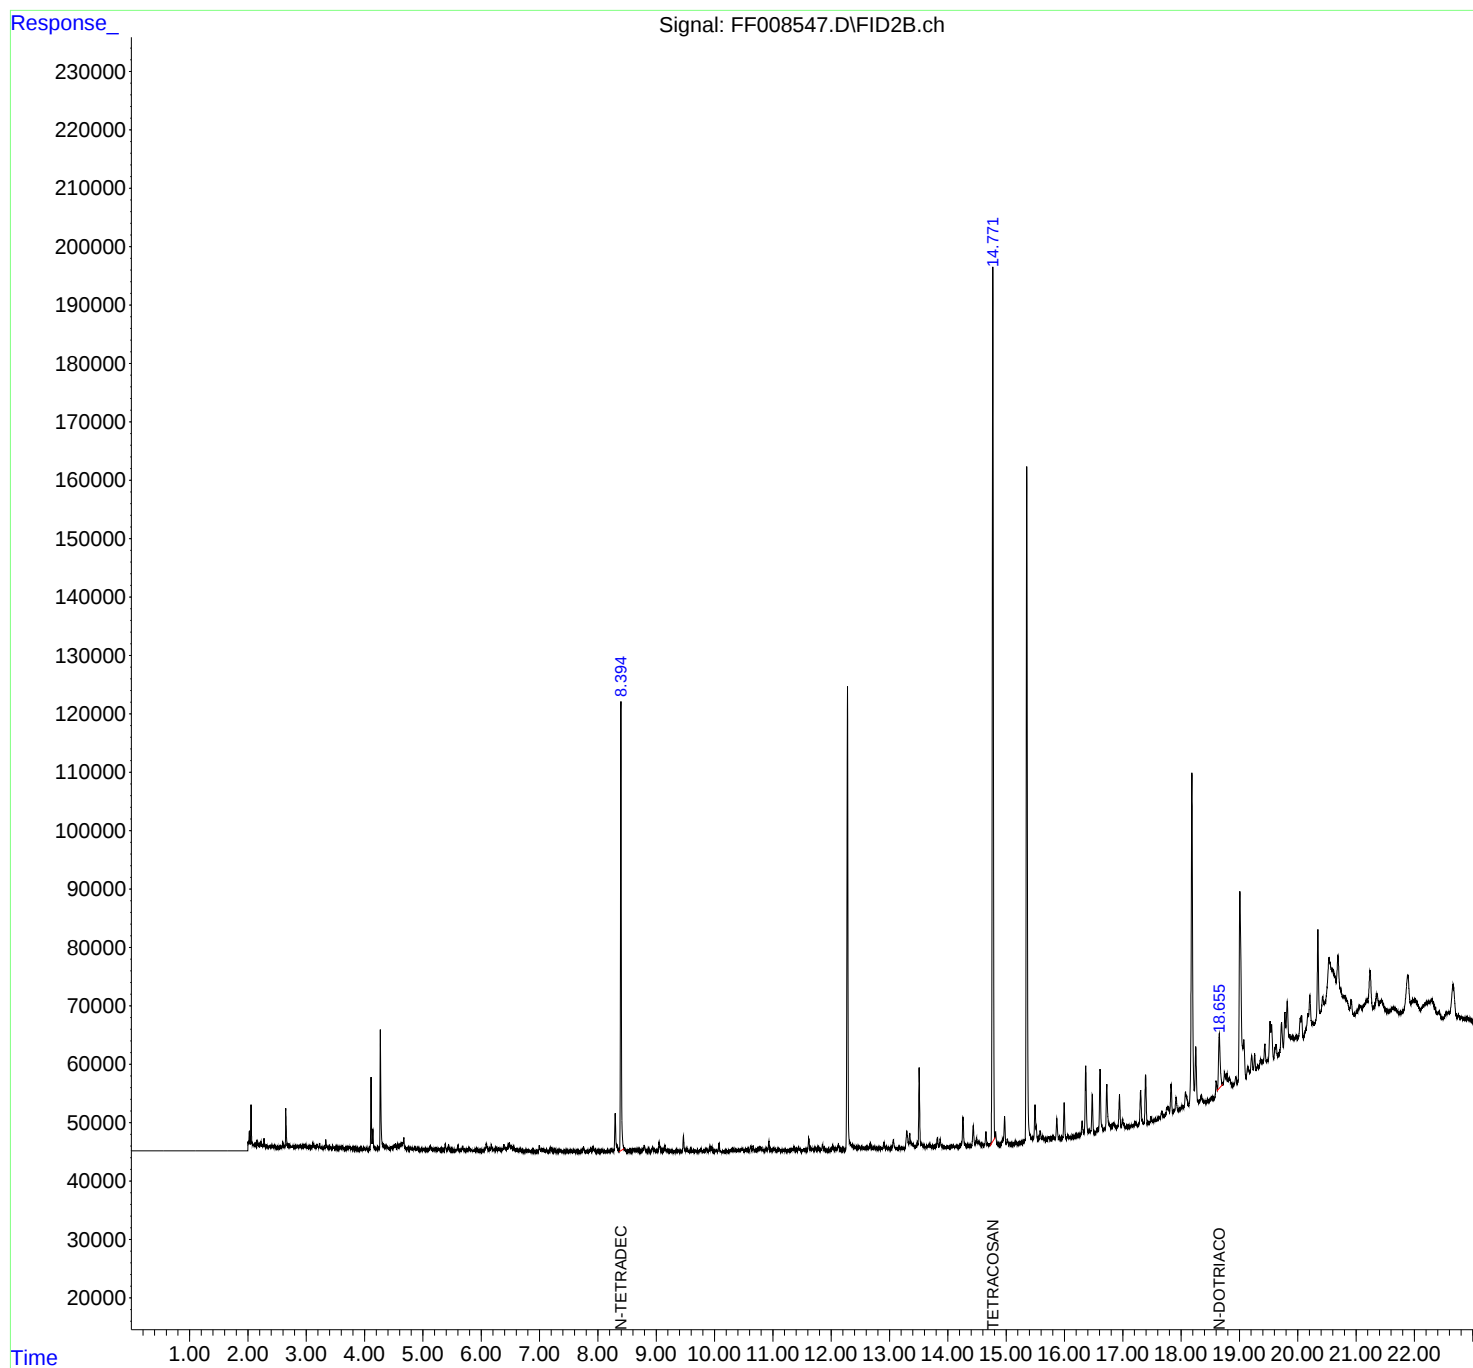


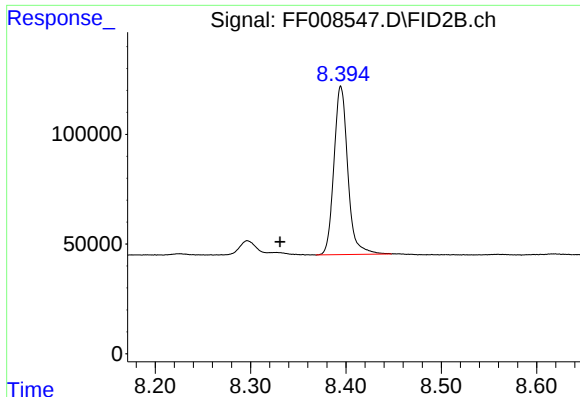

#4 N-TETRADECANE


R.T.: 8.395 min
Delta R.T.: 0.064 min
Response: 772336
Conc: 6.07 ug/ml

Instrument :
FID_F
ClientSampleId :

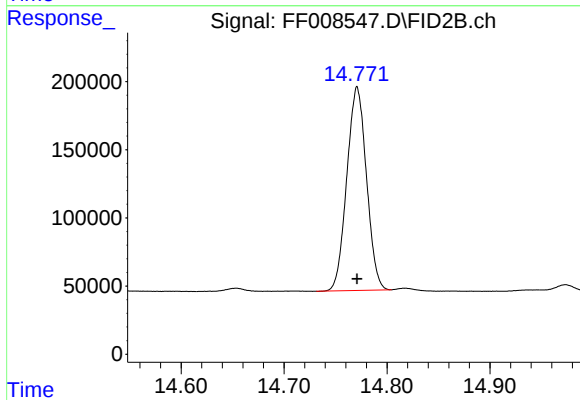

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.771 min
Delta R.T.: 0.000 min
Response: 1980085
Conc: 18.79 ug/ml

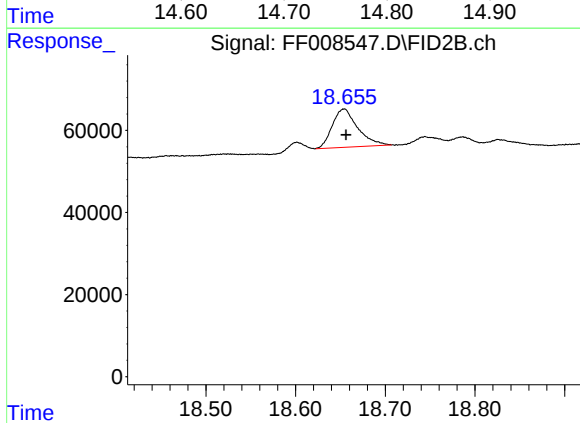

#14 N-DOTRIACONTANE

R.T.: 18.654 min
Delta R.T.: -0.002 min
Response: 183253
Conc: 1.52 ug/ml