

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
 Data File : FF008548.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jun 2021 12:30
 Operator : DD\AJ
 Sample : M2612-07
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 08 01:30:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.771	1939903	18.411 ug/ml
Target Compounds			
4) N-TETRADECANE	8.395f	704724	5.538 ug/ml
14) N-DOTRIACONTANE	18.653	205578	1.708 ug/ml
18) N-TETRACONTANE	21.886	175375	1.660 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
Data File : FF008548.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2021 12:30
Operator : DD\AJ
Sample : M2612-07
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:30:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

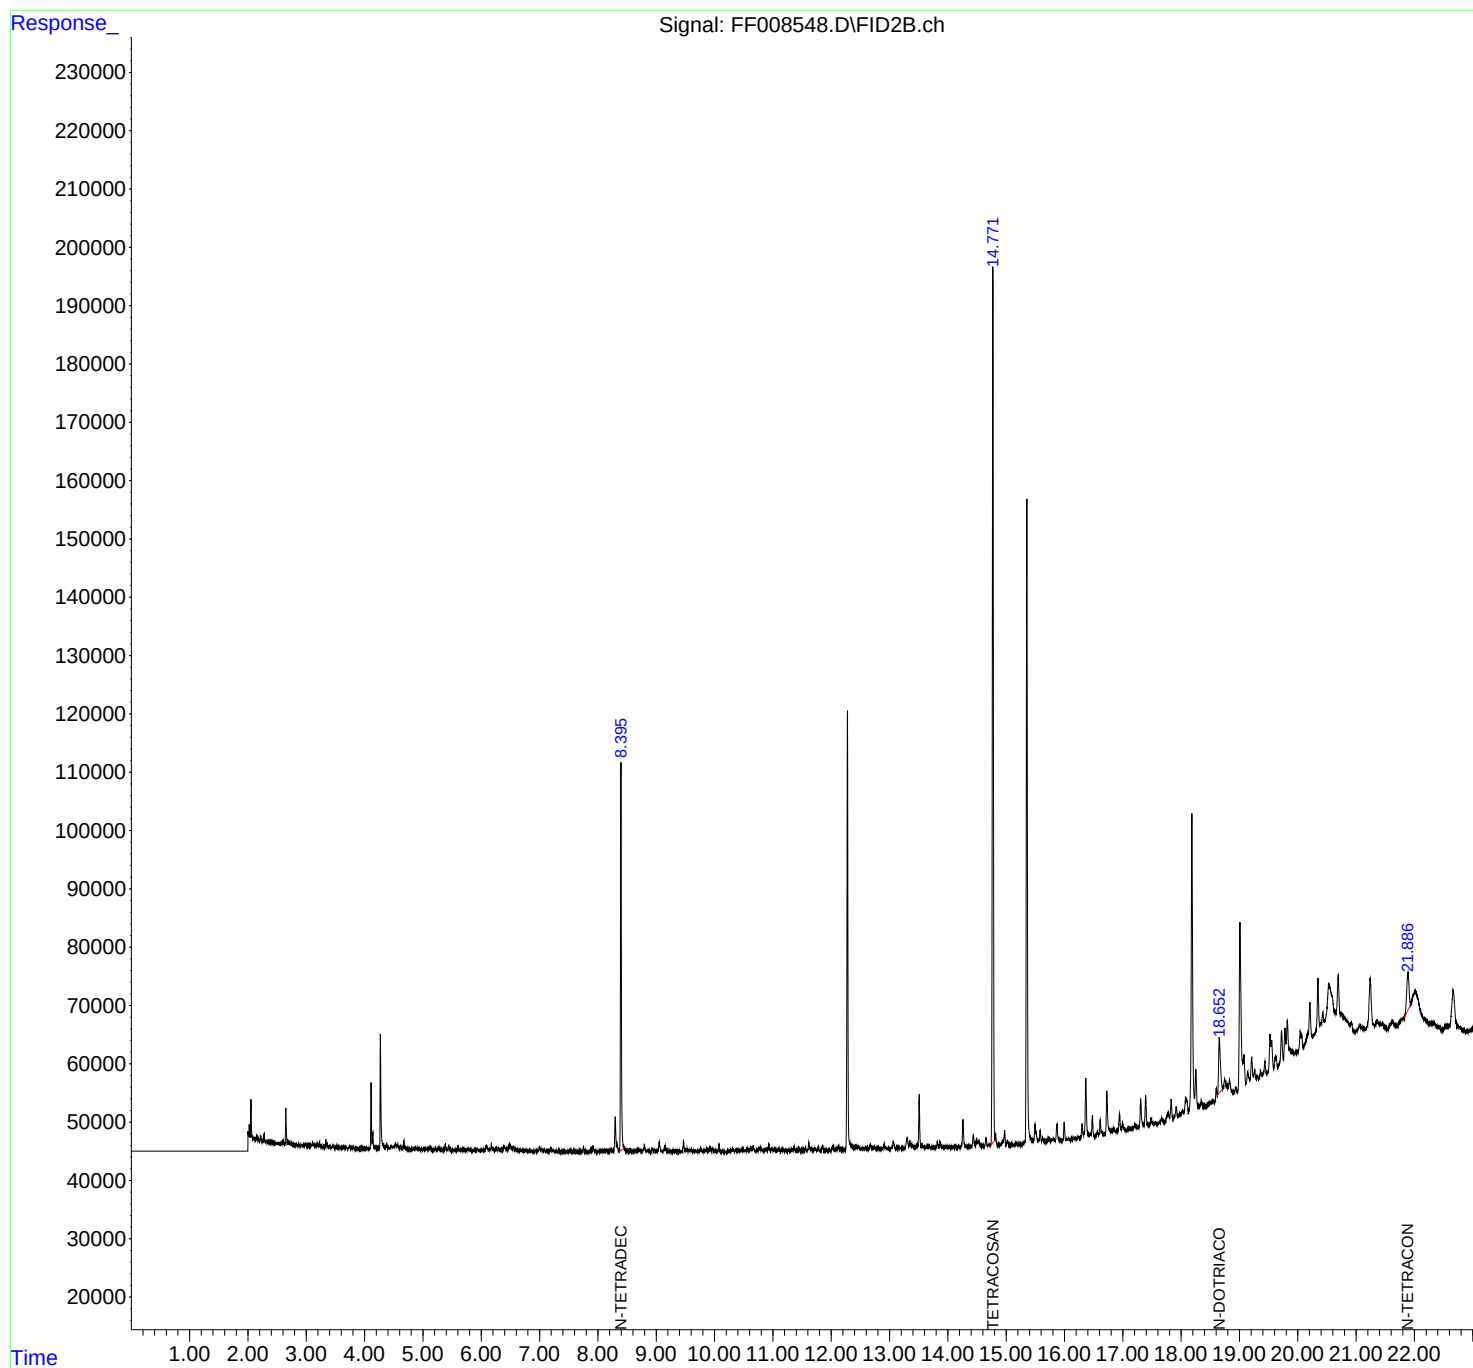


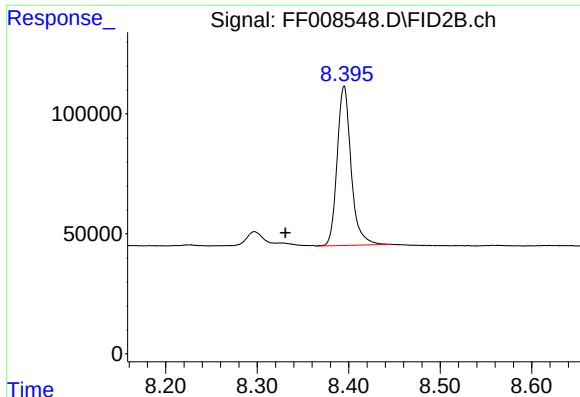

#4 N-TETRADECANE


R.T.: 8.395 min
Delta R.T.: 0.064 min
Response: 704724
Conc: 5.54 ug/ml

Instrument :
FID_F
ClientSampleId :

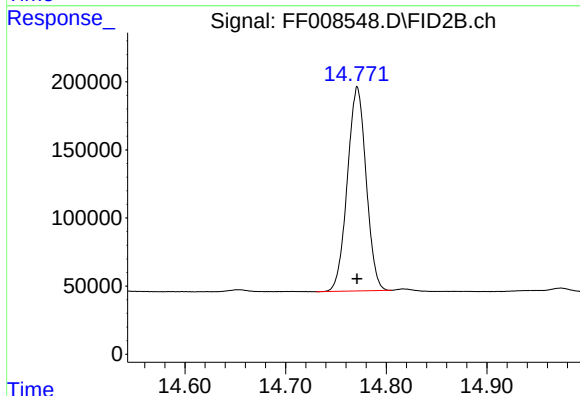


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.771 min
Delta R.T.: 0.000 min
Response: 1939903
Conc: 18.41 ug/ml

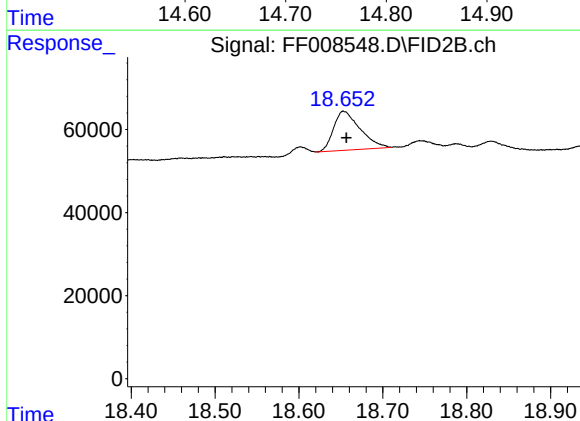

#14 N-DOTRIACONTANE

R.T.: 18.653 min
Delta R.T.: -0.004 min
Response: 205578
Conc: 1.71 ug/ml

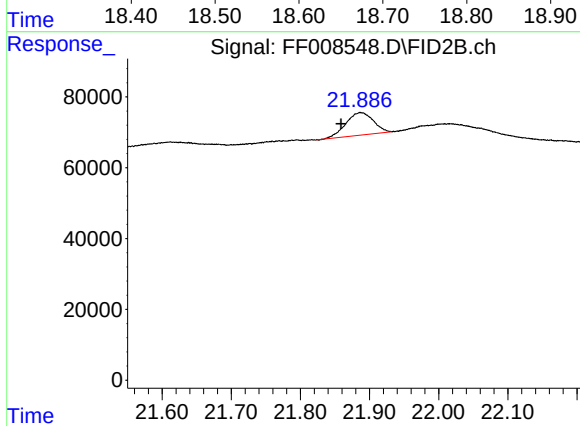

#18 N-TETRACONTANE

R.T.: 21.886 min
Delta R.T.: 0.028 min
Response: 175375
Conc: 1.66 ug/ml