

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
 Data File : FF008551.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jun 2021 14:06
 Operator : DD\AJ
 Sample : M2612-10
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 08 01:30:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.770	1969200	18.689 ug/ml
Target Compounds			
4) N-TETRADECANE	8.394f	629814	4.949 ug/ml
10) N-TETRACOSANE	14.973	94392	0.770 ug/ml
11) N-HEXACOSANE	15.996	135014	1.126 ug/ml
12) N-OCTACOSANE	16.944	115198	0.971 ug/ml
13) N-TRIACONTANE	17.828	90947	0.768 ug/ml
14) N-DOTRIACONTANE	18.653	105202	0.874 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
Data File : FF008551.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2021 14:06
Operator : DD\AJ
Sample : M2612-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:30:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

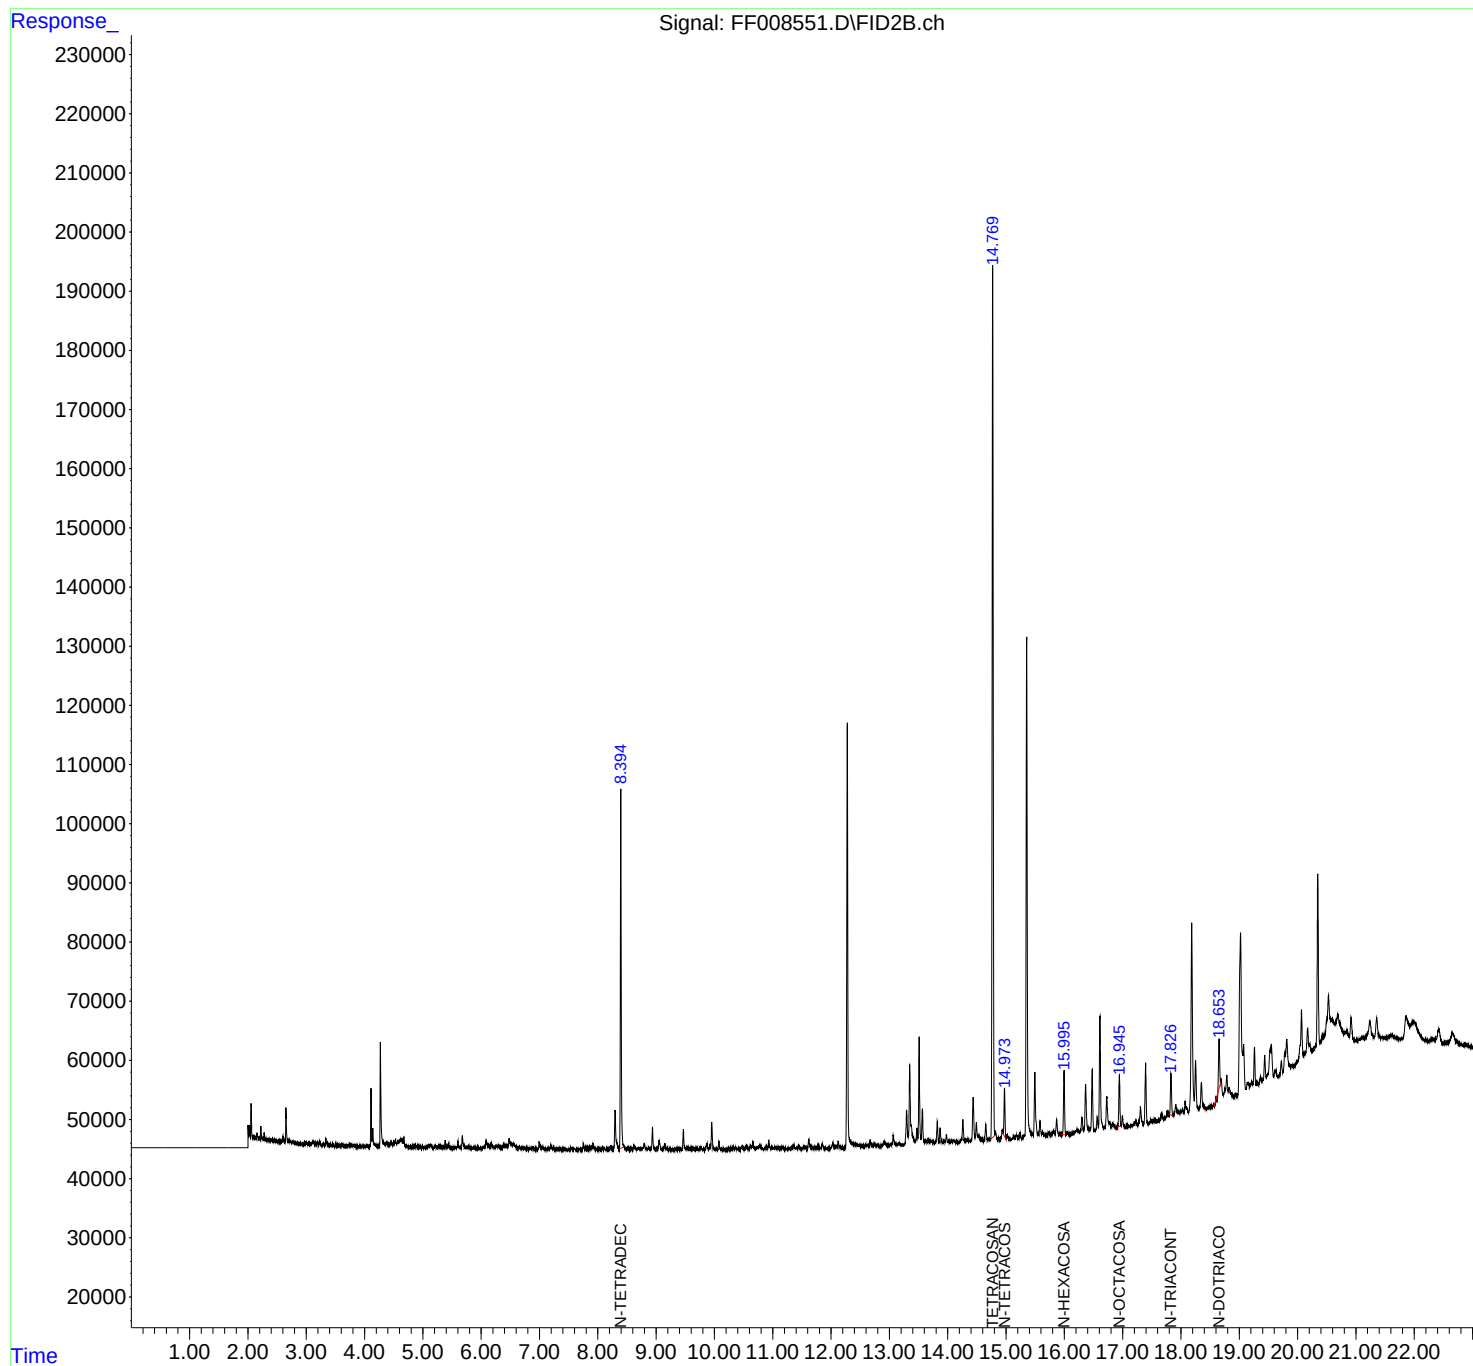


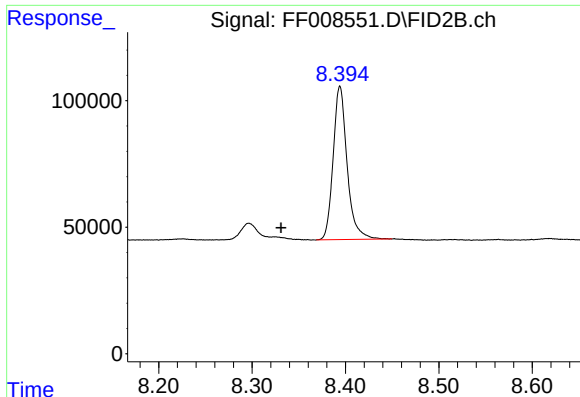

#4 N-TETRADECANE


R.T.: 8.394 min
Delta R.T.: 0.063 min
Response: 629814
Conc: 4.95 ug/ml

Instrument :
FID_F
ClientSampleId :

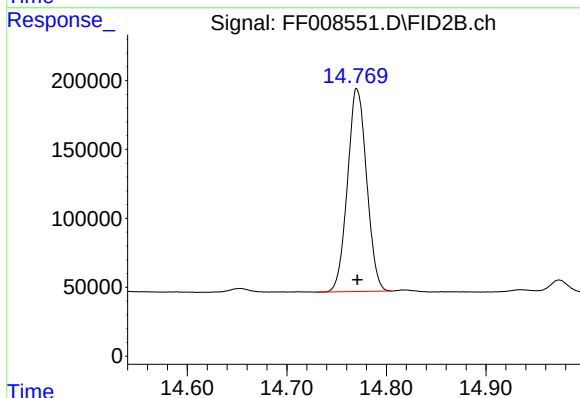


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.770 min
Delta R.T.: 0.000 min
Response: 1969200
Conc: 18.69 ug/ml

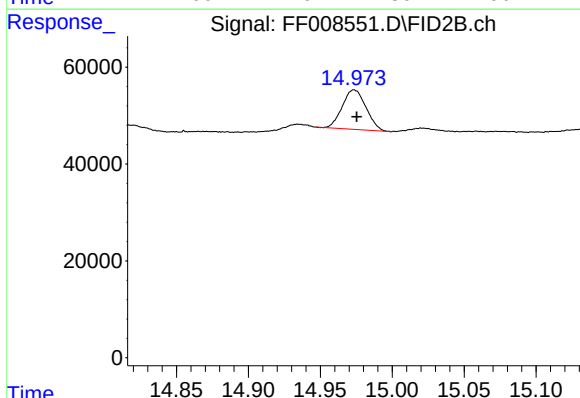


#10 N-TETRACOSANE

R.T.: 14.973 min
Delta R.T.: -0.002 min
Response: 94392
Conc: 0.77 ug/ml

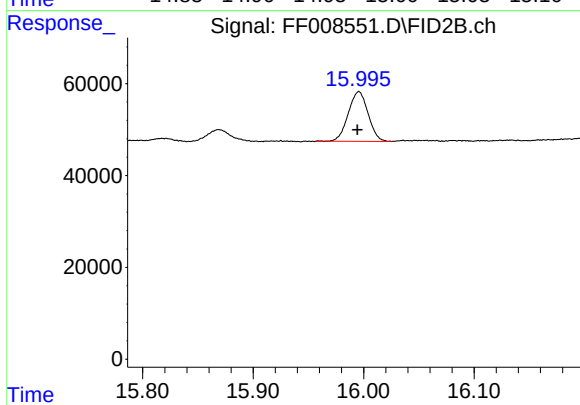

#11 N-HEXACOSANE


R.T.: 15.996 min
Delta R.T.: 0.001 min
Response: 135014
Conc: 1.13 ug/ml

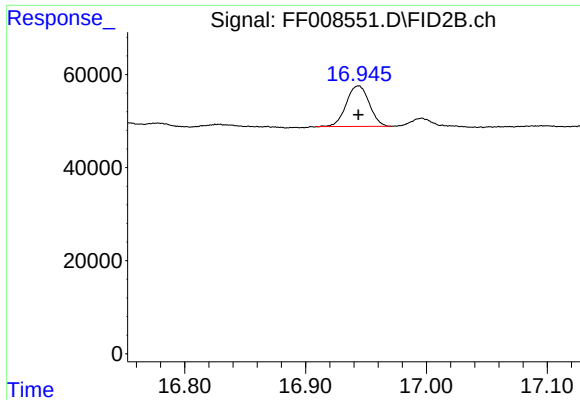

#12 N-OCTACOSANE


R.T.: 16.944 min
Delta R.T.: 0.000 min
Response: 115198
Conc: 0.97 ug/ml

Instrument :
FID_F
ClientSampleId :

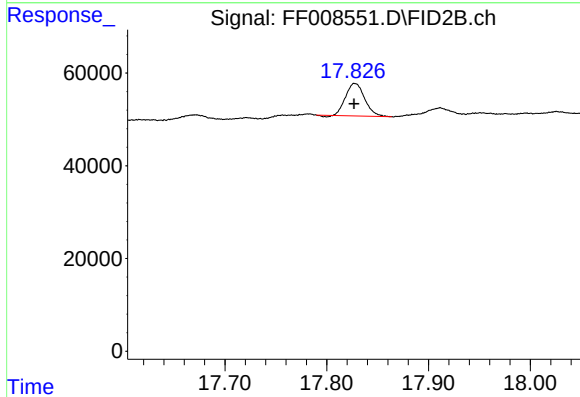

#13 N-TRIACONTANE

R.T.: 17.828 min
Delta R.T.: 0.000 min
Response: 90947
Conc: 0.77 ug/ml

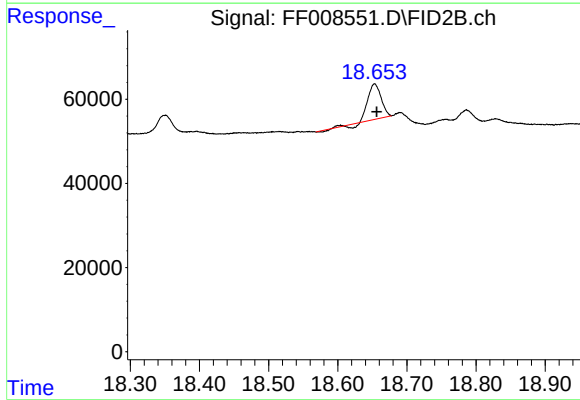

#14 N-DOTRIACONTANE

R.T.: 18.653 min
Delta R.T.: -0.003 min
Response: 105202
Conc: 0.87 ug/ml