

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
 Data File : FF008554.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jun 2021 15:43
 Operator : DD\AJ
 Sample : M2612-13
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 08 01:31:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.771	2133112	20.245 ug/ml
Target Compounds			
4) N-TETRADECANE	8.298	115061	0.904 ug/ml
14) N-DOTRIACONTANE	18.653	177314	1.473 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
Data File : FF008554.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2021 15:43
Operator : DD\AJ
Sample : M2612-13
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:31:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

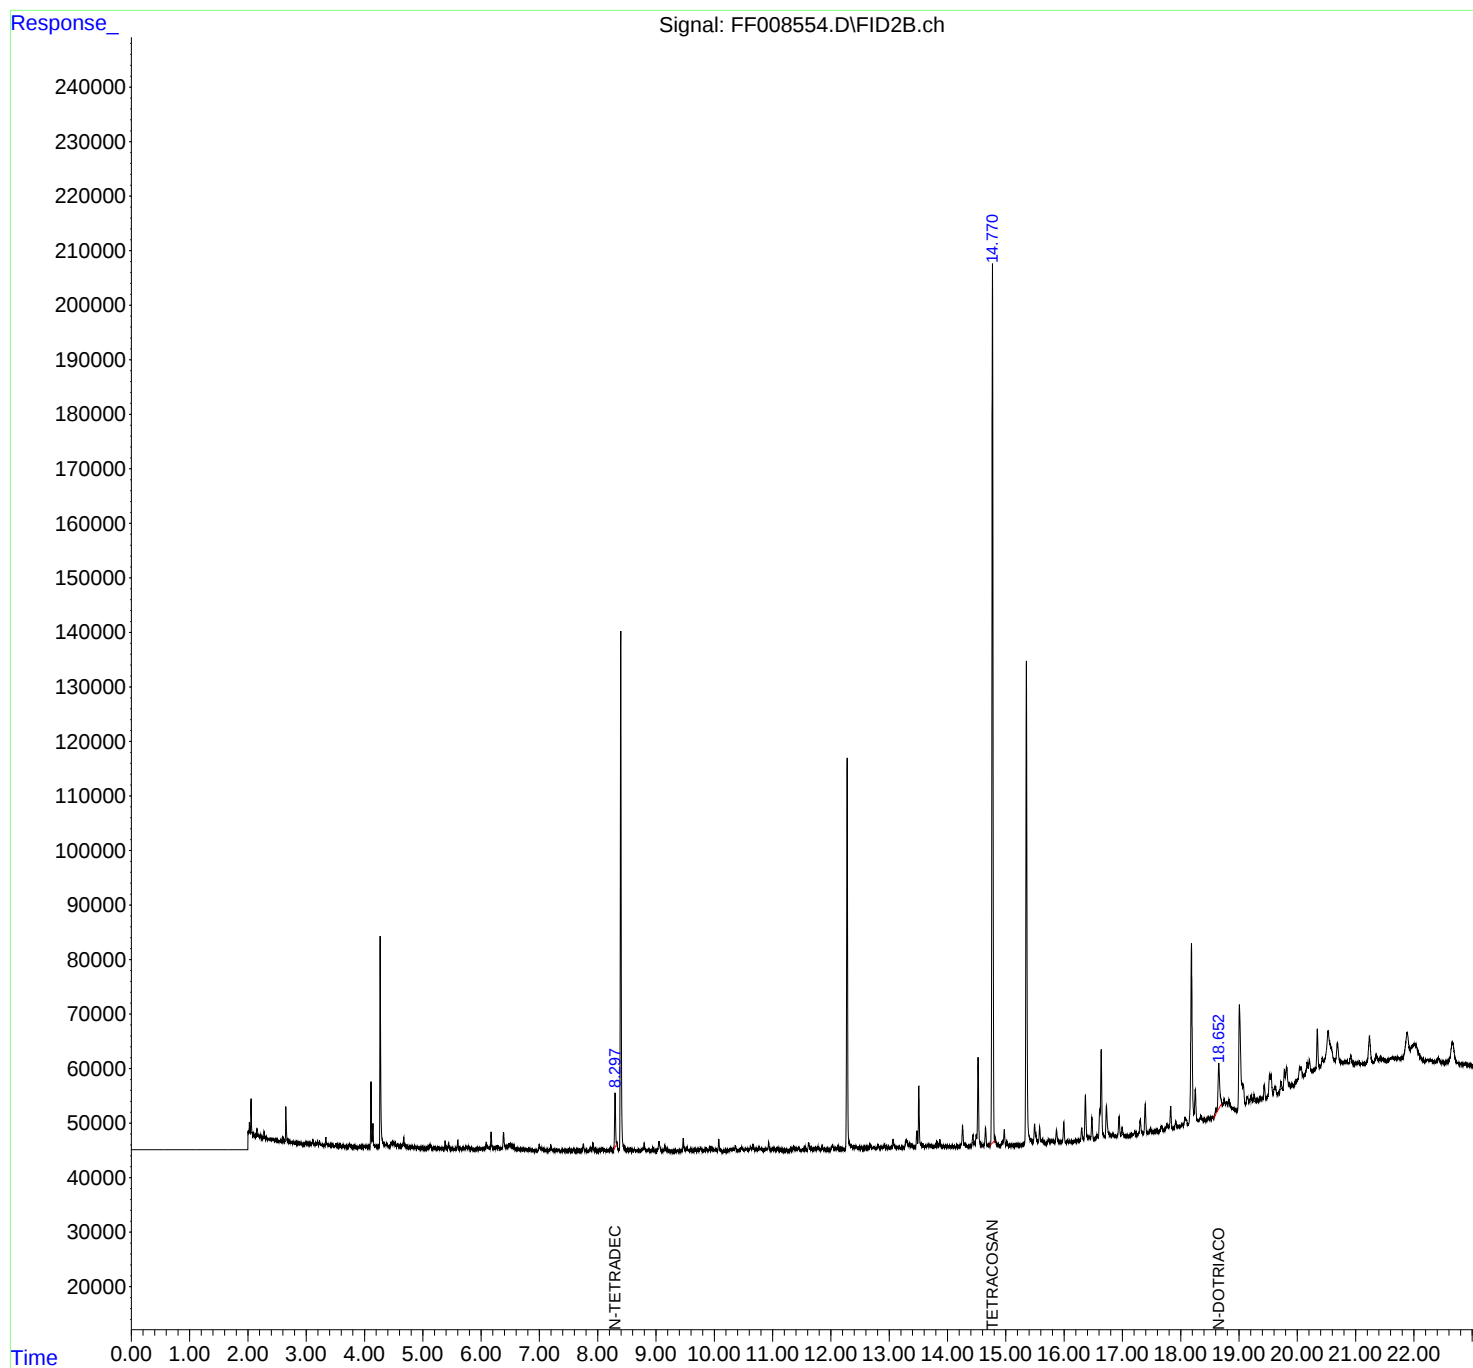


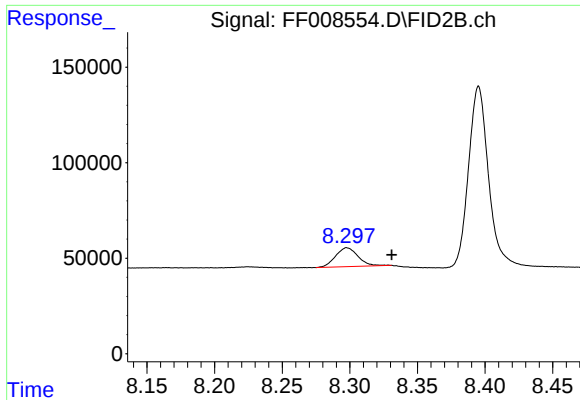

#4 N-TETRADECANE


R.T.: 8.298 min
Delta R.T.: -0.033 min
Response: 115061
Conc: 0.90 ug/ml

Instrument :
FID_F
ClientSampleId :

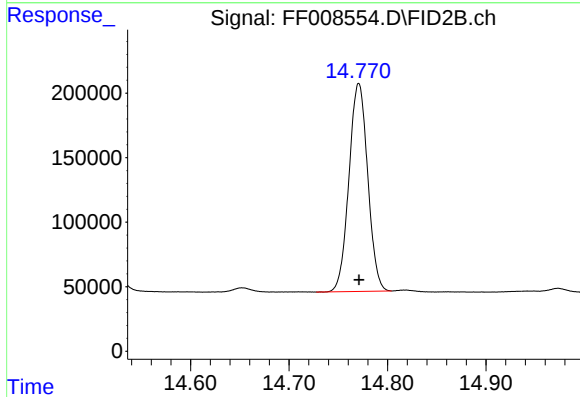

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.771 min
Delta R.T.: 0.000 min
Response: 2133112
Conc: 20.24 ug/ml

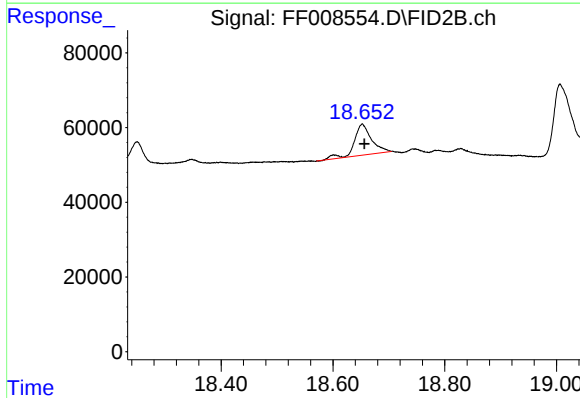

#14 N-DOTRIACONTANE

R.T.: 18.653 min
Delta R.T.: -0.004 min
Response: 177314
Conc: 1.47 ug/ml