

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
 Data File : FF008557.D
 Signal(s) : FID2B.ch
 Acq On : 07 Jun 2021 18:48
 Operator : DD\AJ
 Sample : M2612-01 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 08 01:31:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.770	414345	3.932 ug/ml
Target Compounds			
4) N-TETRADECANE	8.394f	132128	1.038 ug/ml
10) N-TETRACOSANE	14.967	204309	1.667 ug/ml
14) N-DOTRIACONTANE	18.660	146147	1.214 ug/ml
16) N-HEXATRIACONTANE	20.205	250048	2.255 ug/ml
18) N-TETRACONTANE	21.883	318599	3.016 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060721\
Data File : FF008557.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2021 18:48
Operator : DD\AJ
Sample : M2612-01 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:31:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

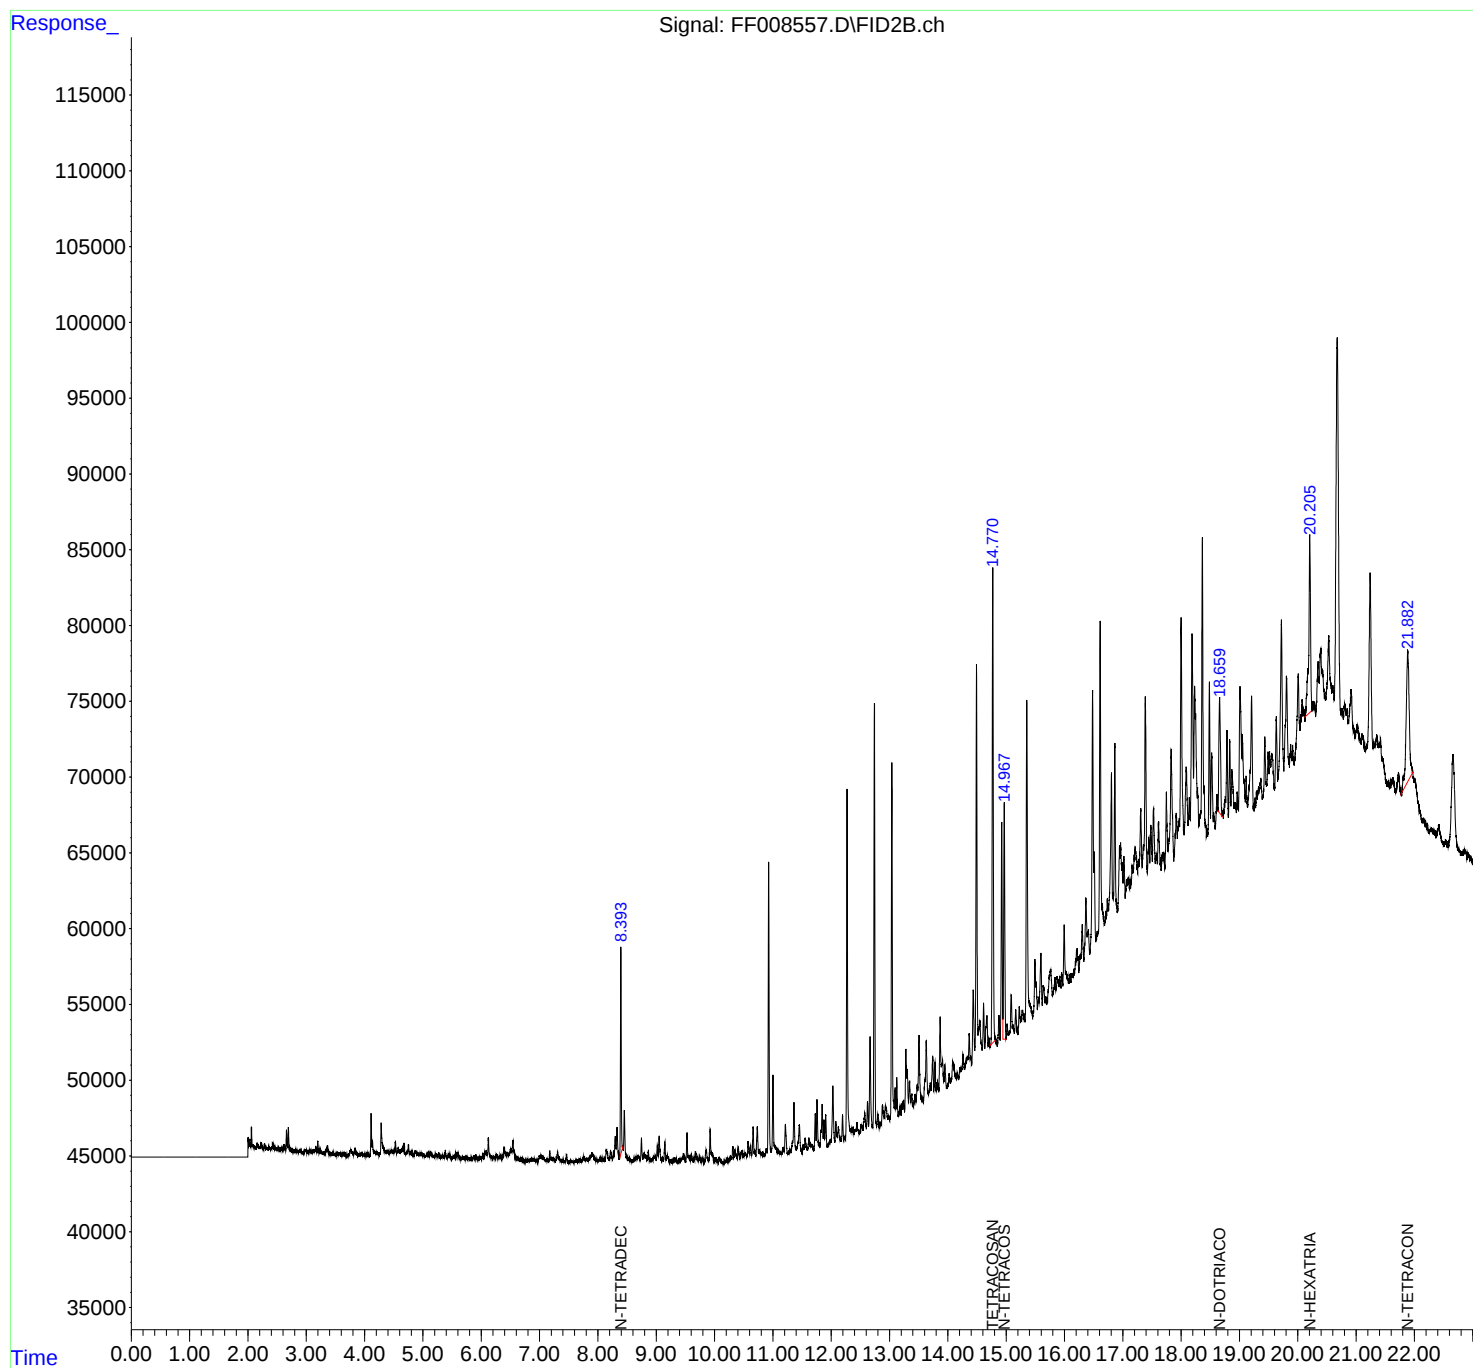


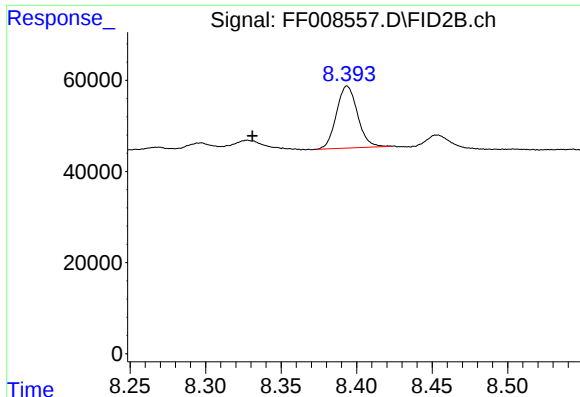

#4 N-TETRADECANE


R.T.: 8.394 min
Delta R.T.: 0.063 min
Response: 132128
Conc: 1.04 ug/ml

Instrument :
FID_F
ClientSampleId :

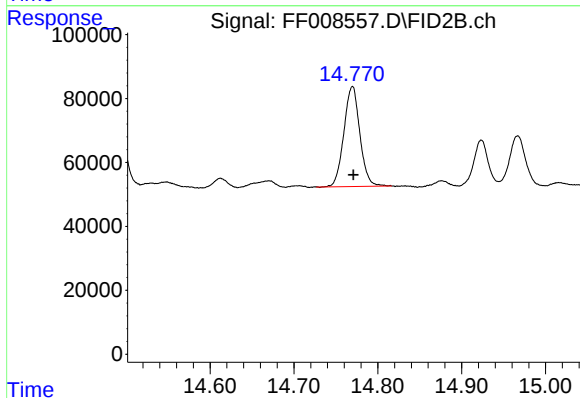


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.770 min
Delta R.T.: 0.000 min
Response: 414345
Conc: 3.93 ug/ml

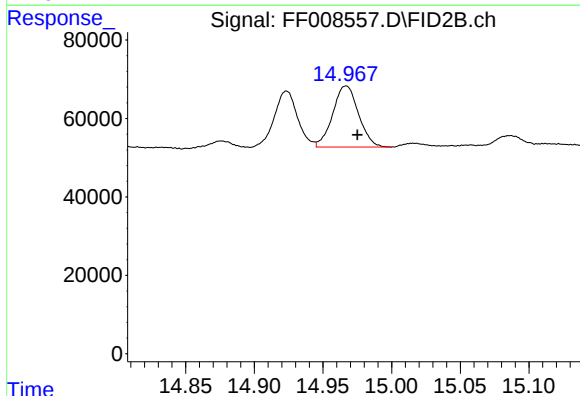


#10 N-TETRACOSANE

R.T.: 14.967 min
Delta R.T.: -0.008 min
Response: 204309
Conc: 1.67 ug/ml

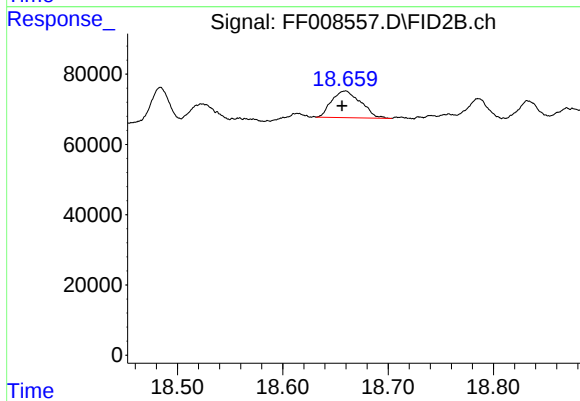

#14 N-DOTRIACONTANE


R.T.: 18.660 min
Delta R.T.: 0.003 min
Response: 146147
Conc: 1.21 ug/ml

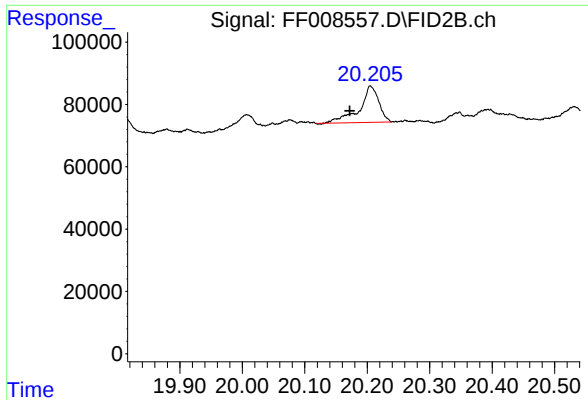

#16 N-HEXATRIACONTANE

R.T.: 20.205 min
Delta R.T.: 0.033 min
Response: 250048
Conc: 2.26 ug/ml

Instrument :
FID_F
ClientSampleId :

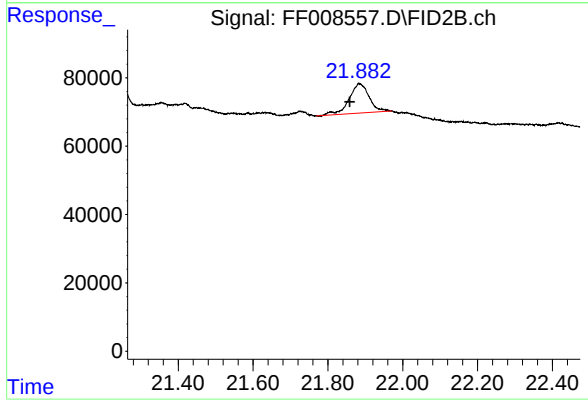

#18 N-TETRACONTANE

R.T.: 21.883 min
Delta R.T.: 0.024 min
Response: 318599
Conc: 3.02 ug/ml