

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060722\
Data File : FF010706.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2022 09:53
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:33:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
11)	N-HEXACOSANE	16.071	559162	4.414 ug/ml
13)	N-TRIACONTANE	17.874	157308	1.284 ug/ml
14)	N-DOTRIACONTANE	18.711	510521	4.207 ug/ml
15)	N-TETRATRIACONTANE	19.487	115050	1.107 ug/ml
16)	N-HEXATRIACONTANE	20.224	159866	1.859 ug/ml
18)	N-TETRACONTANE	21.802	159157	2.037 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060722\
Data File : FF010706.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2022 09:53
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:33:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

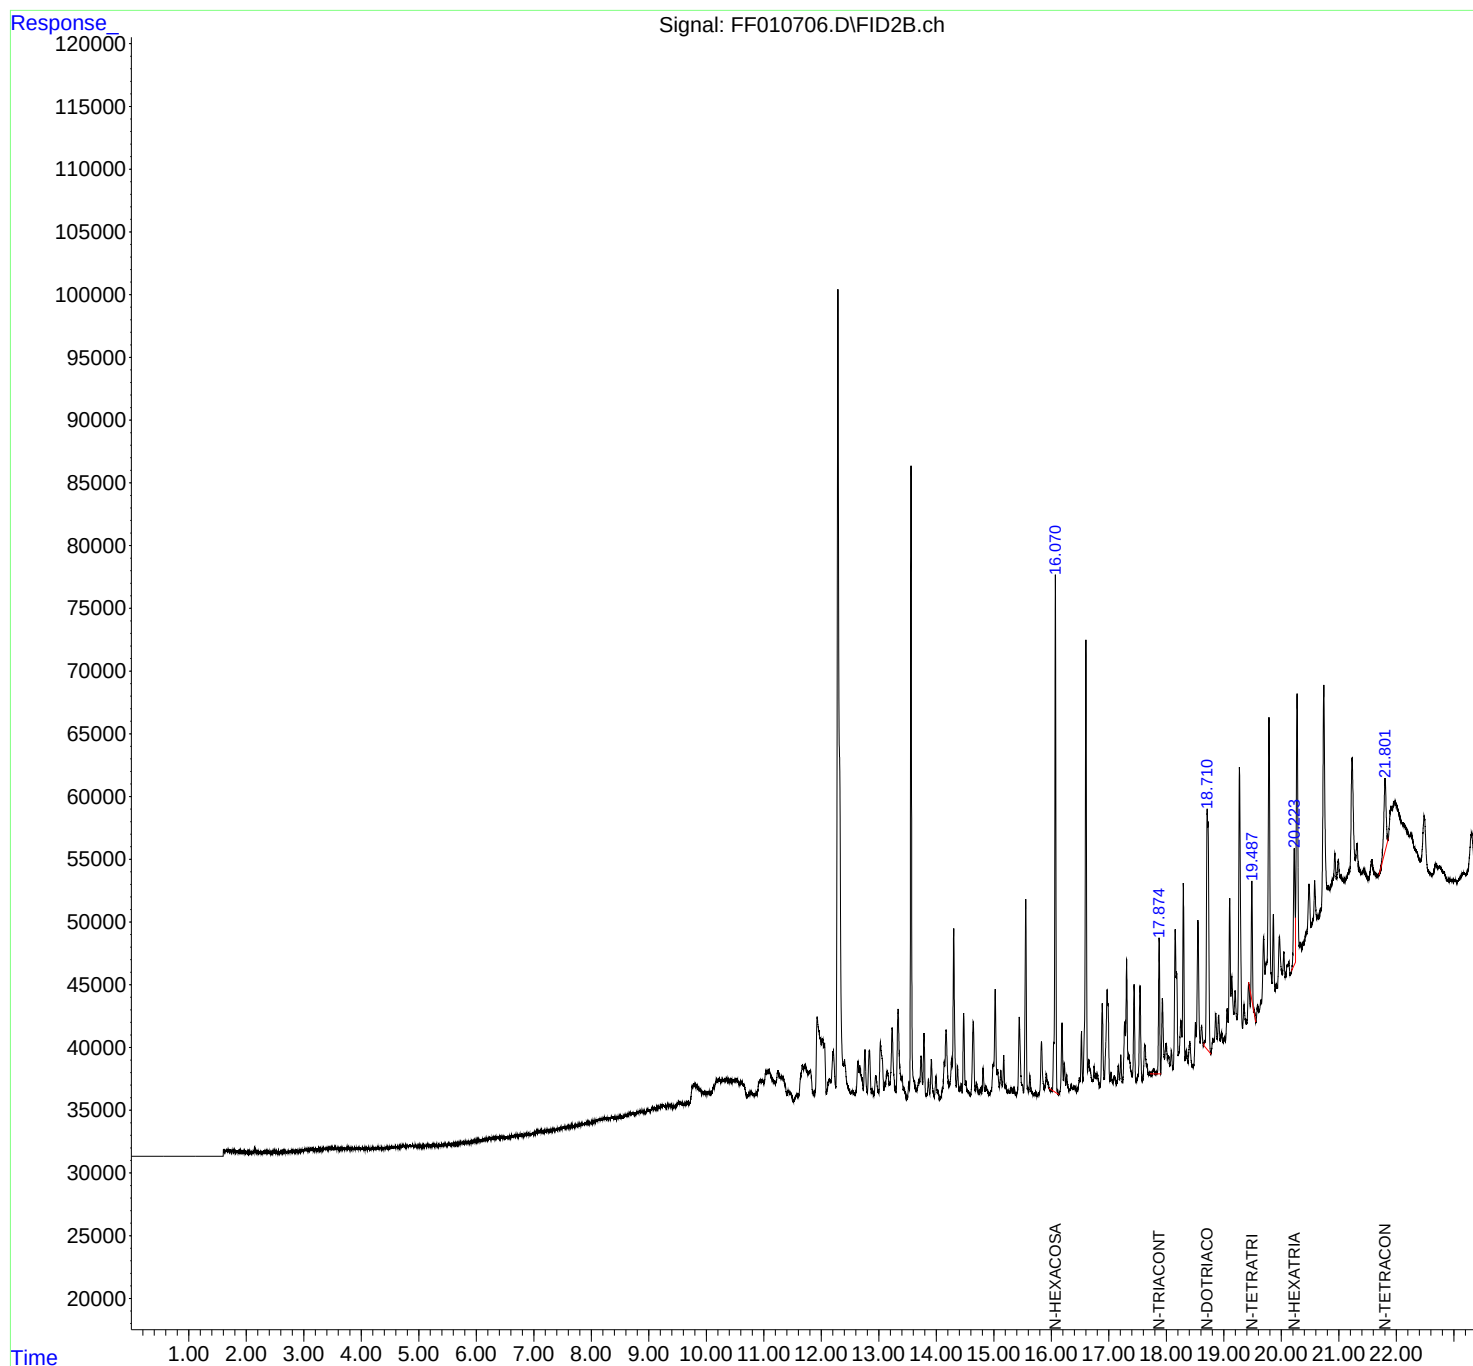


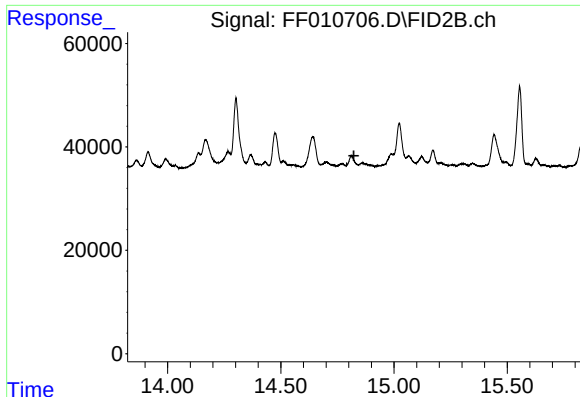

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.823 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

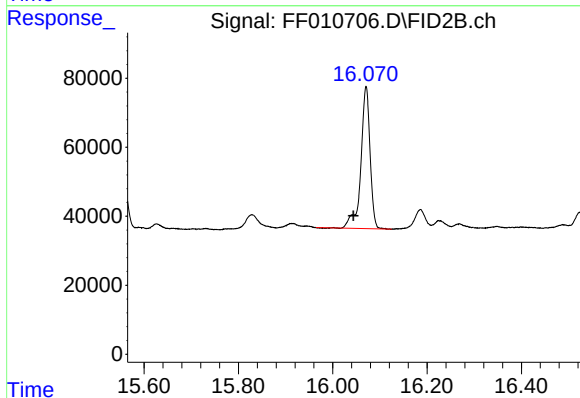


#11 N-HEXACOSANE

R.T.: 16.071 min
Delta R.T.: 0.027 min
Response: 559162
Conc: 4.41 ug/ml

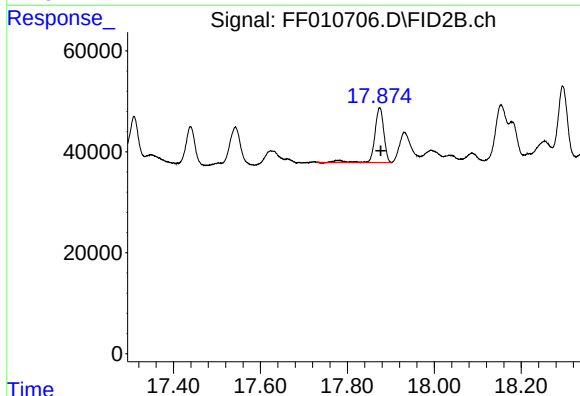


#13 N-TRIACONTANE

R.T.: 17.874 min
Delta R.T.: -0.002 min
Response: 157308
Conc: 1.28 ug/ml

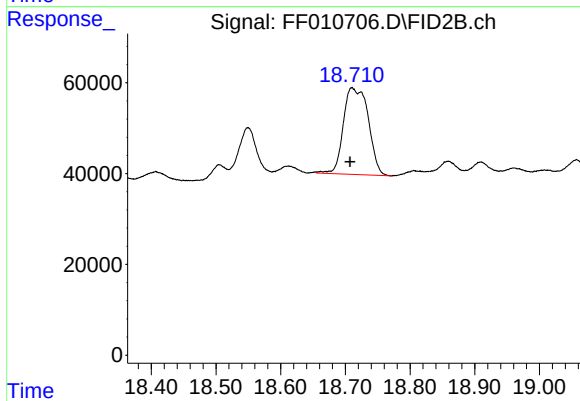

#14 N-DOTRIACONTANE


R.T.: 18.711 min
Delta R.T.: 0.003 min
Response: 510521
Conc: 4.21 ug/ml

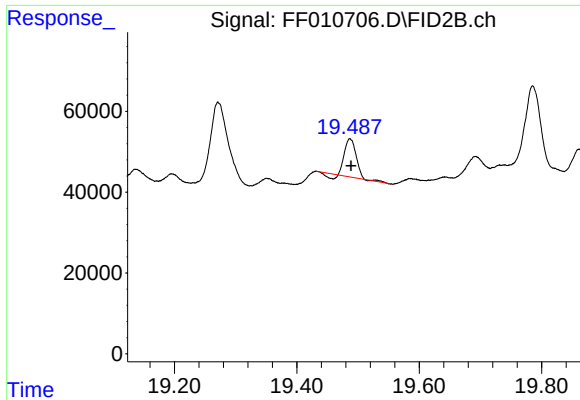

#15 N-TETRATRIACONTANE


R.T.: 19.487 min
Delta R.T.: -0.002 min
Response: 115050
Conc: 1.11 ug/ml

Instrument :
FID_F
ClientSampleId :

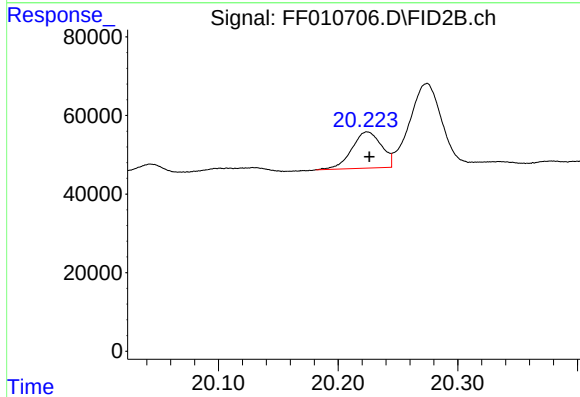

#16 N-HEXATRIACONTANE

R.T.: 20.224 min
Delta R.T.: -0.002 min
Response: 159866
Conc: 1.86 ug/ml

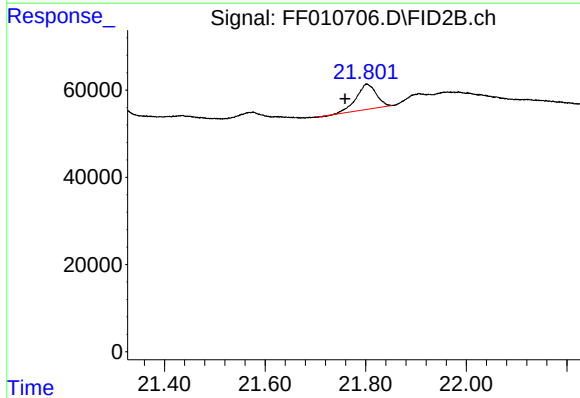

#18 N-TETRACONTANE

R.T.: 21.802 min
Delta R.T.: 0.043 min
Response: 159157
Conc: 2.04 ug/ml