

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060722\
Data File : FF010714.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2022 17:24
Operator : AJ\MA
Sample : N3194-08
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:35:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.823	2010302	17.785 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.706	93397	0.770 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060722\
Data File : FF010714.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2022 17:24
Operator : AJ\MA
Sample : N3194-08
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:35:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

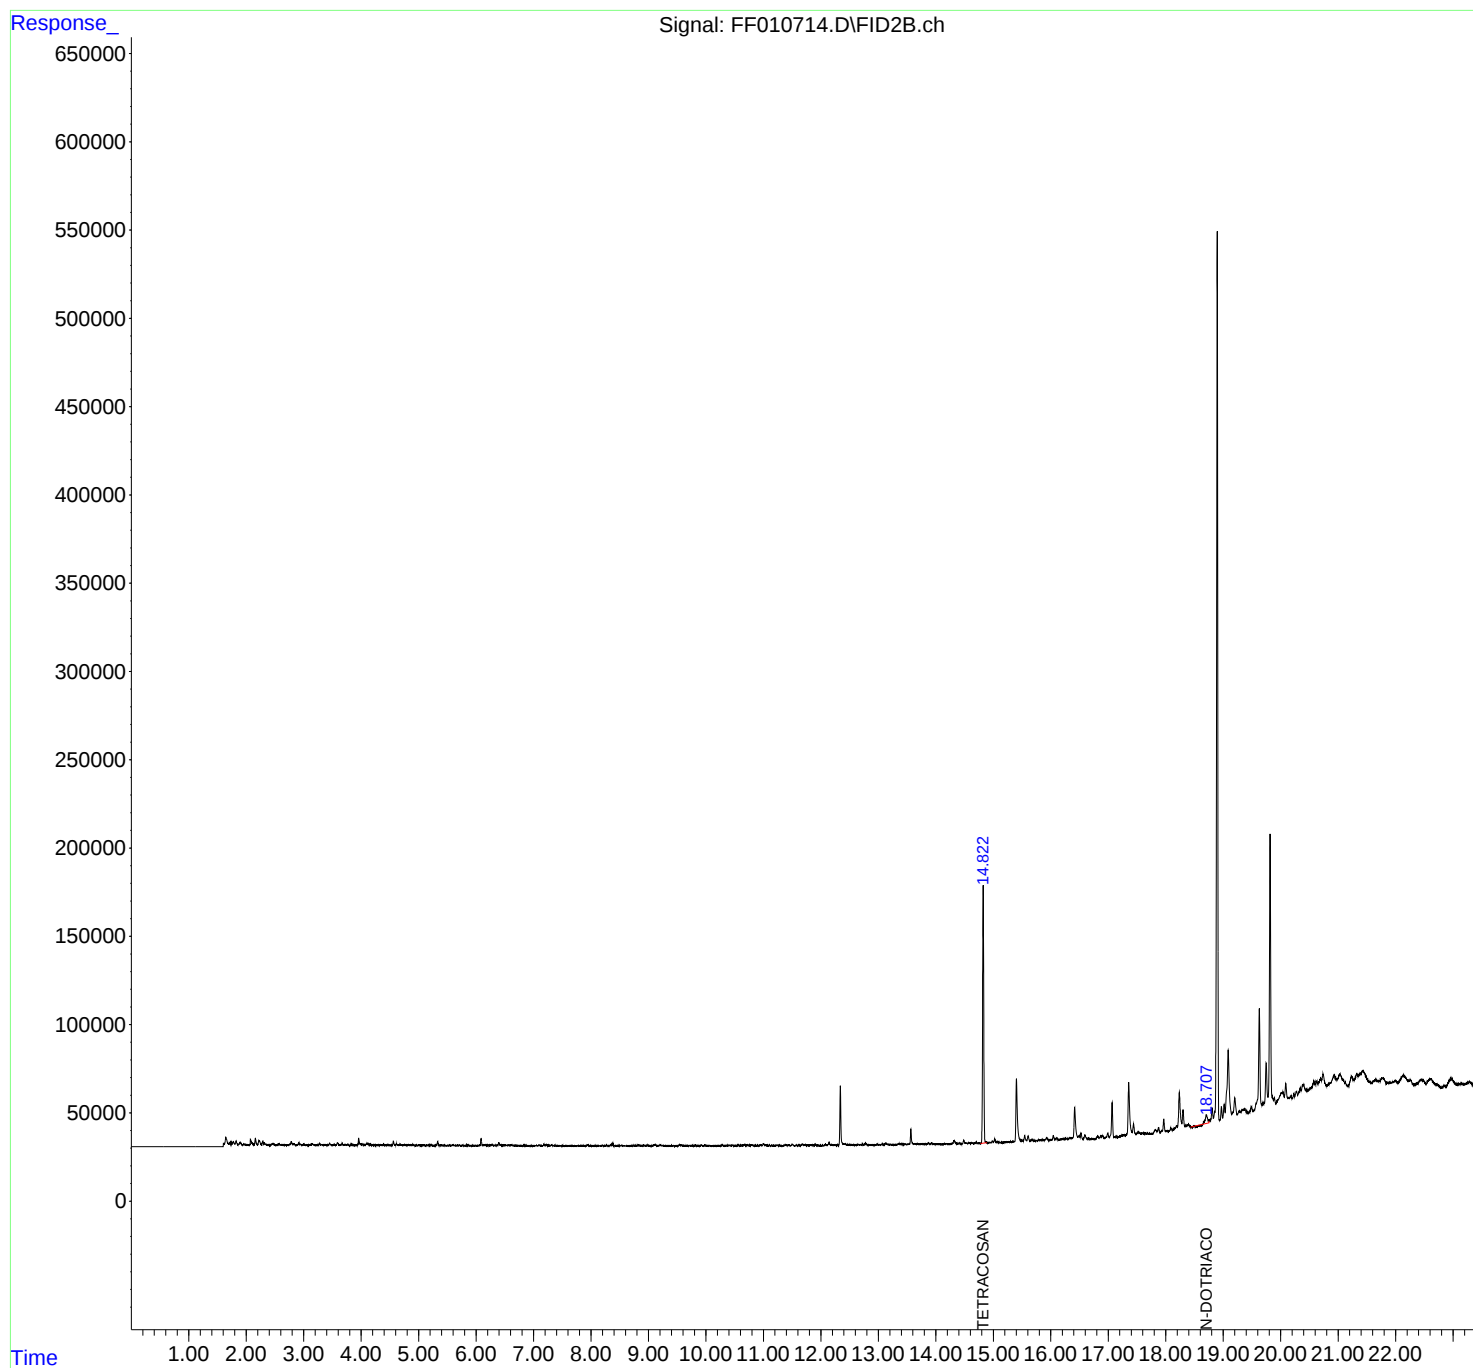


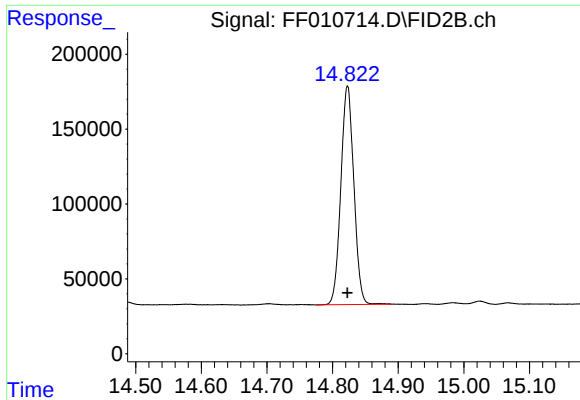

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.823 min
Delta R.T.: 0.000 min
Response: 2010302
Conc: 17.78 ug/ml

Instrument :
FID_F
ClientSampleId :

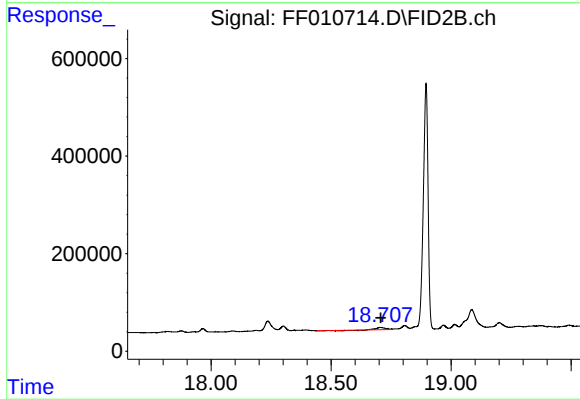

#14 N-DOTRIACONTANE

R.T.: 18.706 min
Delta R.T.: -0.001 min
Response: 93397
Conc: 0.77 ug/ml