

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060722\
Data File : FF010719.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2022 19:51
Operator : AJ\MA
Sample : N3194-13
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:36:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.823	1429483	12.646 ug/ml
Target Compounds			
1) N-OCTANE	1.895	219677	1.880 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060722\
Data File : FF010719.D
Signal(s) : FID2B.ch
Acq On : 07 Jun 2022 19:51
Operator : AJ\MA
Sample : N3194-13
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:36:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

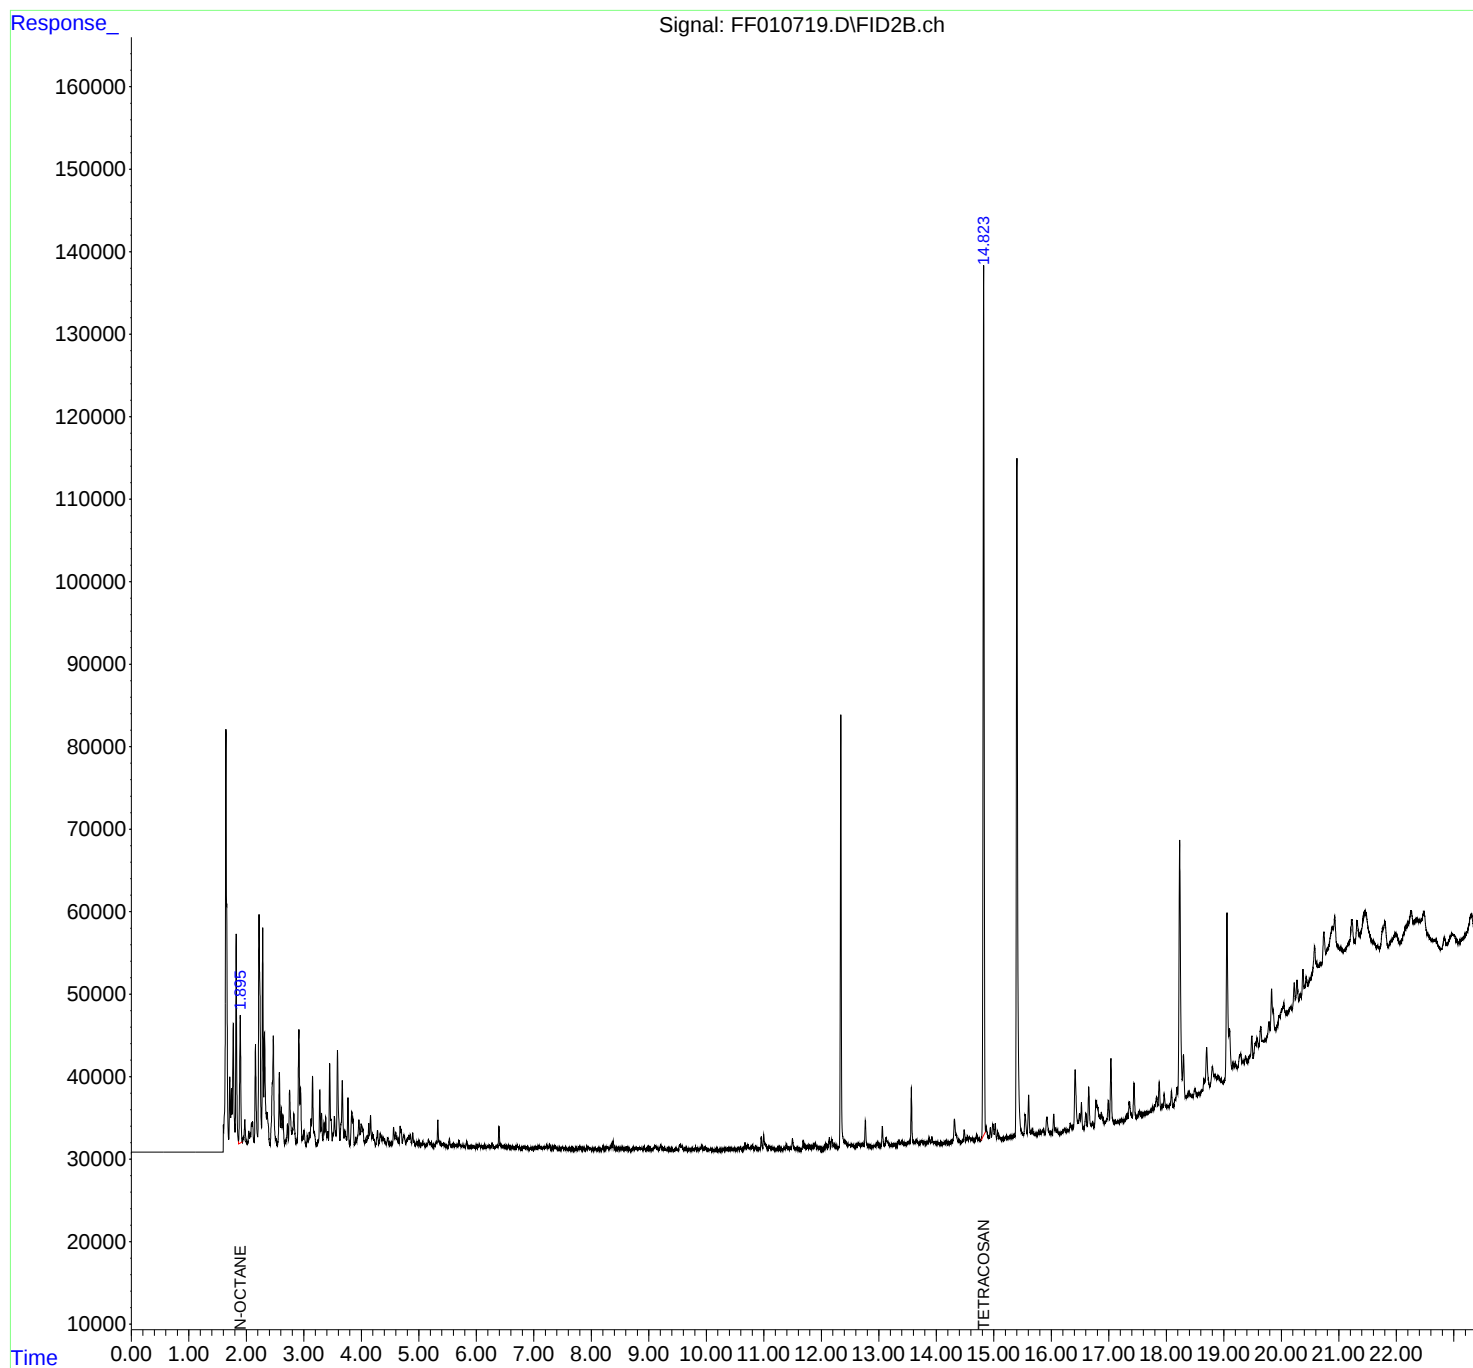


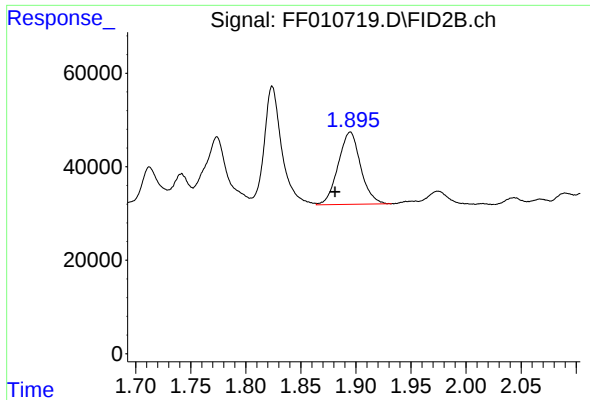

#1 N-OCTANE

R.T.: 1.895 min
Delta R.T.: 0.014 min
Response: 219677
Conc: 1.88 ug/ml

Instrument :
FID_F
ClientSampleId :

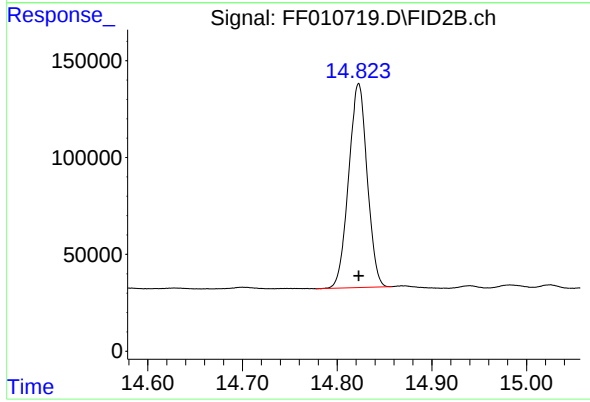

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.823 min
Delta R.T.: 0.000 min
Response: 1429483
Conc: 12.65 ug/ml