

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060822\
 Data File : FF010730.D
 Signal(s) : FID2B.ch
 Acq On : 08 Jun 2022 09:39
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 08 14:05:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.824	2695656	23.848 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.708	122318	1.008 ug/ml
16) N-HEXATRIACONTANE	20.276	93098	1.083 ug/ml
18) N-TETRACONTANE	21.800	247286	3.165 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060822\
Data File : FF010730.D
Signal(s) : FID2B.ch
Acq On : 08 Jun 2022 09:39
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 14:05:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

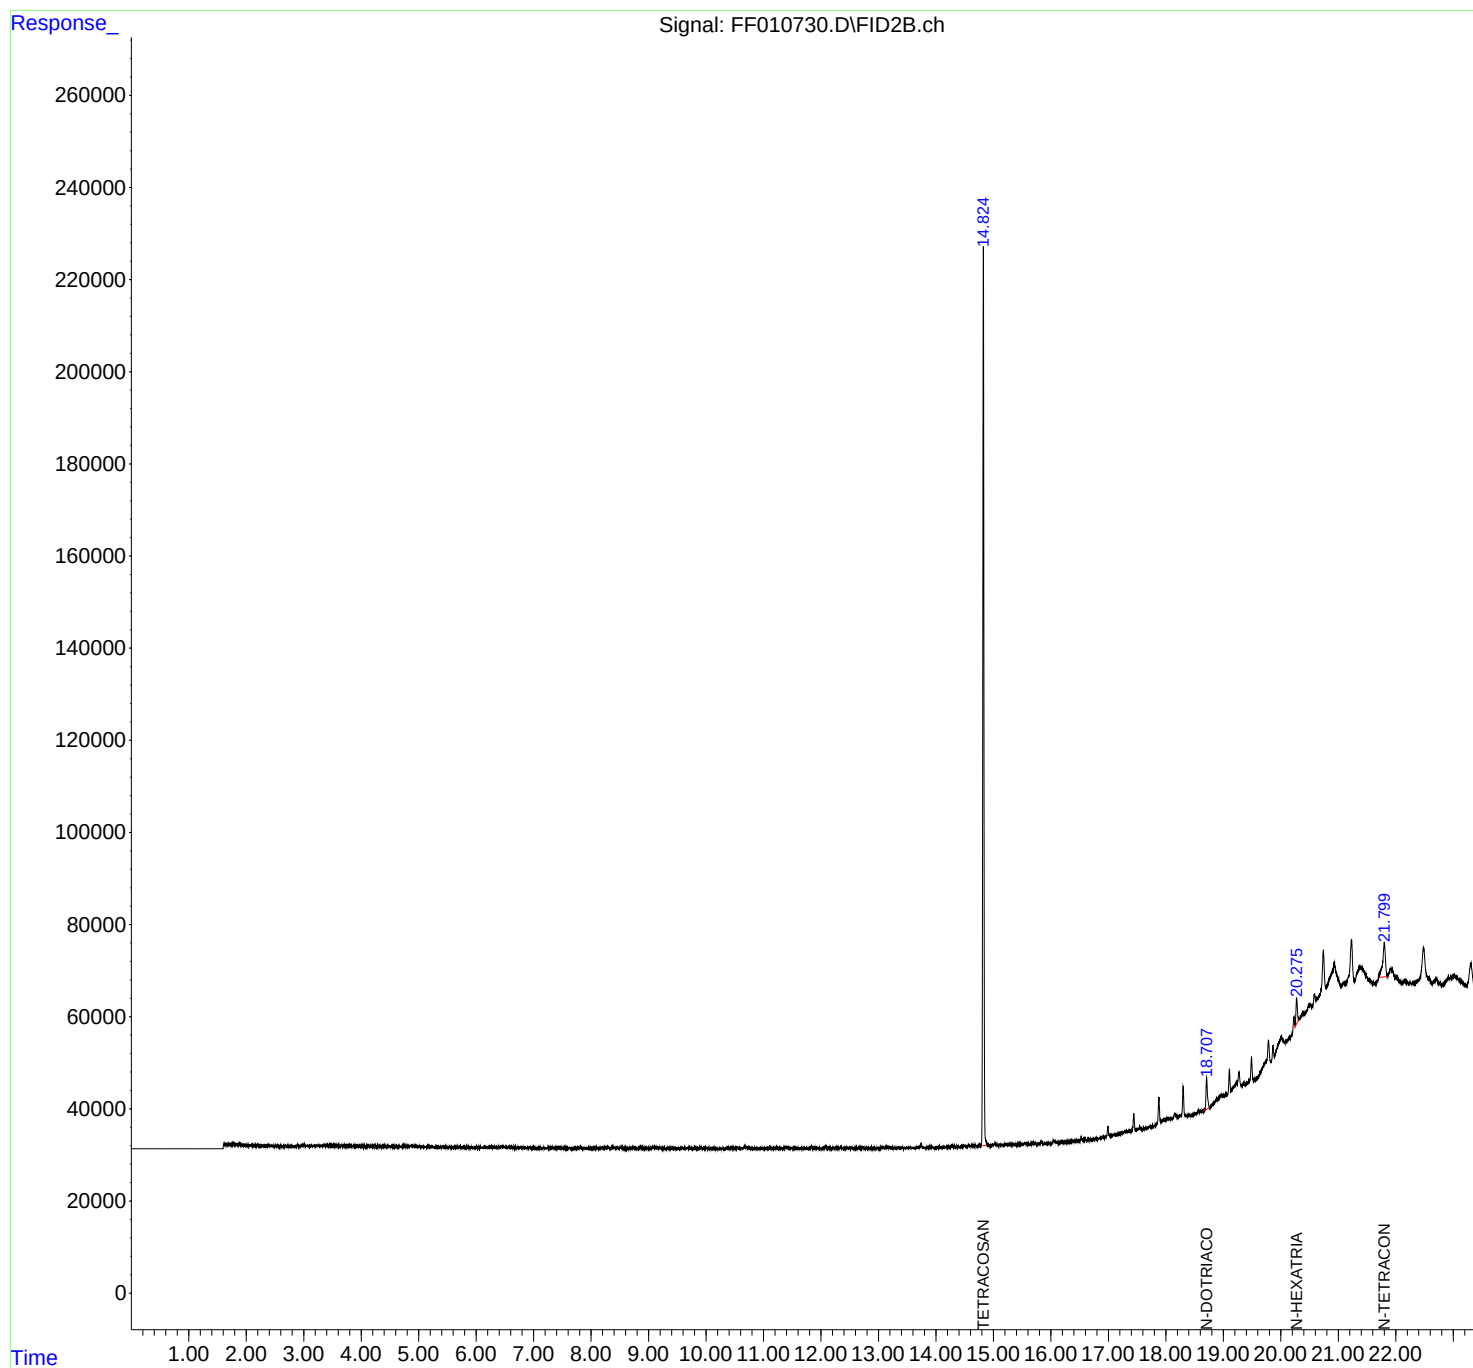


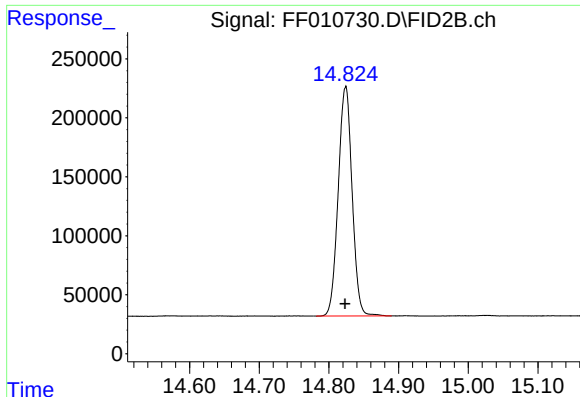

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.824 min
Delta R.T.: 0.000 min
Response: 2695656
Conc: 23.85 ug/ml

Instrument :
FID_F
ClientSampleId :

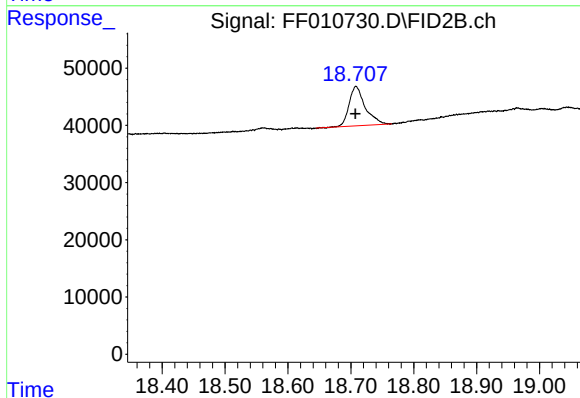


#14 N-DOTRIACONTANE

R.T.: 18.708 min
Delta R.T.: 0.000 min
Response: 122318
Conc: 1.01 ug/ml

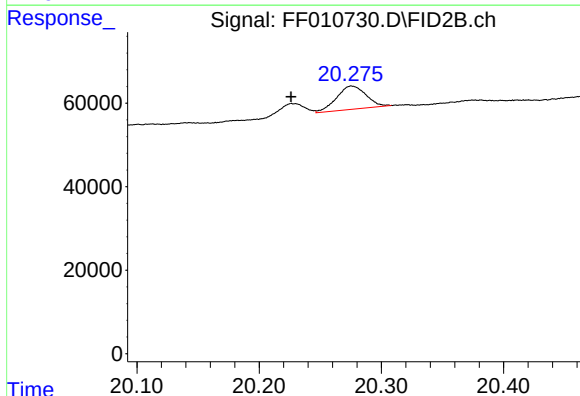

#16 N-HEXATRIACONTANE

R.T.: 20.276 min
Delta R.T.: 0.050 min
Response: 93098
Conc: 1.08 ug/ml

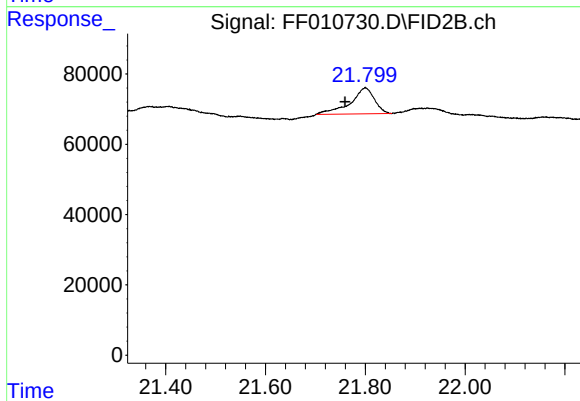

#18 N-TETRACONTANE

R.T.: 21.800 min
Delta R.T.: 0.041 min
Response: 247286
Conc: 3.16 ug/ml