

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060822\
Data File : FF010732.D
Signal(s) : FID2B.ch
Acq On : 08 Jun 2022 11:09
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 14:05:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.557	2880426	23.702 ug/ml
12)	N-OCTACOSANE	16.993	2873385	23.545 ug/ml
13)	N-TRIACONTANE	17.877	146540	1.196 ug/ml
14)	N-DOTRIACONTANE	18.707	203516	1.677 ug/ml
15)	N-TETRATRIACONTANE	19.487	140014	1.347 ug/ml
16)	N-HEXATRIACONTANE	20.227	72202	0.840 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060822\
Data File : FF010732.D
Signal(s) : FID2B.ch
Acq On : 08 Jun 2022 11:09
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 14:05:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

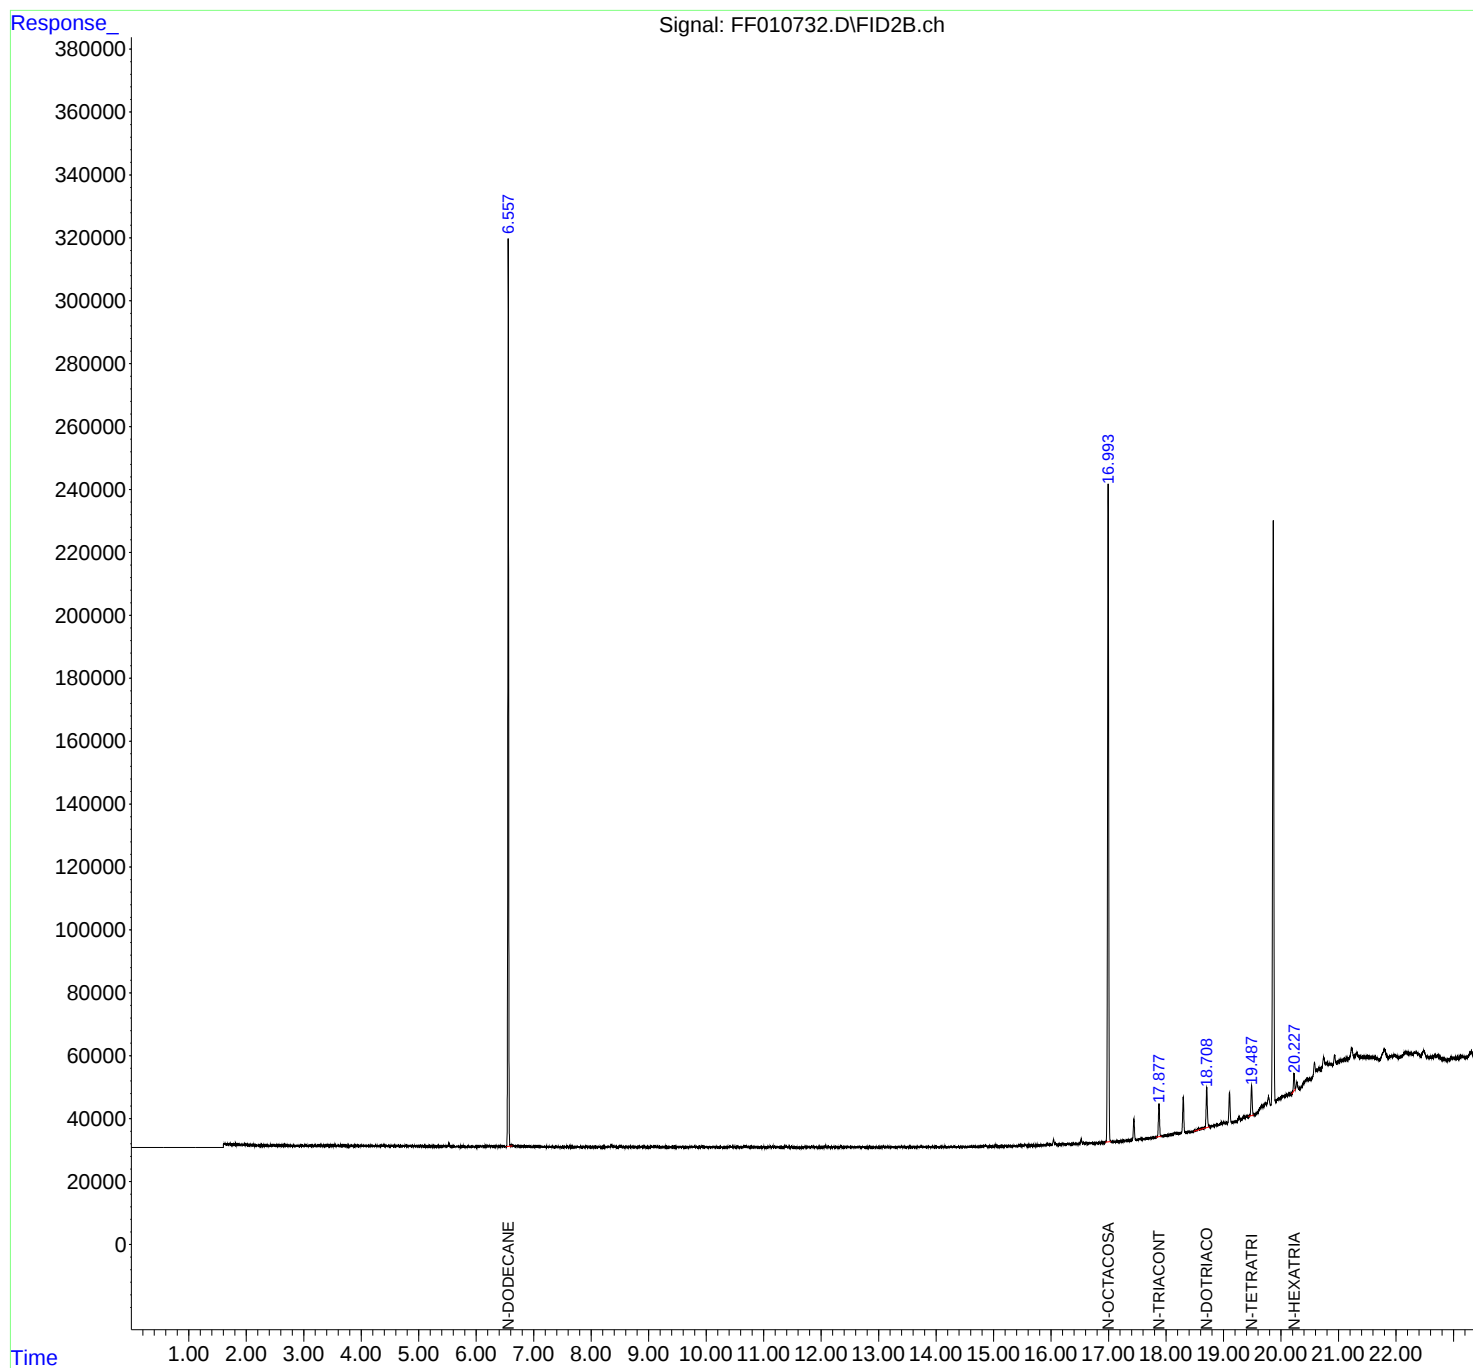


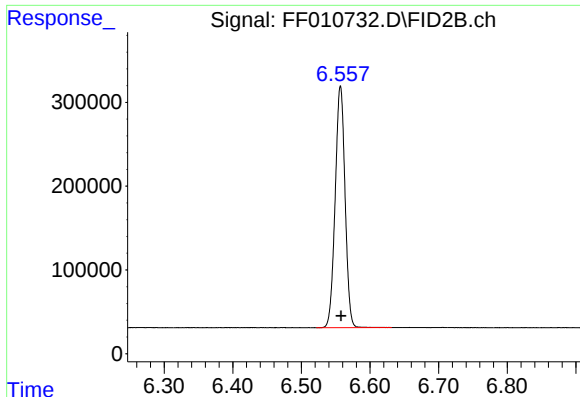

#3 N-DODECANE


R.T.: 6.557 min
Delta R.T.: 0.000 min
Response: 2880426
Conc: 23.70 ug/ml

Instrument :
FID_F
ClientSampleId :

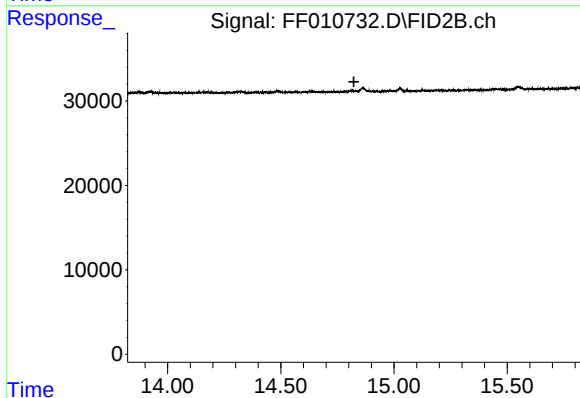


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.823 min
Response: 0
Conc: N.D.

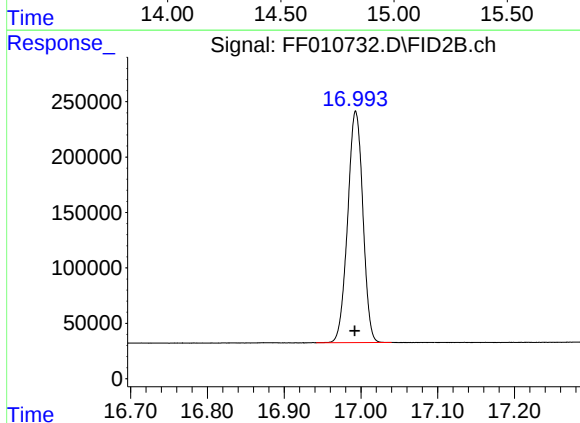


#12 N-OCTACOSANE

R.T.: 16.993 min
Delta R.T.: 0.001 min
Response: 2873385
Conc: 23.54 ug/ml

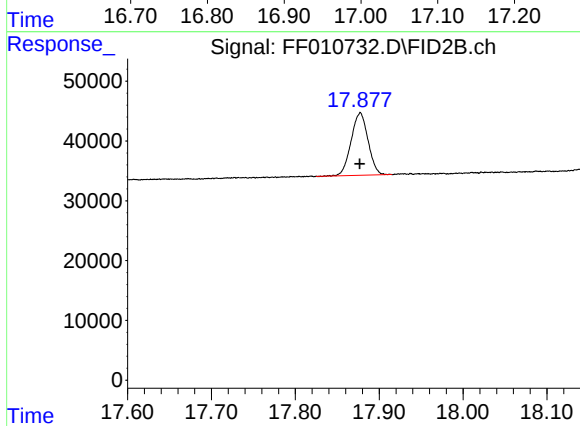

#13 N-TRIACONTANE


R.T.: 17.877 min
Delta R.T.: 0.000 min
Response: 146540
Conc: 1.20 ug/ml

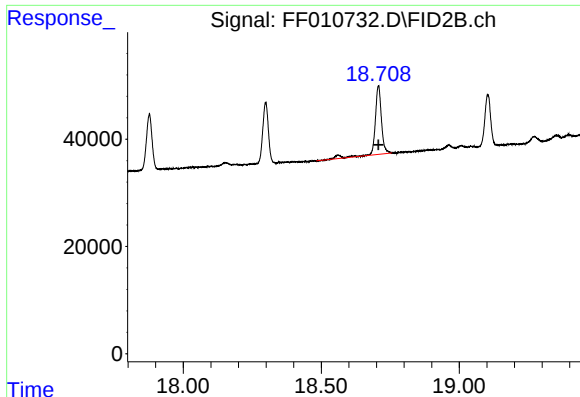

#14 N-DOTRIACONTANE


R.T.: 18.707 min
Delta R.T.: 0.000 min
Response: 203516
Conc: 1.68 ug/ml

Instrument :
FID_F
ClientSampleId :

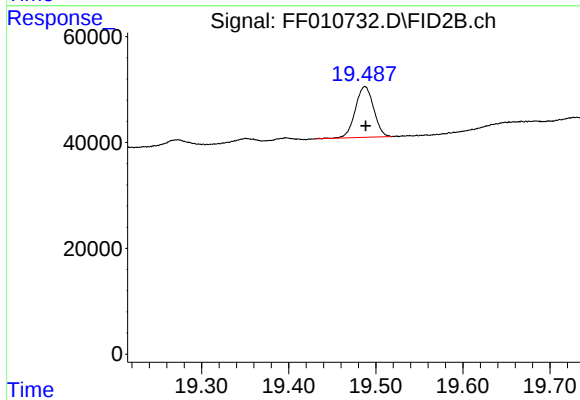

#15 N-TETRATRIACONTANE

R.T.: 19.487 min
Delta R.T.: -0.001 min
Response: 140014
Conc: 1.35 ug/ml

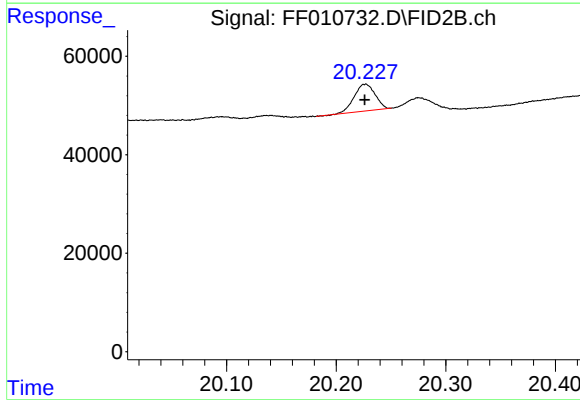

#16 N-HEXATRIACONTANE

R.T.: 20.227 min
Delta R.T.: 0.000 min
Response: 72202
Conc: 0.84 ug/ml