

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF060822\  
Data File : FF010733.D  
Signal(s) : FID2B.ch  
Acq On : 08 Jun 2022 11:49  
Operator : AJ\MA  
Sample : N3209-04 100X  
Misc :  
ALS Vial : 55 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 08 14:05:55 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060622.M  
Quant Title :  
QLast Update : Tue Jun 07 09:12:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------|----------|-------------|
| -----                       |        |          |             |
| System Monitoring Compounds |        |          |             |
| Target Compounds            |        |          |             |
| 3) N-DODECANE               | 6.570  | 253754   | 2.088 ug/ml |
| 4) N-TETRADECANE            | 8.347  | 405217   | 3.269 ug/ml |
| 5) N-HEXADECANE             | 9.933f | 259853   | 2.078 ug/ml |
| -----                       |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF060822\  
Data File : FF010733.D  
Signal(s) : FID2B.ch  
Acq On : 08 Jun 2022 11:49  
Operator : AJ\MA  
Sample : N3209-04 100X  
Misc :  
ALS Vial : 55 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 08 14:05:55 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060622.M  
Quant Title :  
QLast Update : Tue Jun 07 09:12:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

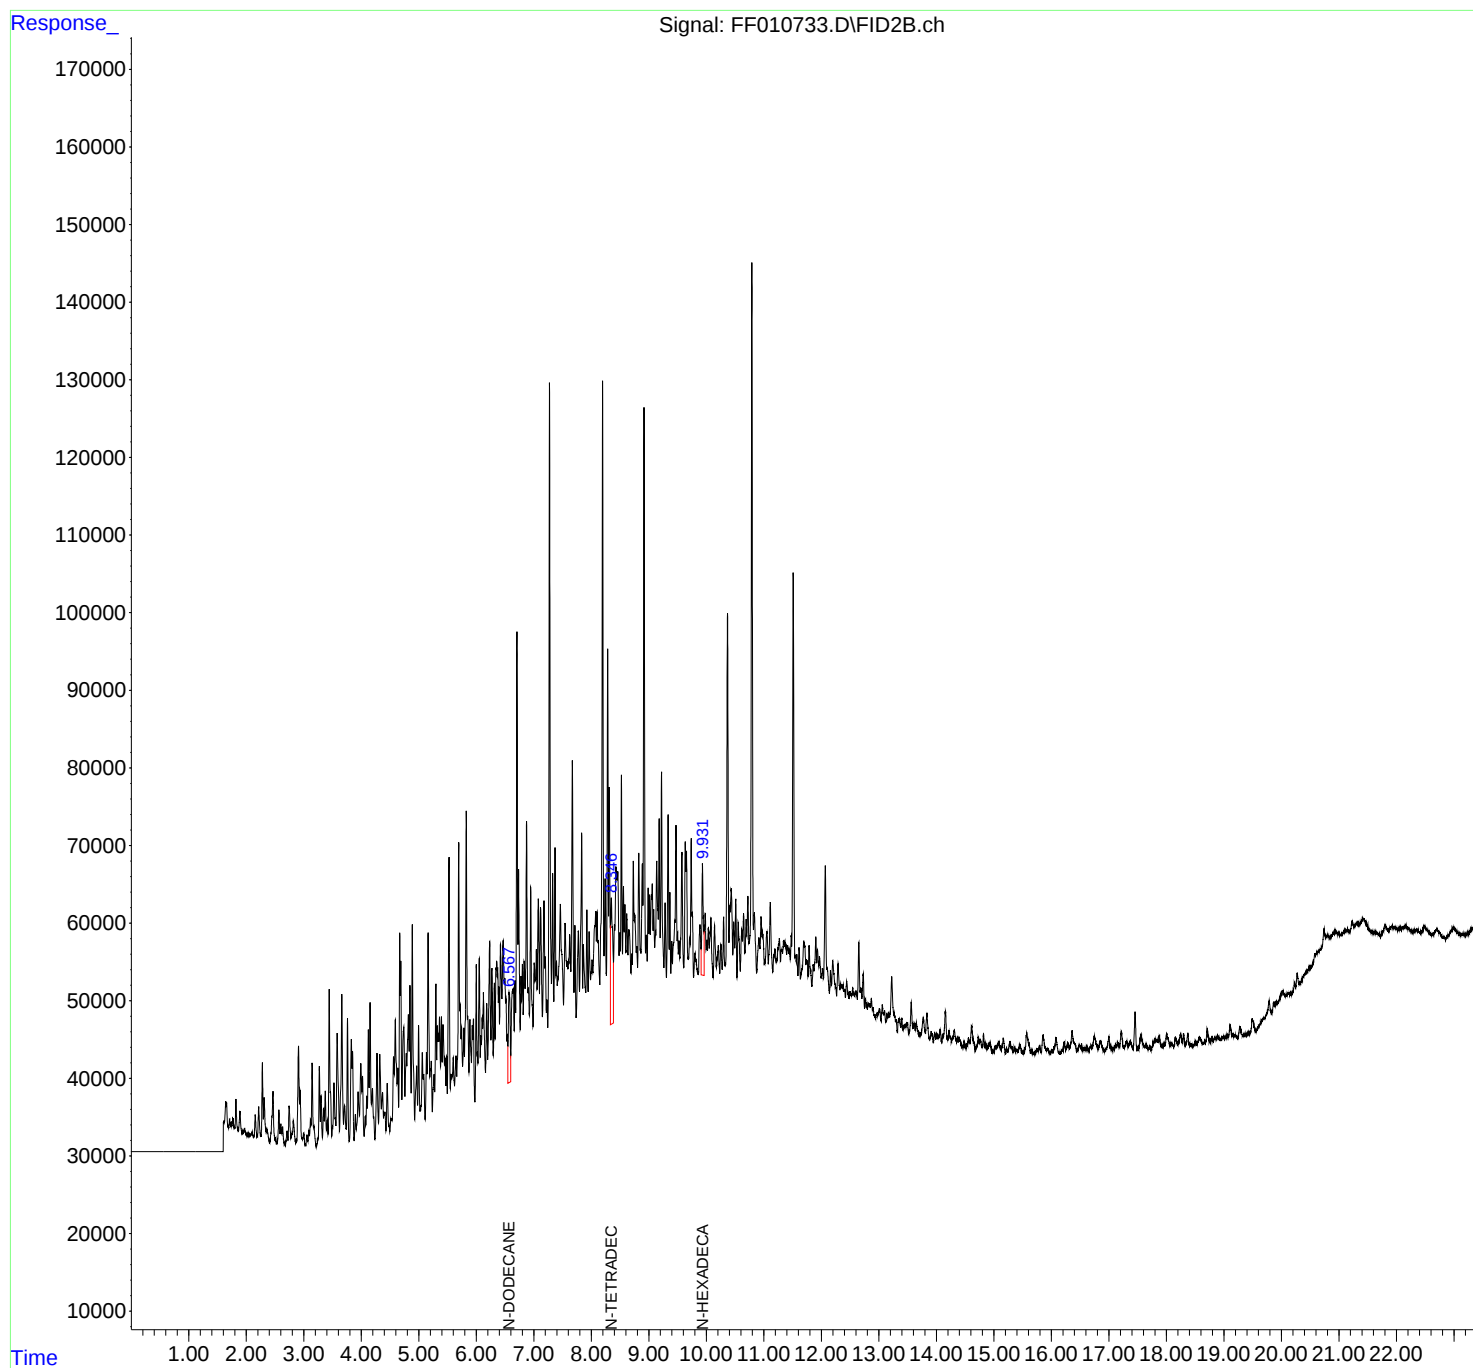


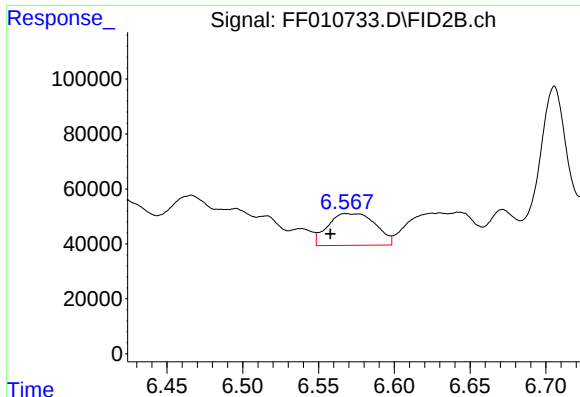

#3 N-DODECANE


R.T.: 6.570 min  
Delta R.T.: 0.012 min  
Response: 253754  
Conc: 2.09 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

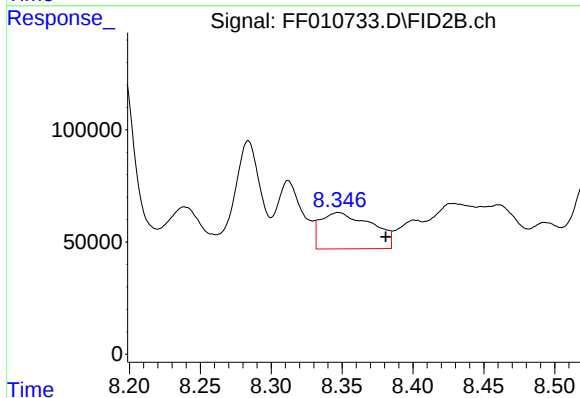


#4 N-TETRADECANE

R.T.: 8.347 min  
Delta R.T.: -0.033 min  
Response: 405217  
Conc: 3.27 ug/ml

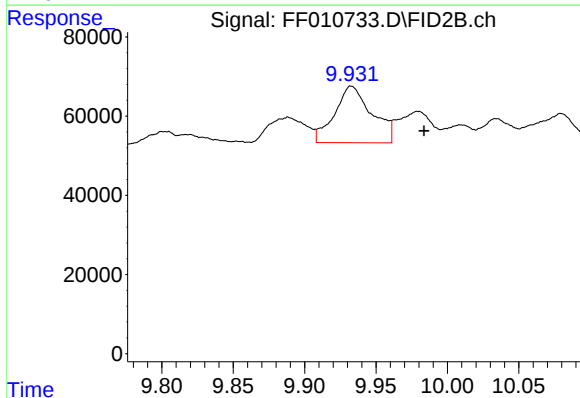

#5 N-HEXADECANE

R.T.: 9.933 min  
Delta R.T.: -0.051 min  
Response: 259853  
Conc: 2.08 ug/ml

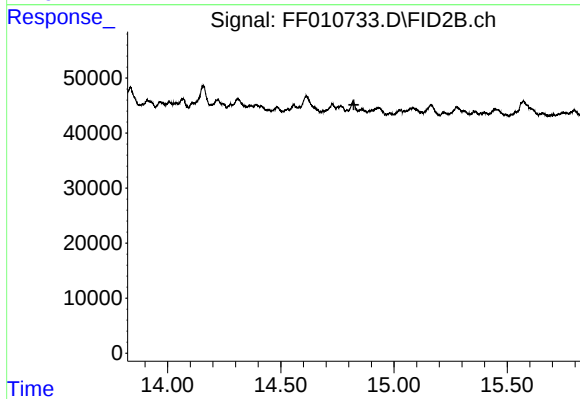

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.823 min  
Response: 0  
Conc: N.D.