

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060822\
 Data File : FF010736.D
 Signal(s) : FID2B.ch
 Acq On : 08 Jun 2022 13:17
 Operator : AJ\MA
 Sample : N3194-06RE
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 08 14:06:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.823	885840	7.837 ug/ml
Target Compounds			
7) N-EICOSANE	12.767	483697	3.825 ug/ml
8) N-DOCOSANE	13.927	86605	0.686 ug/ml
11) N-HEXACOSANE	16.074	193795	1.530 ug/ml
14) N-DOTRIACONTANE	18.708	167162	1.378 ug/ml
15) N-TETRATRIACONTANE	19.506	114835	1.105 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060822\
Data File : FF010736.D
Signal(s) : FID2B.ch
Acq On : 08 Jun 2022 13:17
Operator : AJ\MA
Sample : N3194-06RE
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 14:06:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

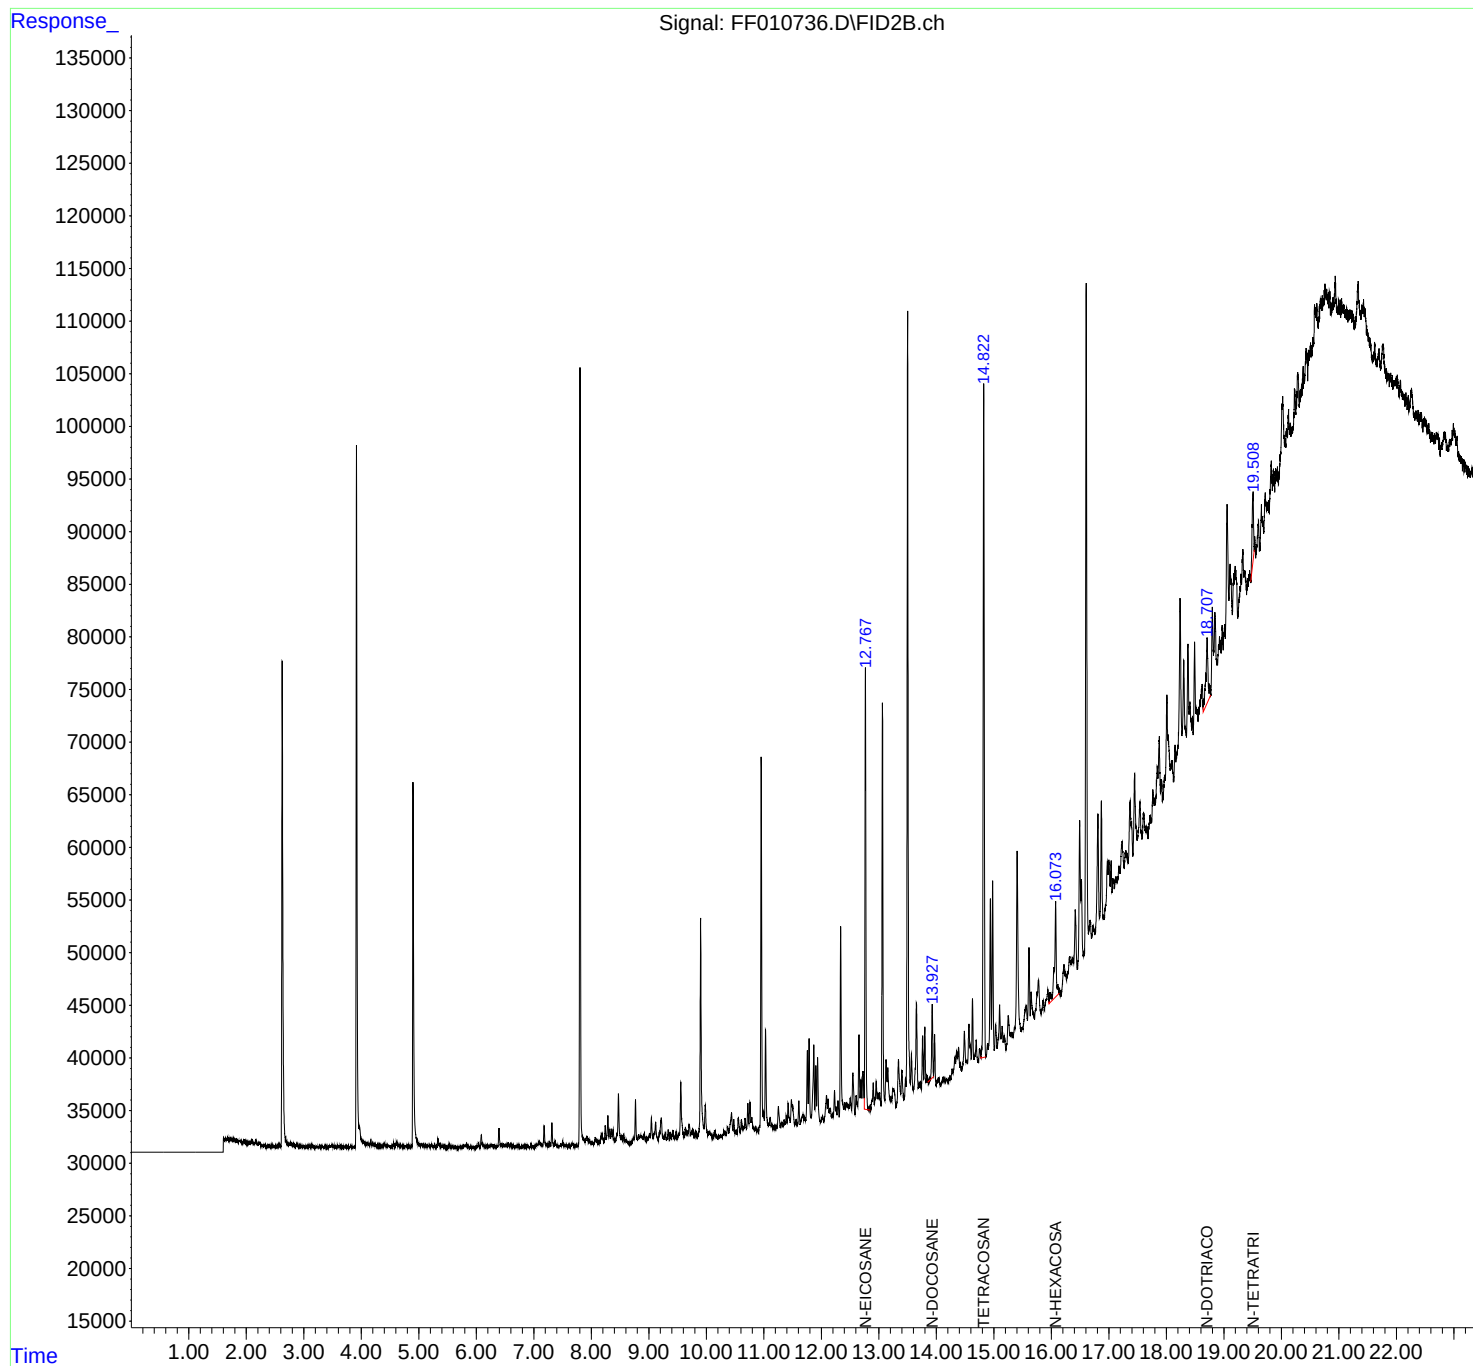


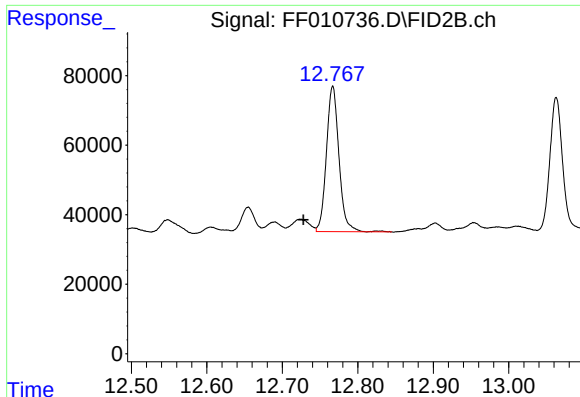

#7 N-EICOSANE


R.T.: 12.767 min
Delta R.T.: 0.039 min
Response: 483697
Conc: 3.82 ug/ml

Instrument :
FID_F
ClientSampleId :

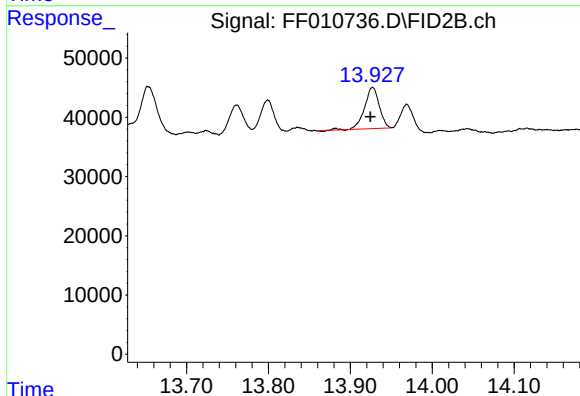


#8 N-DOCOSANE

R.T.: 13.927 min
Delta R.T.: 0.003 min
Response: 86605
Conc: 0.69 ug/ml

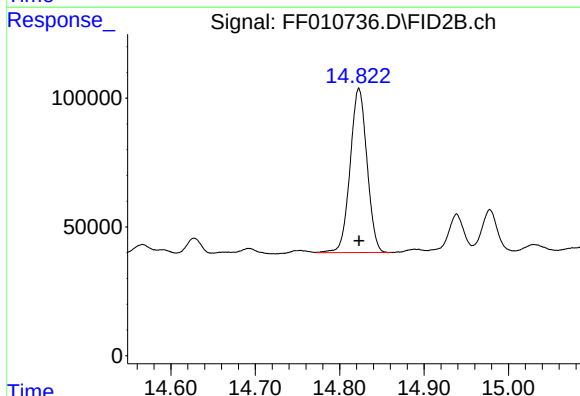


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.823 min
Delta R.T.: 0.000 min
Response: 885840
Conc: 7.84 ug/ml

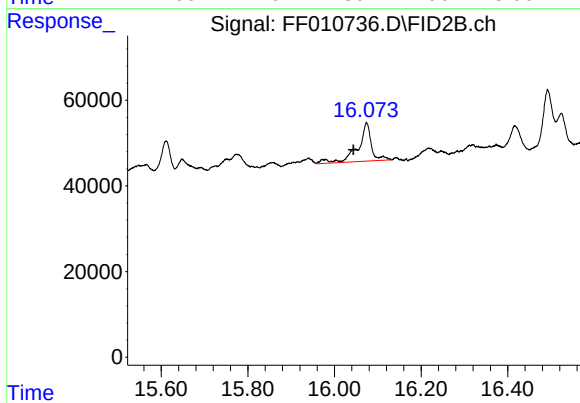

#11 N-HEXACOSANE


R.T.: 16.074 min
Delta R.T.: 0.030 min
Response: 193795
Conc: 1.53 ug/ml

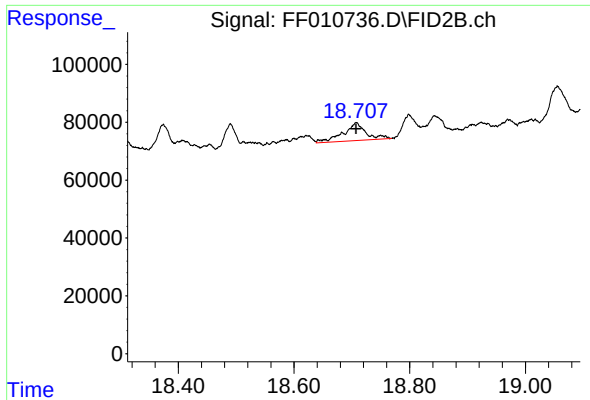

#14 N-DOTRIACONTANE

R.T.: 18.708 min
Delta R.T.: 0.000 min
Response: 167162
Conc: 1.38 ug/ml

Instrument :
FID_F
ClientSampleId :

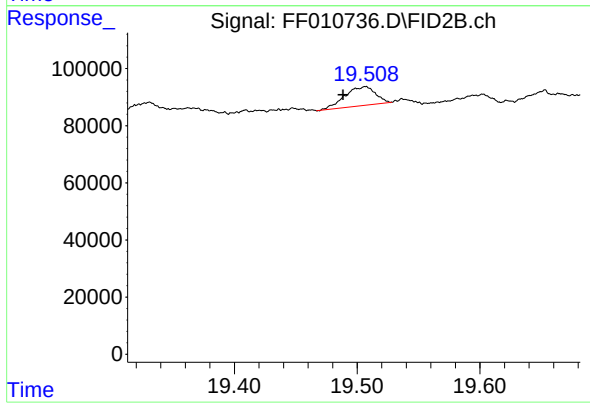

#15 N-TETRATRIACONTANE

R.T.: 19.506 min
Delta R.T.: 0.017 min
Response: 114835
Conc: 1.10 ug/ml