

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF060822\  
Data File : FF010730.D  
Signal(s) : FID2B.ch  
Acq On : 08 Jun 2022 09:39  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Jun 09 01:38:46 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060622.M  
Quant Title :  
QLast Update : Tue Jun 07 09:12:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.824 | 2695656  | 23.848 ug/ml |

Target Compounds  
-----

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF060822\  
Data File : FF010730.D  
Signal(s) : FID2B.ch  
Acq On : 08 Jun 2022 09:39  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Jun 09 01:38:46 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060622.M  
Quant Title :  
QLast Update : Tue Jun 07 09:12:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

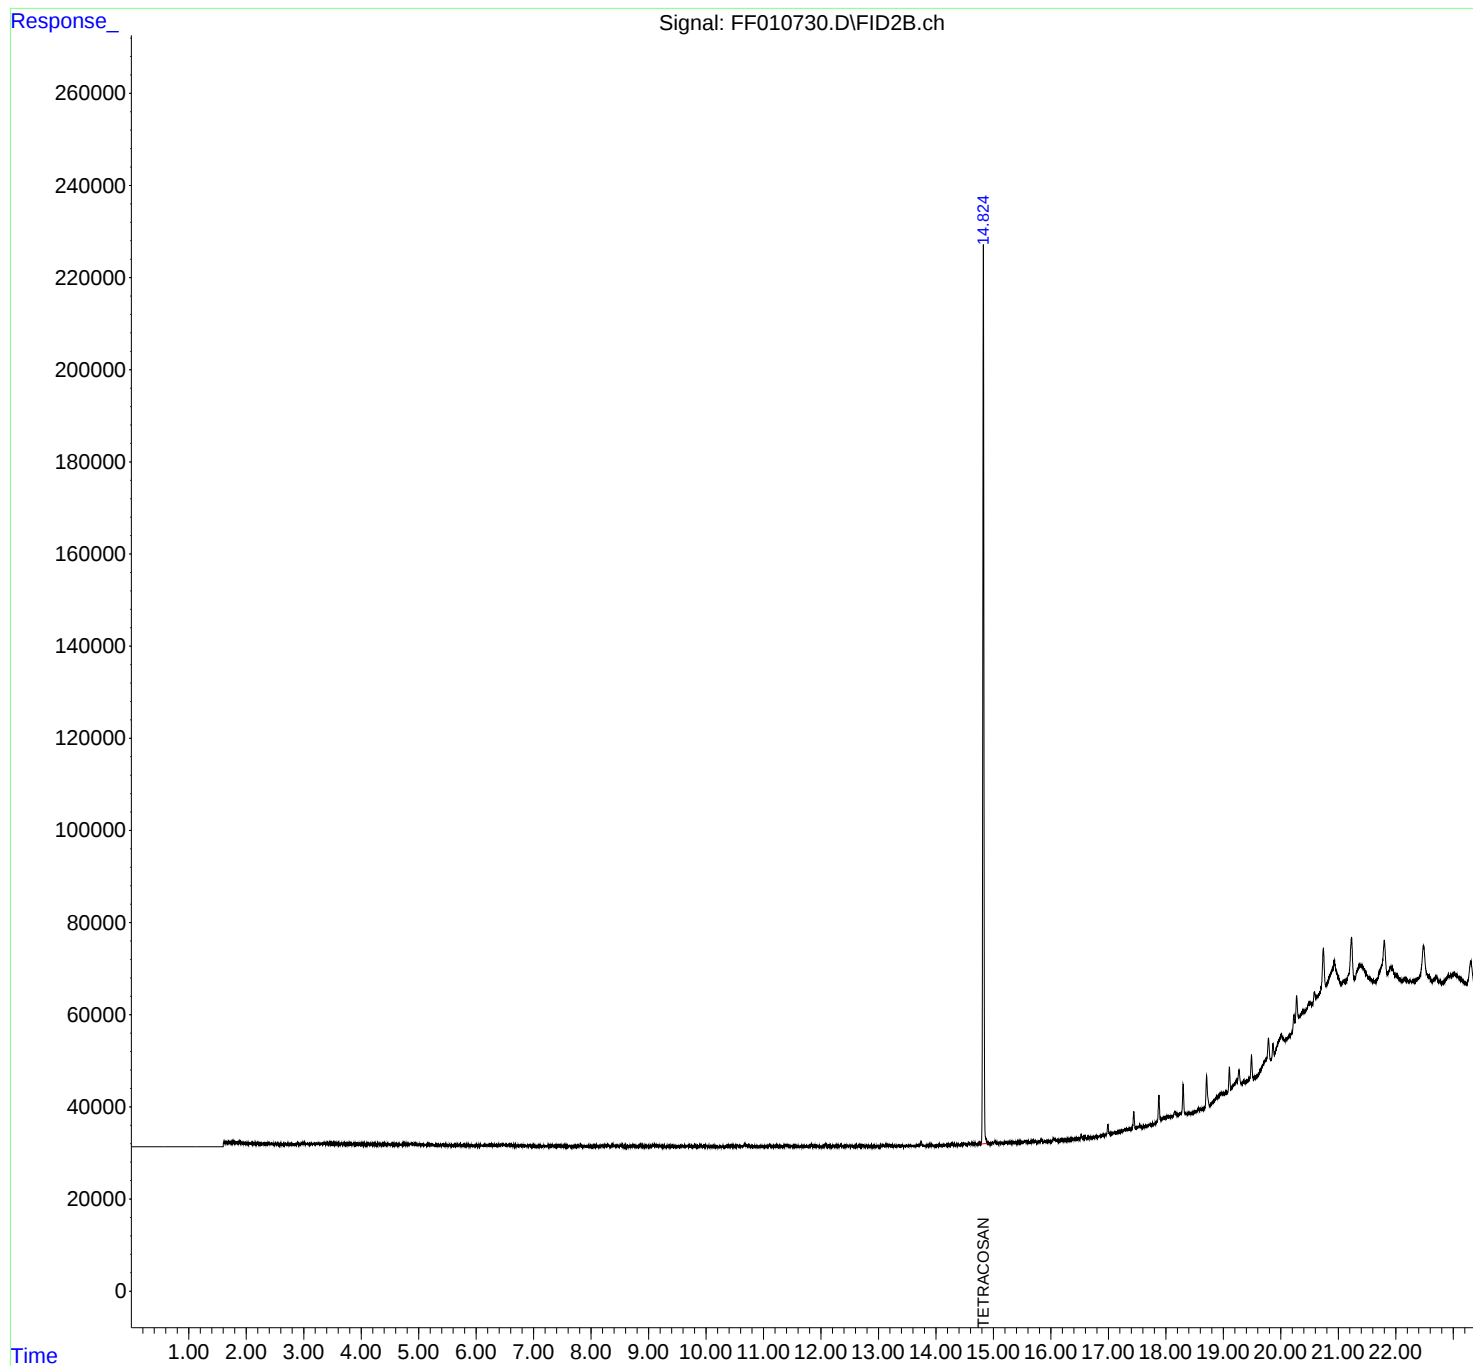

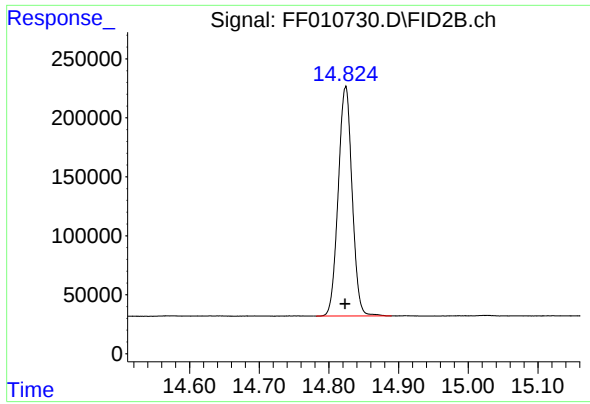

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.824 min  
Delta R.T.: 0.000 min  
Response: 2695656  
Conc: 23.85 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK