

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060822\
Data File : FF010736.D
Signal(s) : FID2B.ch
Acq On : 08 Jun 2022 13:17
Operator : AJ\MA
Sample : N3194-06RE
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TPH-1-TP-1RE

Integration File: autoint1.e
Quant Time: Jun 08 14:06:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.823	885840	7.837 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060822\
Data File : FF010736.D
Signal(s) : FID2B.ch
Acq On : 08 Jun 2022 13:17
Operator : AJ\MA
Sample : N3194-06RE
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TPH-1-TP-1RE

Integration File: autoint1.e
Quant Time: Jun 08 14:06:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

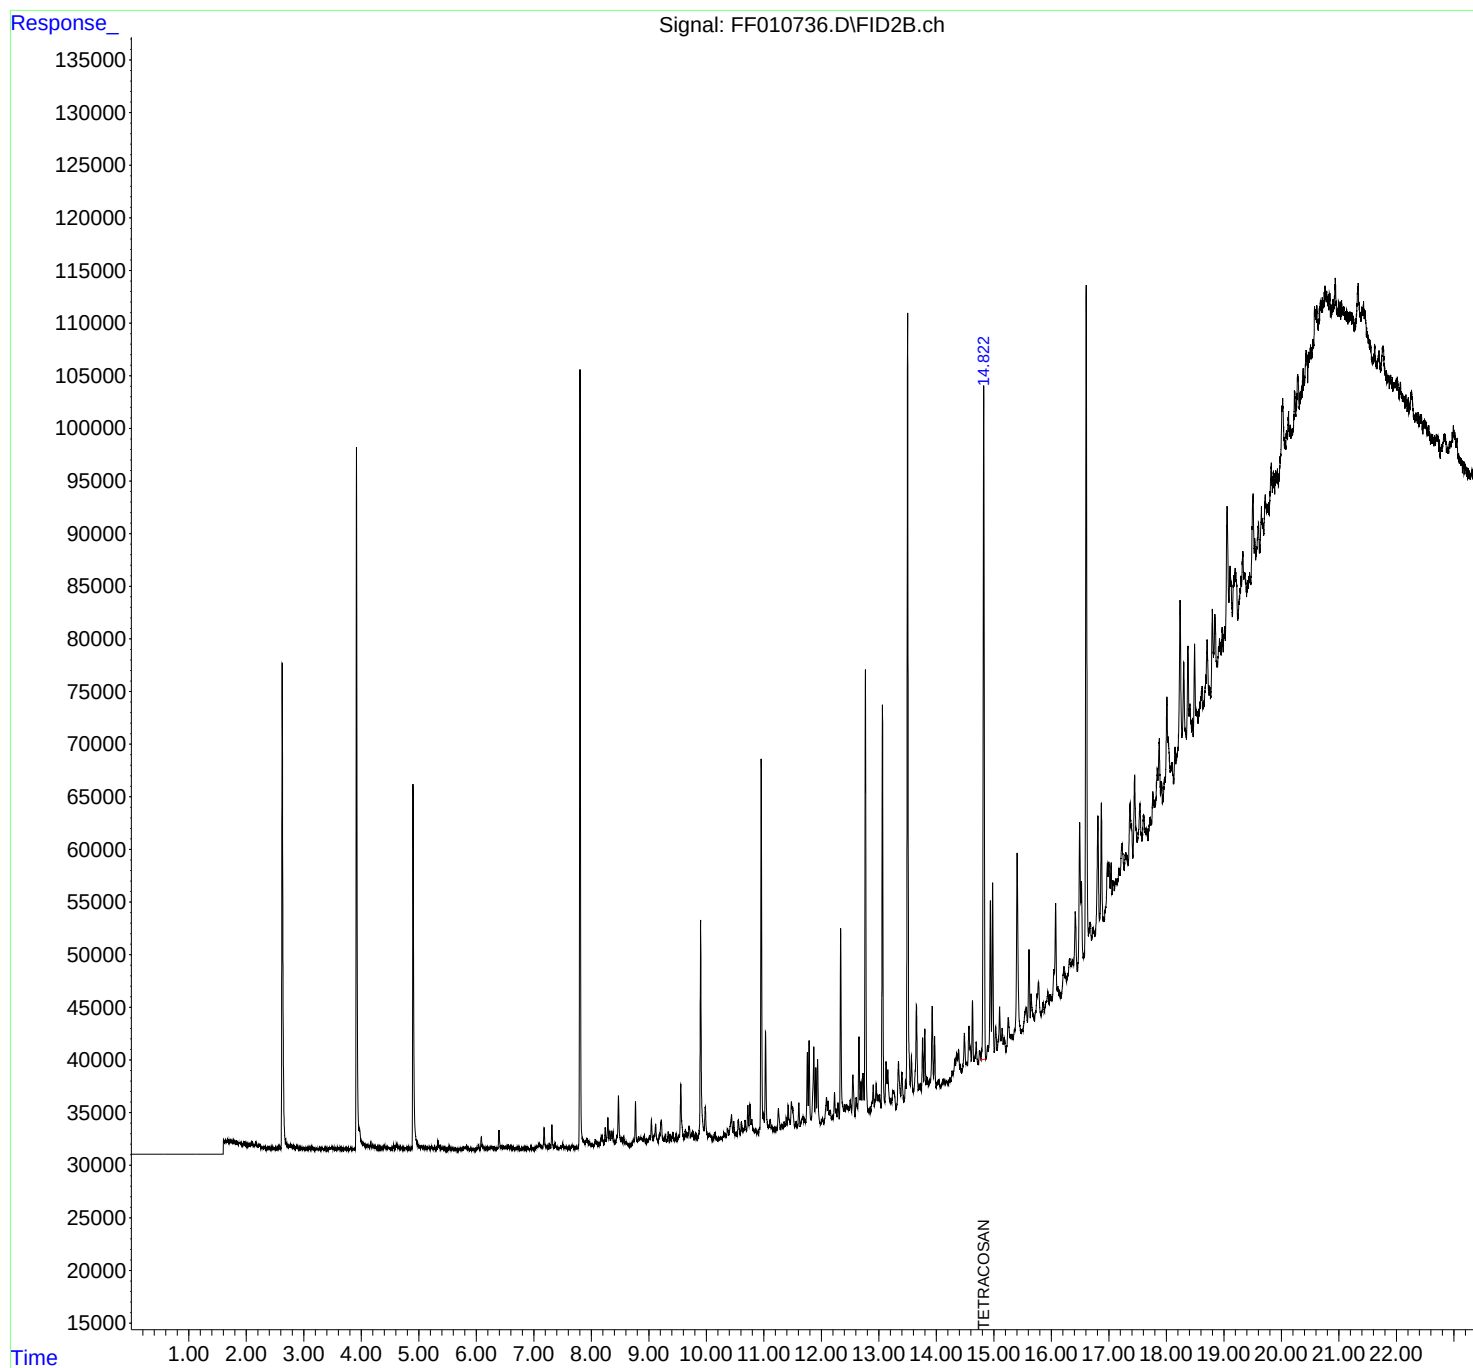

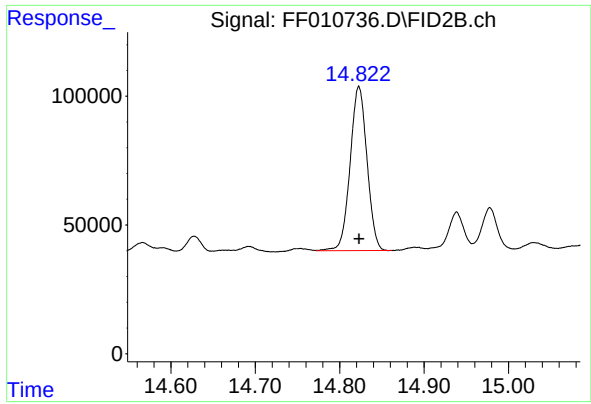

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.823 min
Delta R.T.: 0.000 min
Response: 885840
Conc: 7.84 ug/ml

Instrument :
FID_F
ClientSampleId :
TPH-1-TP-1RE