

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060920\
 Data File : FF007015.D
 Signal(s) : FID2B.ch
 Acq On : 09 Jun 2020 15:17
 Operator : DD\AJ
 Sample : L2815-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 10 01:53:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051520.M
 Quant Title :
 QLast Update : Sat May 16 03:36:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.719	1550554	11.219 ug/ml
Target Compounds			
4) N-TETRADECANE	8.330f	632023	3.776 ug/ml
7) N-EICOSANE	12.685f	6339981	38.835 ug/ml
8) N-DOCOSANE	13.842	471795	2.908 ug/ml
10) N-TETRACOSANE	14.896	2165869	13.697 ug/ml
11) N-HEXACOSANE	15.947	457251	2.981 ug/ml
12) N-OCTACOSANE	16.895	993946	6.678 ug/ml
13) N-TRIACONTANE	17.786	1325385	9.171 ug/ml
14) N-DOTRIACONTANE	18.614	1019597	7.659 ug/ml
15) N-TETRATRIACONTANE	19.403	216247	1.782 ug/ml
16) N-HEXATRIACONTANE	20.141	426236	3.897 ug/ml
18) N-TETRACONTANE	21.808	216646	2.178 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060920\
Data File : FF007015.D
Signal(s) : FID2B.ch
Acq On : 09 Jun 2020 15:17
Operator : DD\AJ
Sample : L2815-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 10 01:53:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051520.M
Quant Title :
QLast Update : Sat May 16 03:36:49 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

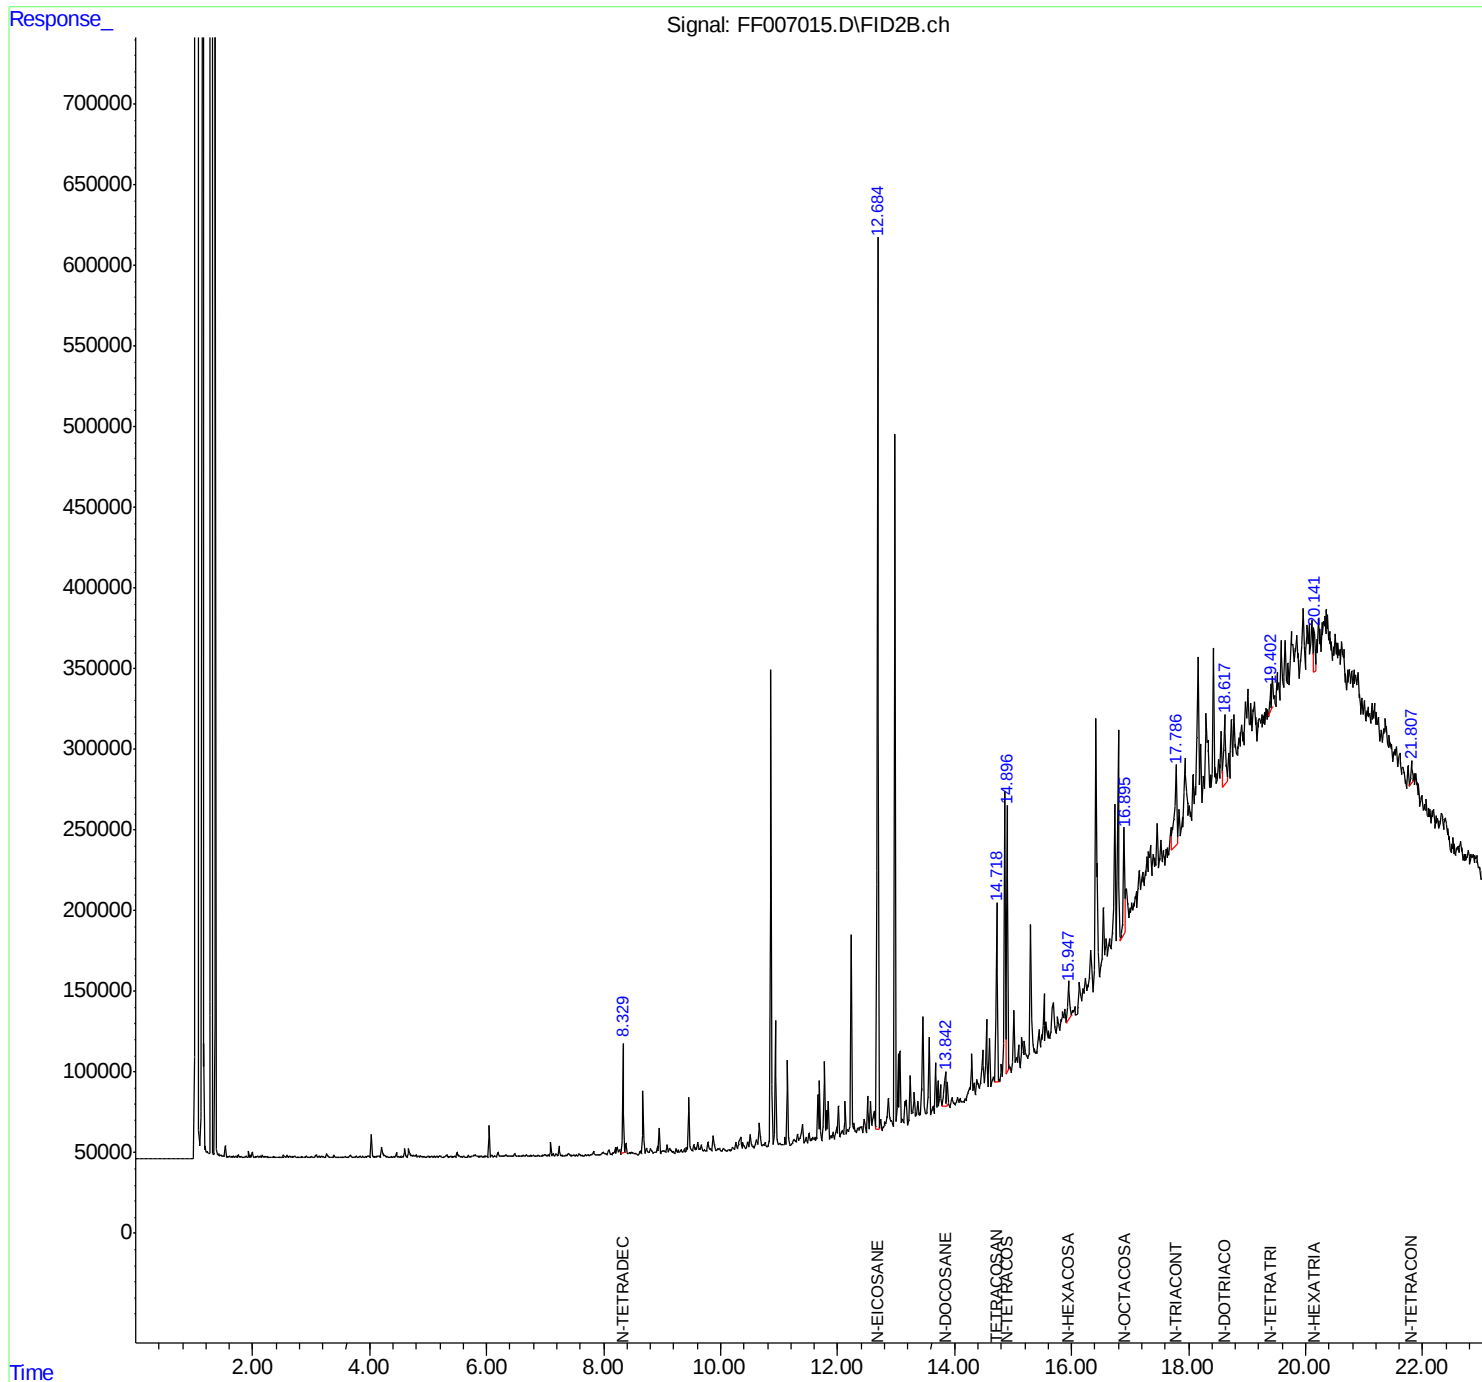

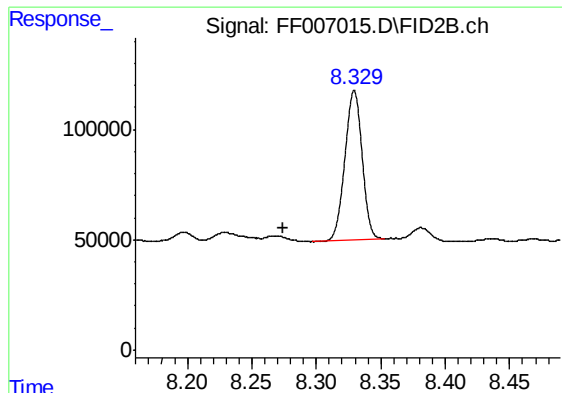


#4 N-TETRADECANE

R.T.: 8.330 min
Delta R.T.: 0.056 min
Response: 632023
Conc: 3.78 ug/ml

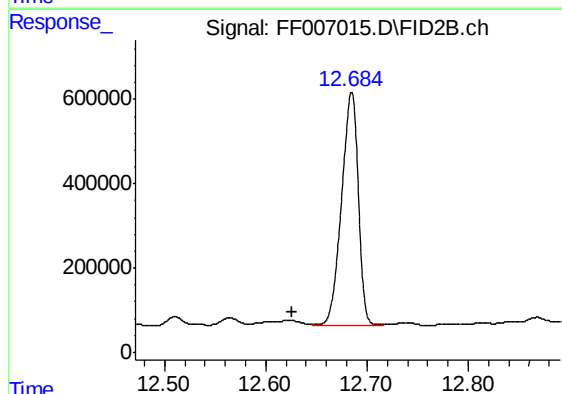


#7 N-EICOSANE

R.T.: 12.685 min
Delta R.T.: 0.058 min
Response: 6339981
Conc: 38.84 ug/ml

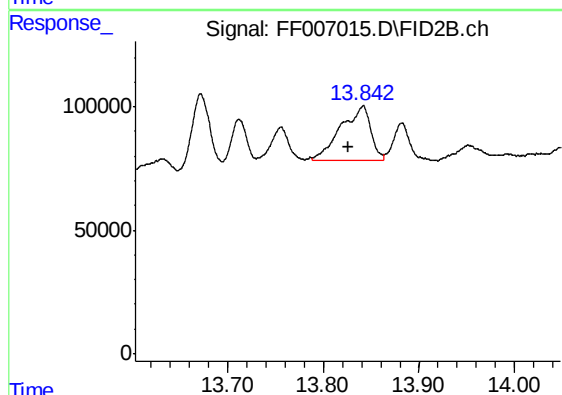


#8 N-DOCOSANE

R.T.: 13.842 min
Delta R.T.: 0.016 min
Response: 471795
Conc: 2.91 ug/ml

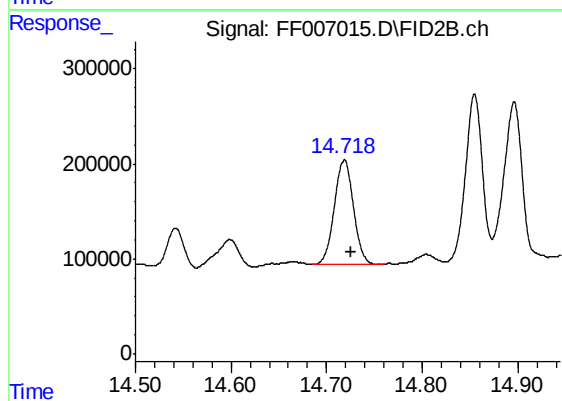


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.719 min
Delta R.T.: -0.007 min
Response: 1550554
Conc: 11.22 ug/ml

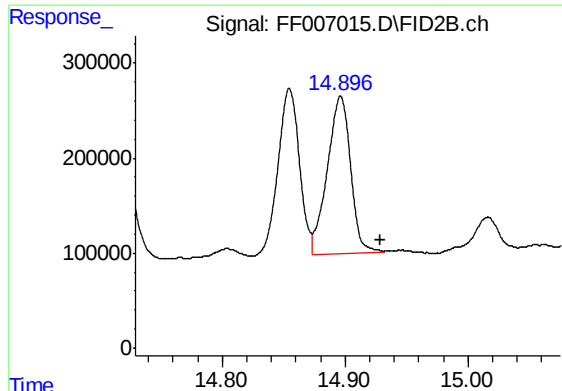


#10 N-TETRACOSANE

R.T.: 14.896 min
Delta R.T.: -0.033 min
Response: 2165869
Conc: 13.70 ug/ml

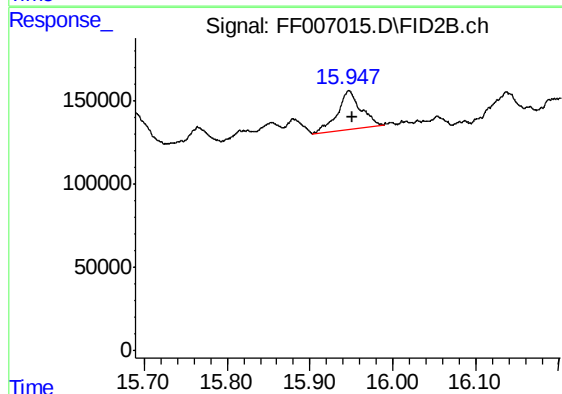


#11 N-HEXACOSANE

R.T.: 15.947 min
Delta R.T.: -0.004 min
Response: 457251
Conc: 2.98 ug/ml

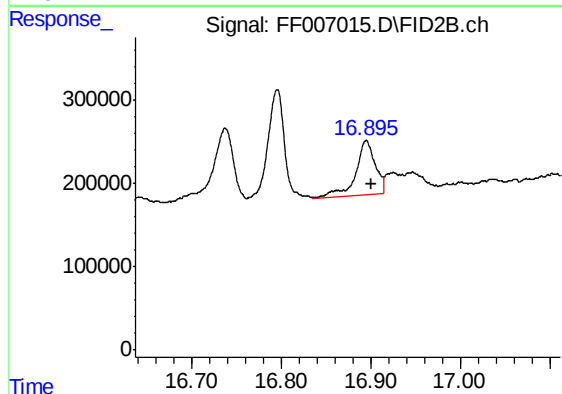


#12 N-OCTACOSANE

R.T.: 16.895 min
Delta R.T.: -0.006 min
Response: 993946
Conc: 6.68 ug/ml

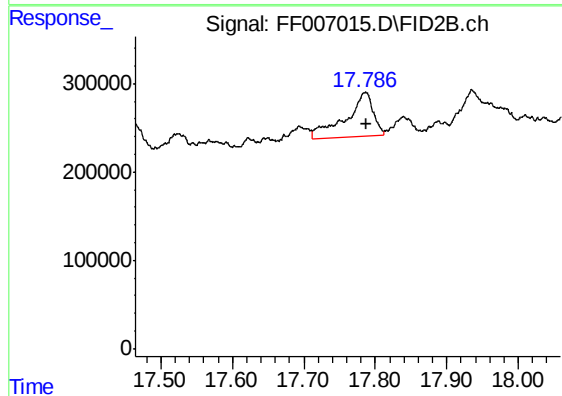


#13 N-TRIACONTANE

R.T.: 17.786 min
Delta R.T.: -0.002 min
Response: 1325385
Conc: 9.17 ug/ml

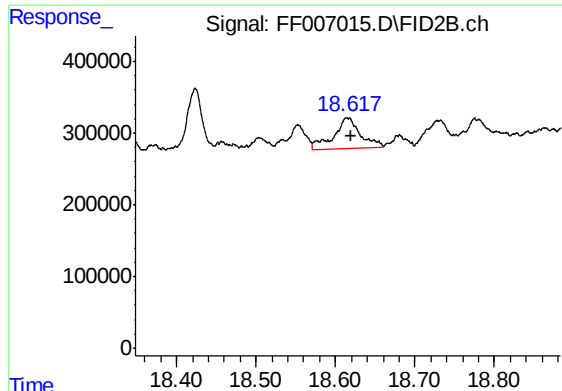


#14 N-DOTRIACONTANE

R.T.: 18.614 min
Delta R.T.: -0.006 min
Response: 1019597
Conc: 7.66 ug/ml

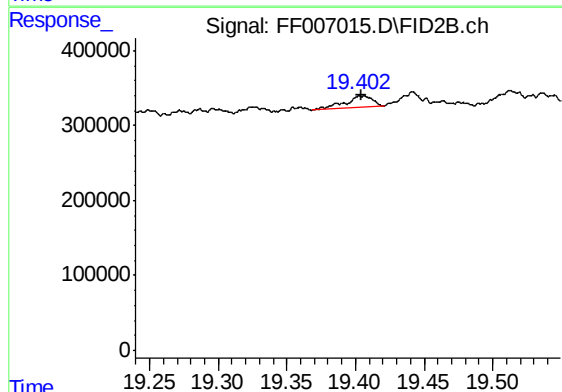


#15 N-TETRATRIACONTANE

R.T.: 19.403 min
Delta R.T.: 0.000 min
Response: 216247
Conc: 1.78 ug/ml

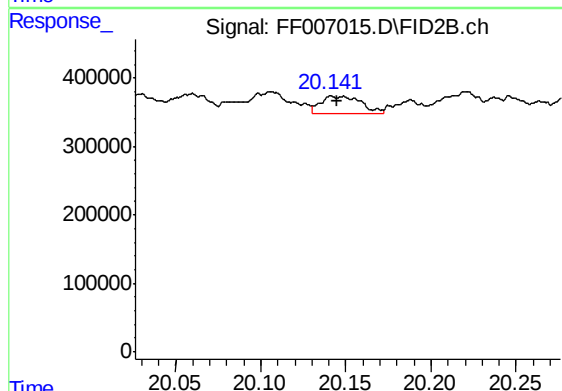

#16 N-HEXATRIACONTANE

R.T.: 20.141 min
Delta R.T.: -0.003 min
Response: 426236
Conc: 3.90 ug/ml

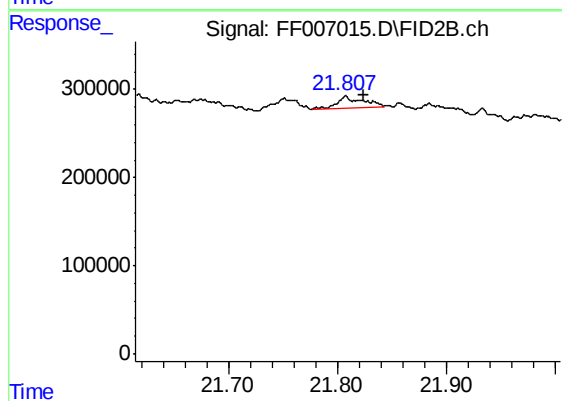

#18 N-TETRACONTANE

R.T.: 21.808 min
Delta R.T.: -0.016 min
Response: 216646
Conc: 2.18 ug/ml