

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060920\
 Data File : FF007020.D
 Signal(s) : FID2B.ch
 Acq On : 09 Jun 2020 17:52
 Operator : DD\AJ
 Sample : L2815-01 2X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 10 01:54:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051520.M
 Quant Title :
 QLast Update : Sat May 16 03:36:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.727	726795	5.258 ug/ml
Target Compounds			
4) N-TETRADECANE	8.336f	280024	1.673 ug/ml
7) N-EICOSANE	12.693f	2929856	17.947 ug/ml
10) N-TETRACOSANE	14.908	1067275	6.749 ug/ml
12) N-OCTACOSANE	16.905	530873	3.567 ug/ml
13) N-TRIACONTANE	17.795	610265	4.223 ug/ml
14) N-DOTRIACONTANE	18.624	373032	2.802 ug/ml
16) N-HEXATRIACONTANE	20.090f	109166	0.998 ug/ml
17) N-OCTATRIACONTANE	20.905	172225	1.737 ug/ml
18) N-TETRACONTANE	21.876f	137245	1.380 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060920\
Data File : FF007020.D
Signal(s) : FID2B.ch
Acq On : 09 Jun 2020 17:52
Operator : DD\AJ
Sample : L2815-01 2X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 10 01:54:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051520.M
Quant Title :
QLast Update : Sat May 16 03:36:49 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

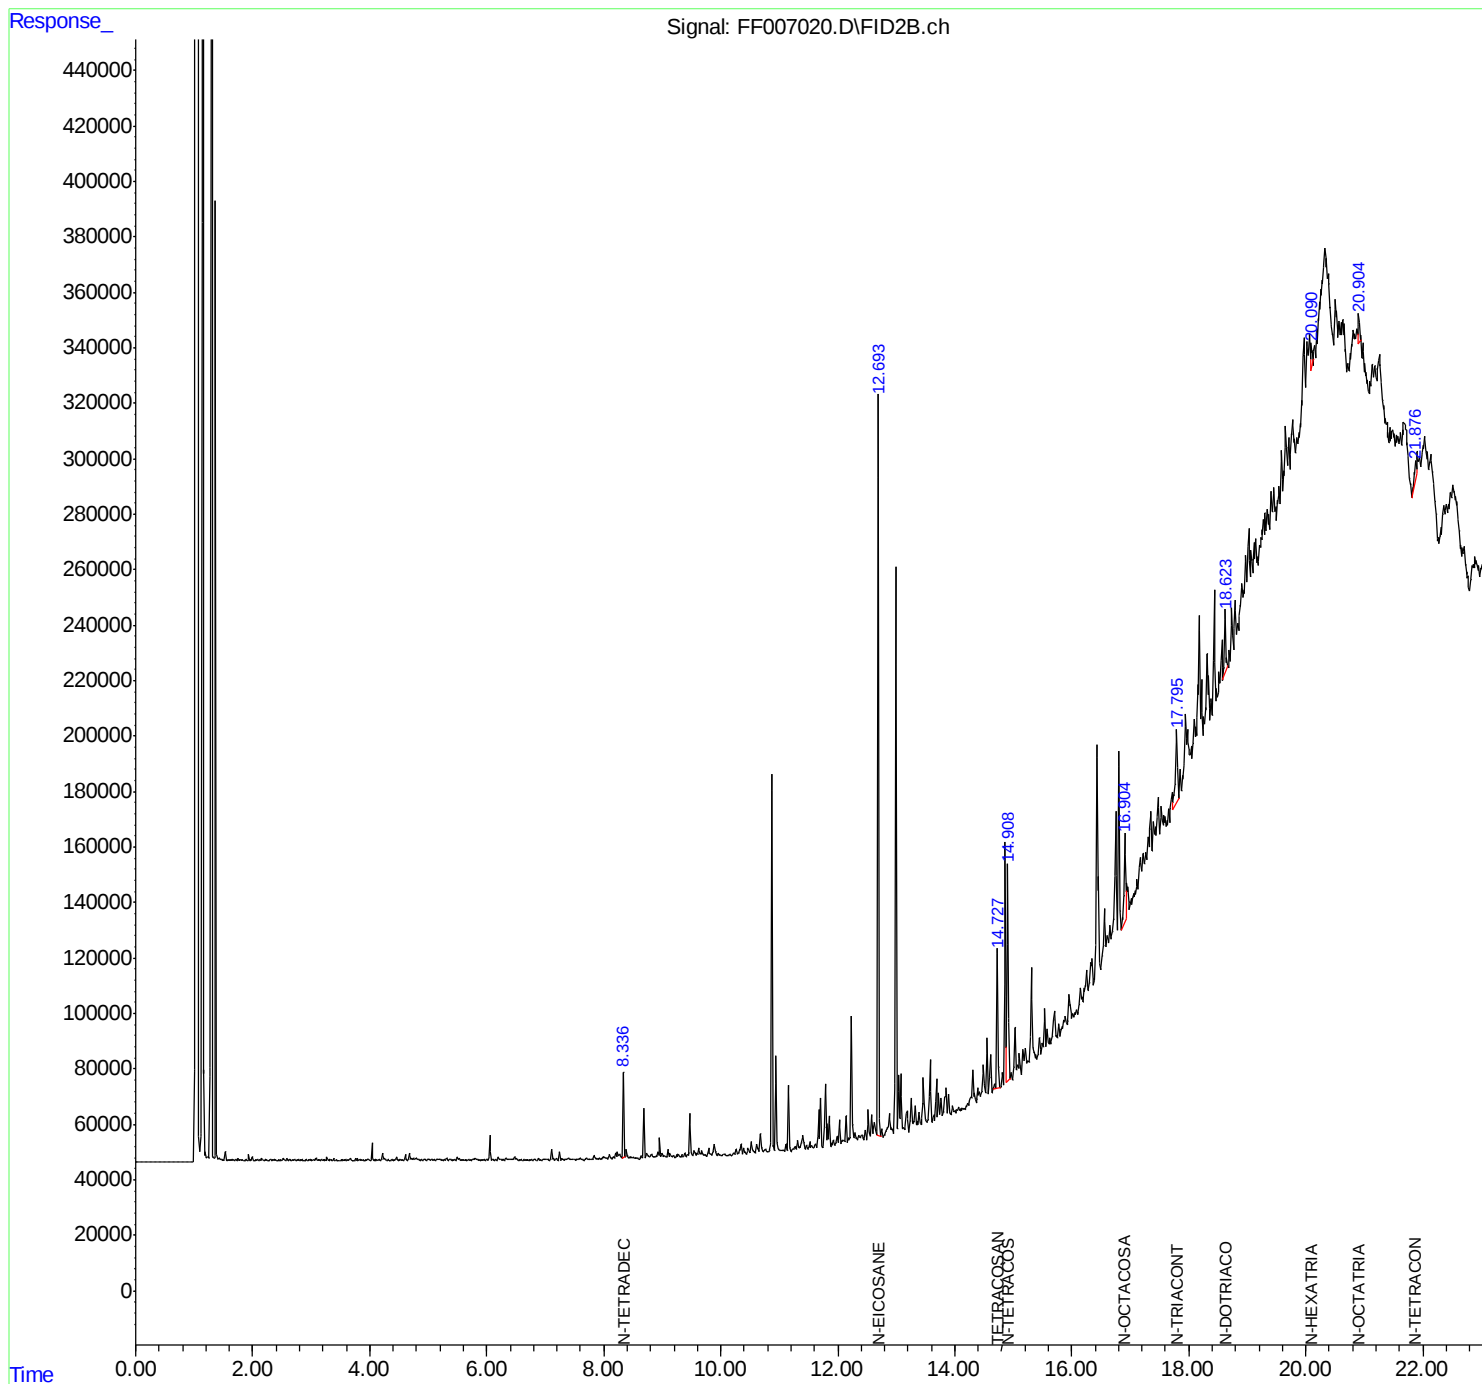

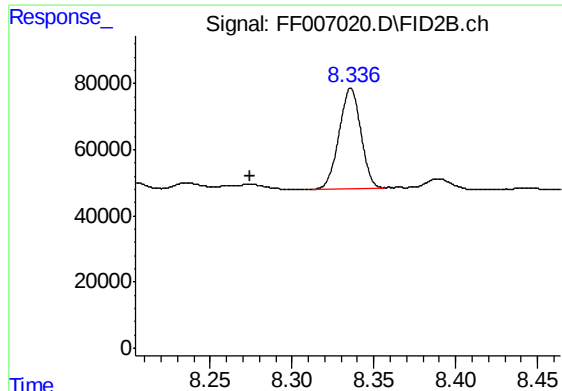


#4 N-TETRADECANE

R.T.: 8.336 min
Delta R.T.: 0.062 min
Response: 280024
Conc: 1.67 ug/ml

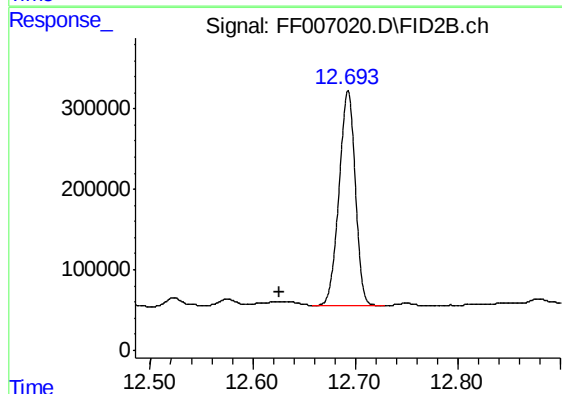


#7 N-EICOSANE

R.T.: 12.693 min
Delta R.T.: 0.066 min
Response: 2929856
Conc: 17.95 ug/ml

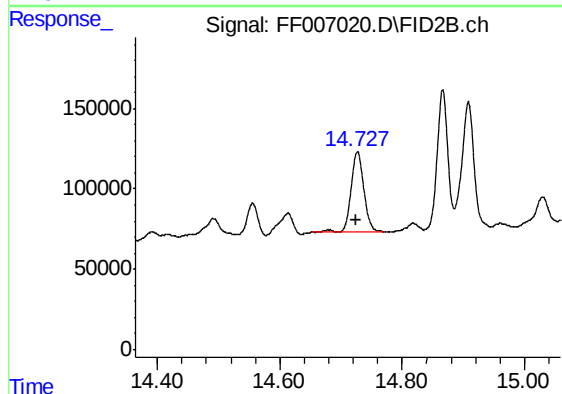


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.727 min
Delta R.T.: 0.002 min
Response: 726795
Conc: 5.26 ug/ml

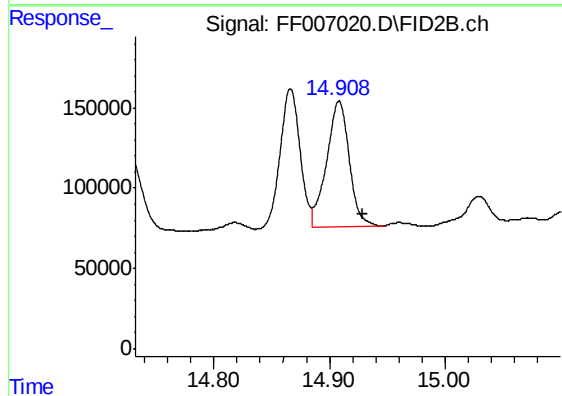


#10 N-TETRACOSANE

R.T.: 14.908 min
Delta R.T.: -0.021 min
Response: 1067275
Conc: 6.75 ug/ml

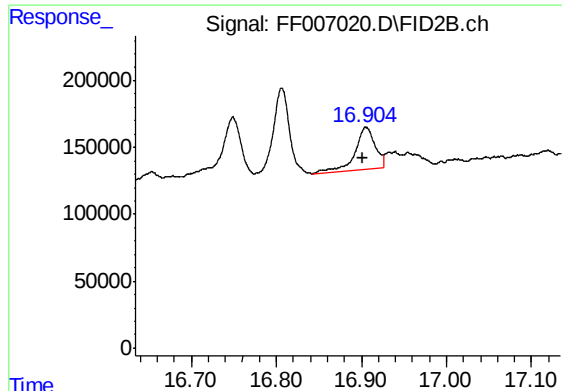


#12 N-OCTACOSANE

R.T.: 16.905 min
Delta R.T.: 0.005 min
Response: 530873
Conc: 3.57 ug/ml

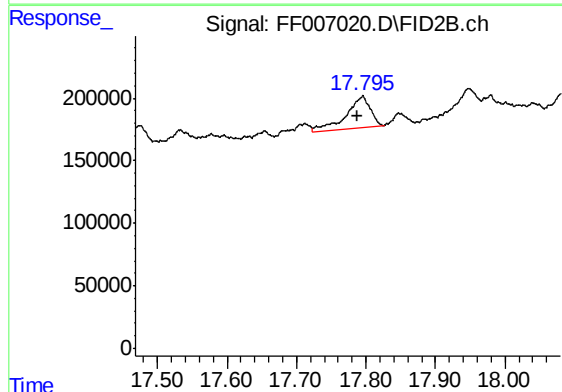


#13 N-TRIACONTANE

R.T.: 17.795 min
Delta R.T.: 0.007 min
Response: 610265
Conc: 4.22 ug/ml

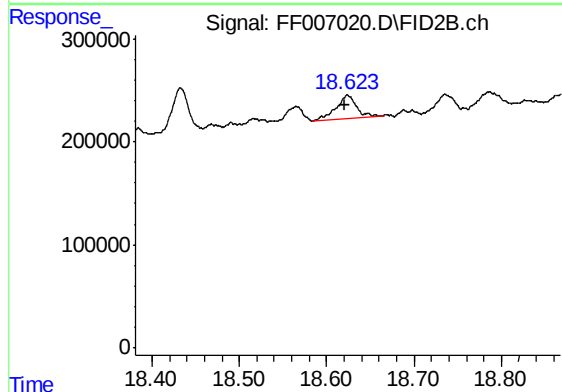


#14 N-DOTRIACONTANE

R.T.: 18.624 min
Delta R.T.: 0.004 min
Response: 373032
Conc: 2.80 ug/ml

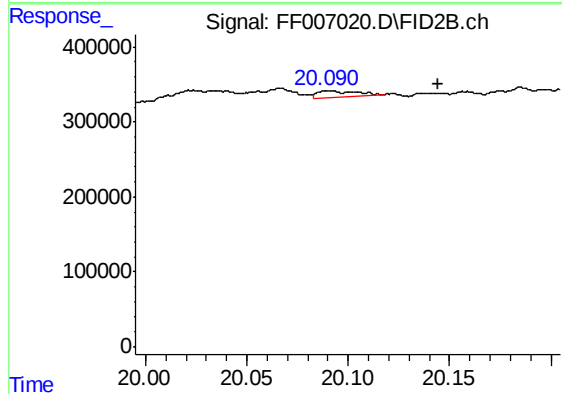


#16 N-HEXATRIACONTANE

R.T.: 20.090 min
Delta R.T.: -0.055 min
Response: 109166
Conc: 1.00 ug/ml

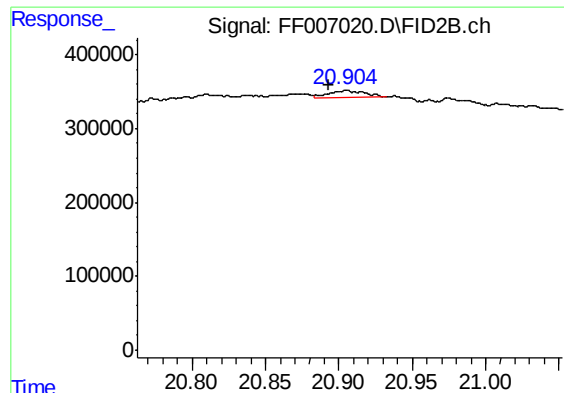

#17 N-OCTATRIACONTANE

R.T.: 20.905 min
Delta R.T.: 0.012 min
Response: 172225
Conc: 1.74 ug/ml

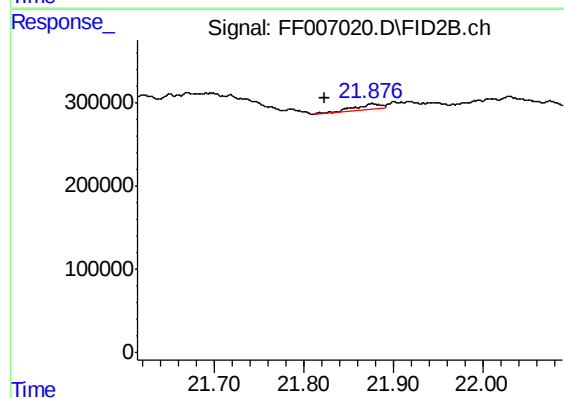

#18 N-TETRACONTANE

R.T.: 21.876 min
Delta R.T.: 0.052 min
Response: 137245
Conc: 1.38 ug/ml