

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060921\
Data File : FF008588.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2021 00:23
Operator : DD\AJ
Sample : M2625-17
Misc :
ALS Vial : 65 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 10 01:37:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.768	1900041	18.033 ug/ml
Target Compounds			


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060921\
Data File : FF008588.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2021 00:23
Operator : DD\AJ
Sample : M2625-17
Misc :
ALS Vial : 65 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 10 01:37:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

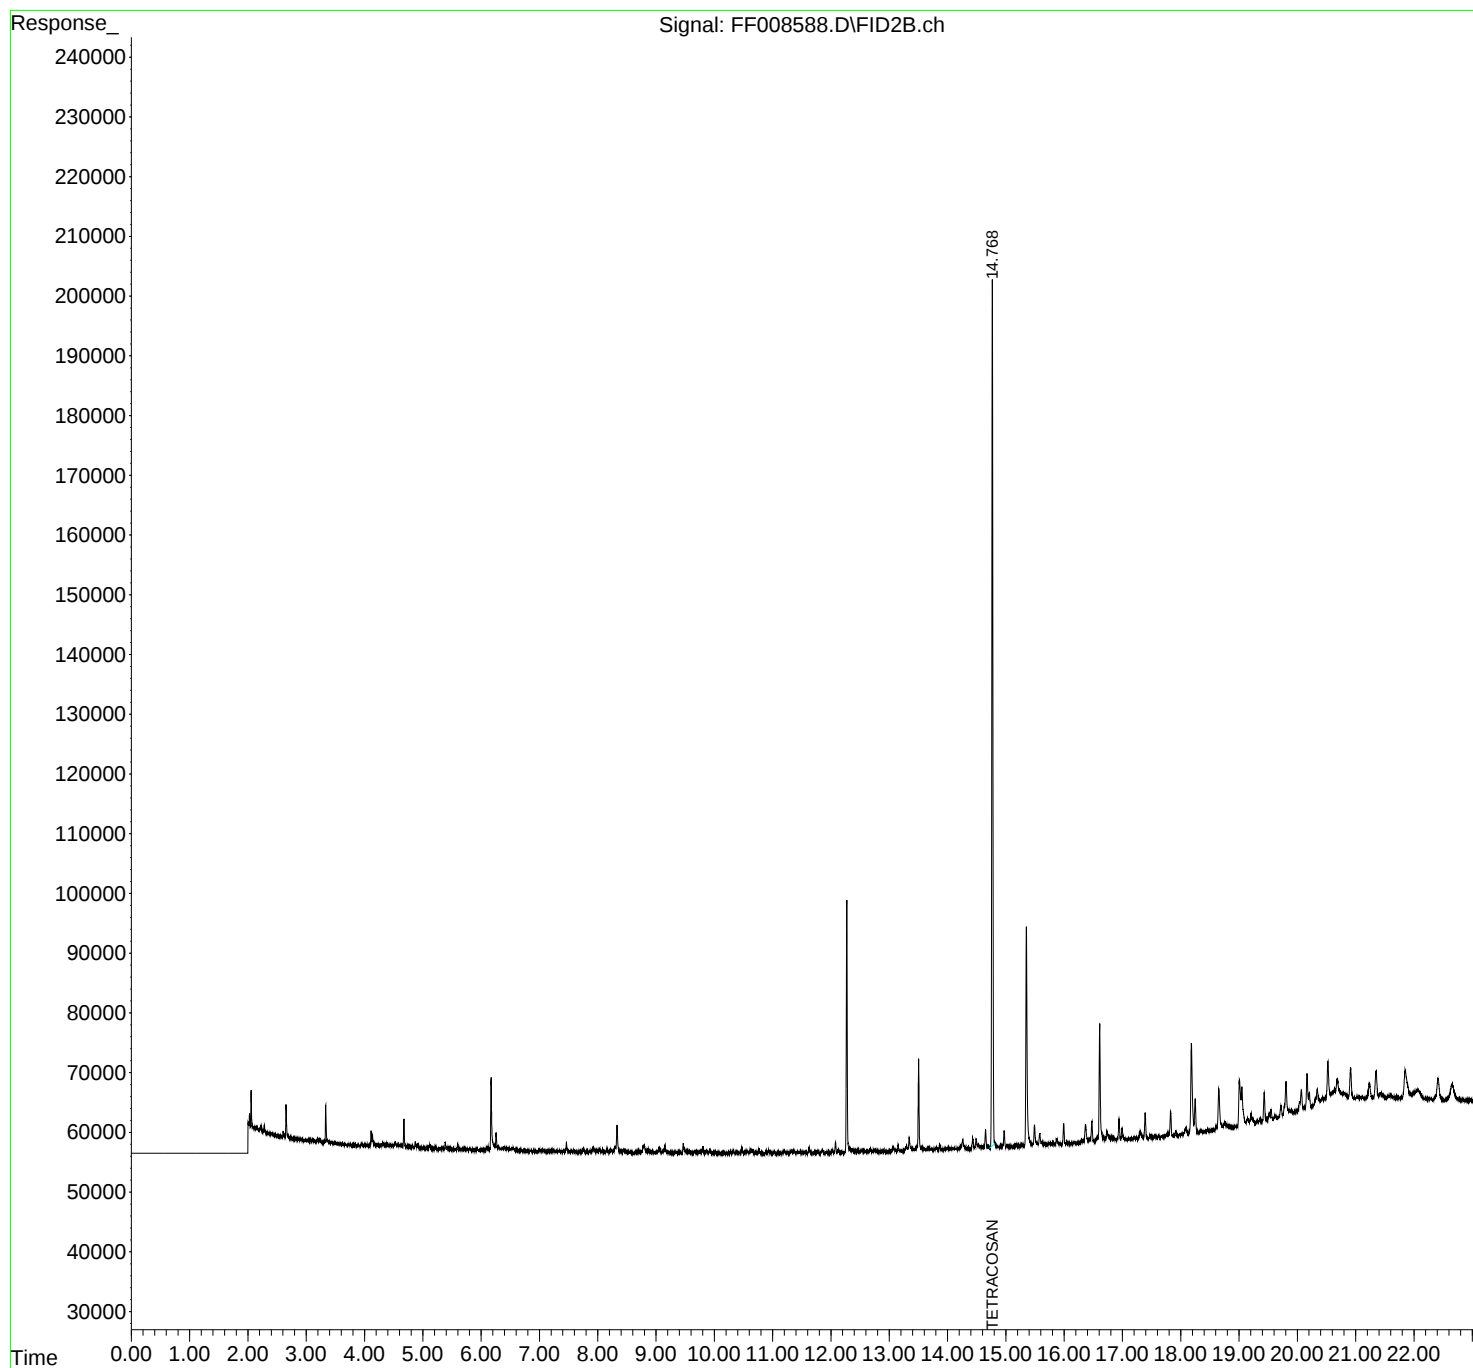

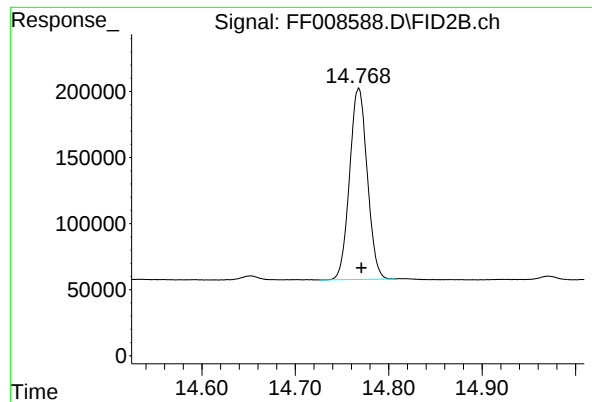

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.768 min
Delta R.T.: -0.003 min
Response: 1900041
Conc: 18.03 ug/ml