

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060923\
Data File : FF012859.D
Signal(s) : FID2B.ch
Acq On : 09 Jun 2023 15:28
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 09 23:25:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.966	1826170	15.638 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.021	65602	0.509 ug/ml
14) N-DOTRIACONTANE	18.852	93693	0.741 ug/ml
15) N-TETRATRIACONTANE	19.636	63478	0.534 ug/ml
16) N-HEXATRIACONTANE	20.374	45520	0.379 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060923\
Data File : FF012859.D
Signal(s) : FID2B.ch
Acq On : 09 Jun 2023 15:28
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 09 23:25:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

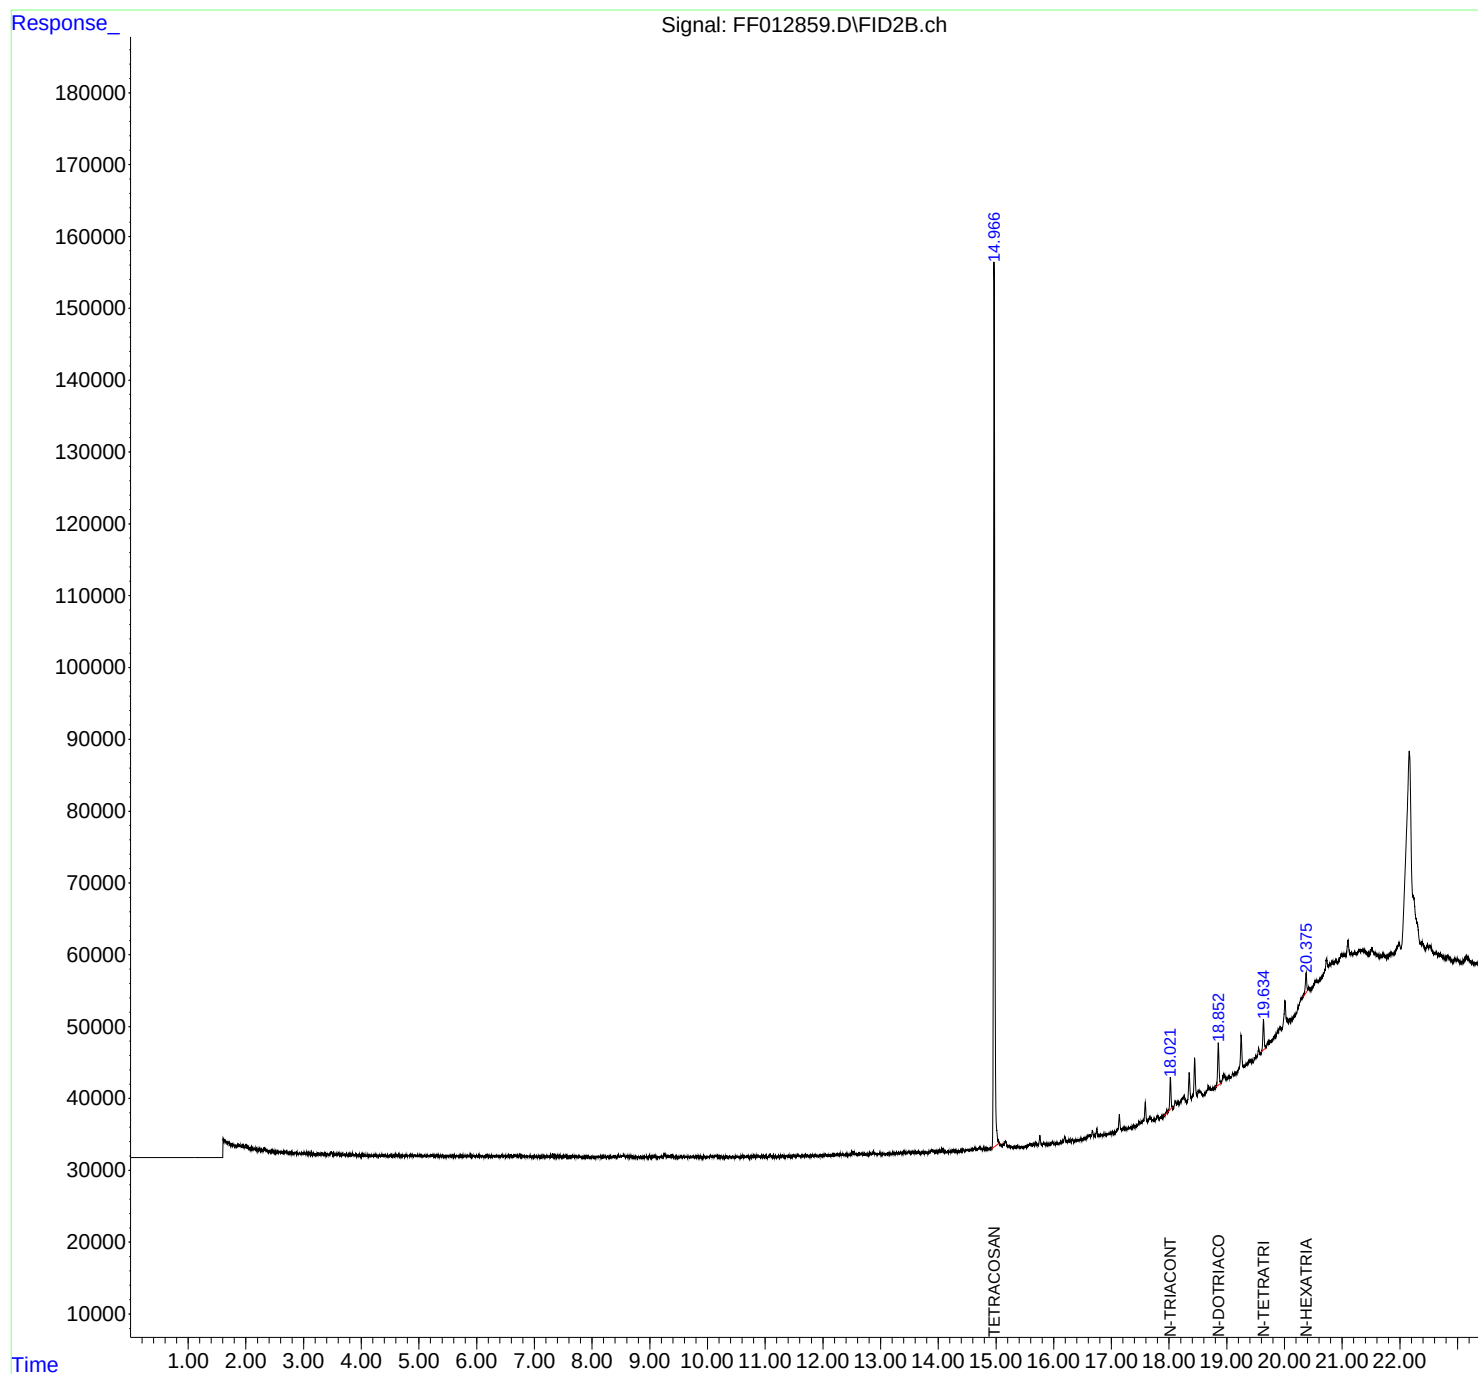


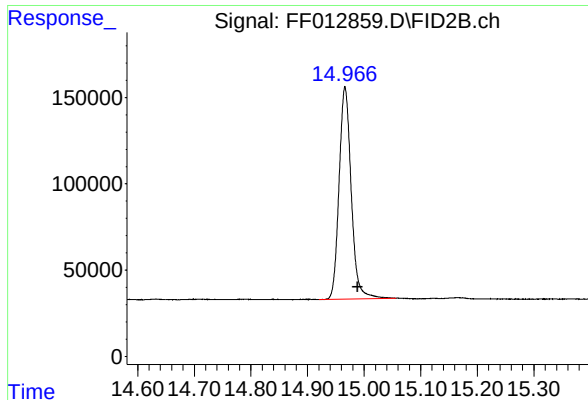

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.966 min
Delta R.T.: -0.023 min
Response: 1826170
Conc: 15.64 ug/ml

Instrument :
FID_F
ClientSampleId :

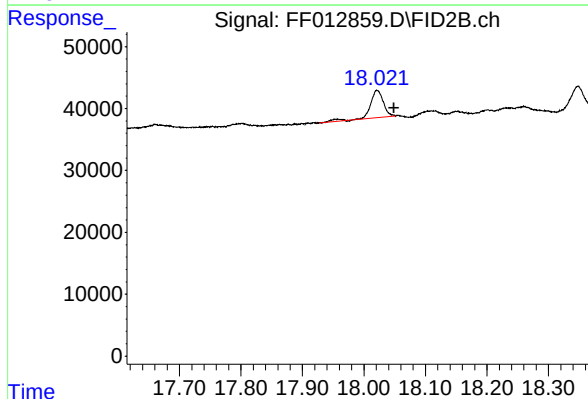


#13 N-TRIACONTANE

R.T.: 18.021 min
Delta R.T.: -0.027 min
Response: 65602
Conc: 0.51 ug/ml

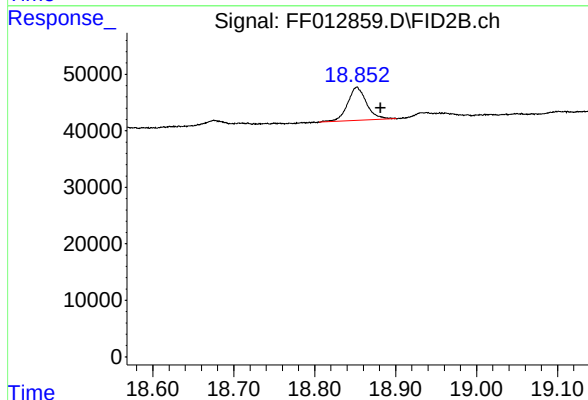


#14 N-DOTRIACONTANE

R.T.: 18.852 min
Delta R.T.: -0.029 min
Response: 93693
Conc: 0.74 ug/ml

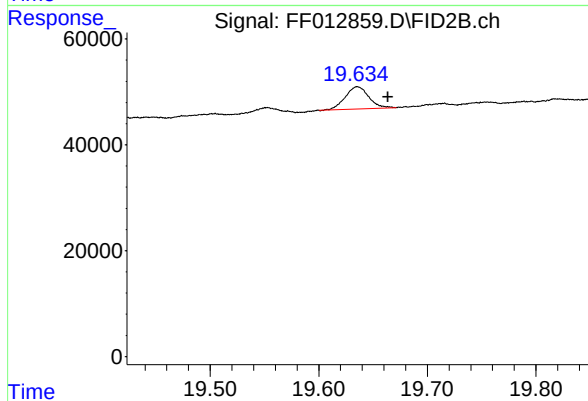

#15 N-TETRATRIACONTANE

R.T.: 19.636 min
Delta R.T.: -0.028 min
Response: 63478
Conc: 0.53 ug/ml

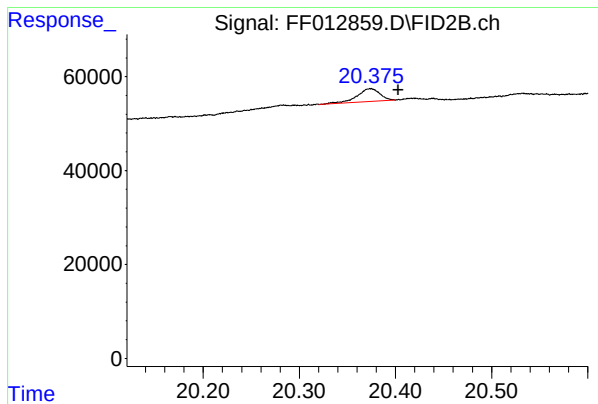

#16 N-HEXATRIACONTANE

R.T.: 20.374 min
Delta R.T.: -0.029 min
Response: 45520
Conc: 0.38 ug/ml

Instrument :

FID_F

ClientSampleId :