

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061019\
 Data File : FF004763.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jun 2019 17:13
 Operator : DD\AJ
 Sample : K3265-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 11 01:41:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.707	2330166	19.082 ug/ml
Target Compounds			
4) N-TETRADECANE	8.293	423700	2.884 ug/ml
7) N-EICOSANE	12.658f	155401	1.073 ug/ml
8) N-DOCOSANE	13.858f	1226891	8.683 ug/ml
10) N-TETRACOSANE	14.883	87010	0.628 ug/ml
11) N-HEXACOSANE	15.936	206318	1.514 ug/ml
12) N-OCTACOSANE	16.890	466936	3.434 ug/ml
13) N-TRIACONTANE	17.781	621916	4.497 ug/ml
14) N-DOTRIACONTANE	18.618	316700	2.289 ug/ml
15) N-TETRATRIACONTANE	19.407	160601	1.175 ug/ml
16) N-HEXATRIACONTANE	20.158	49725	0.378 ug/ml
18) N-TETRACONTANE	21.868	635276	5.159 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061019\
Data File : FF004763.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2019 17:13
Operator : DD\AJ
Sample : K3265-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 11 01:41:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

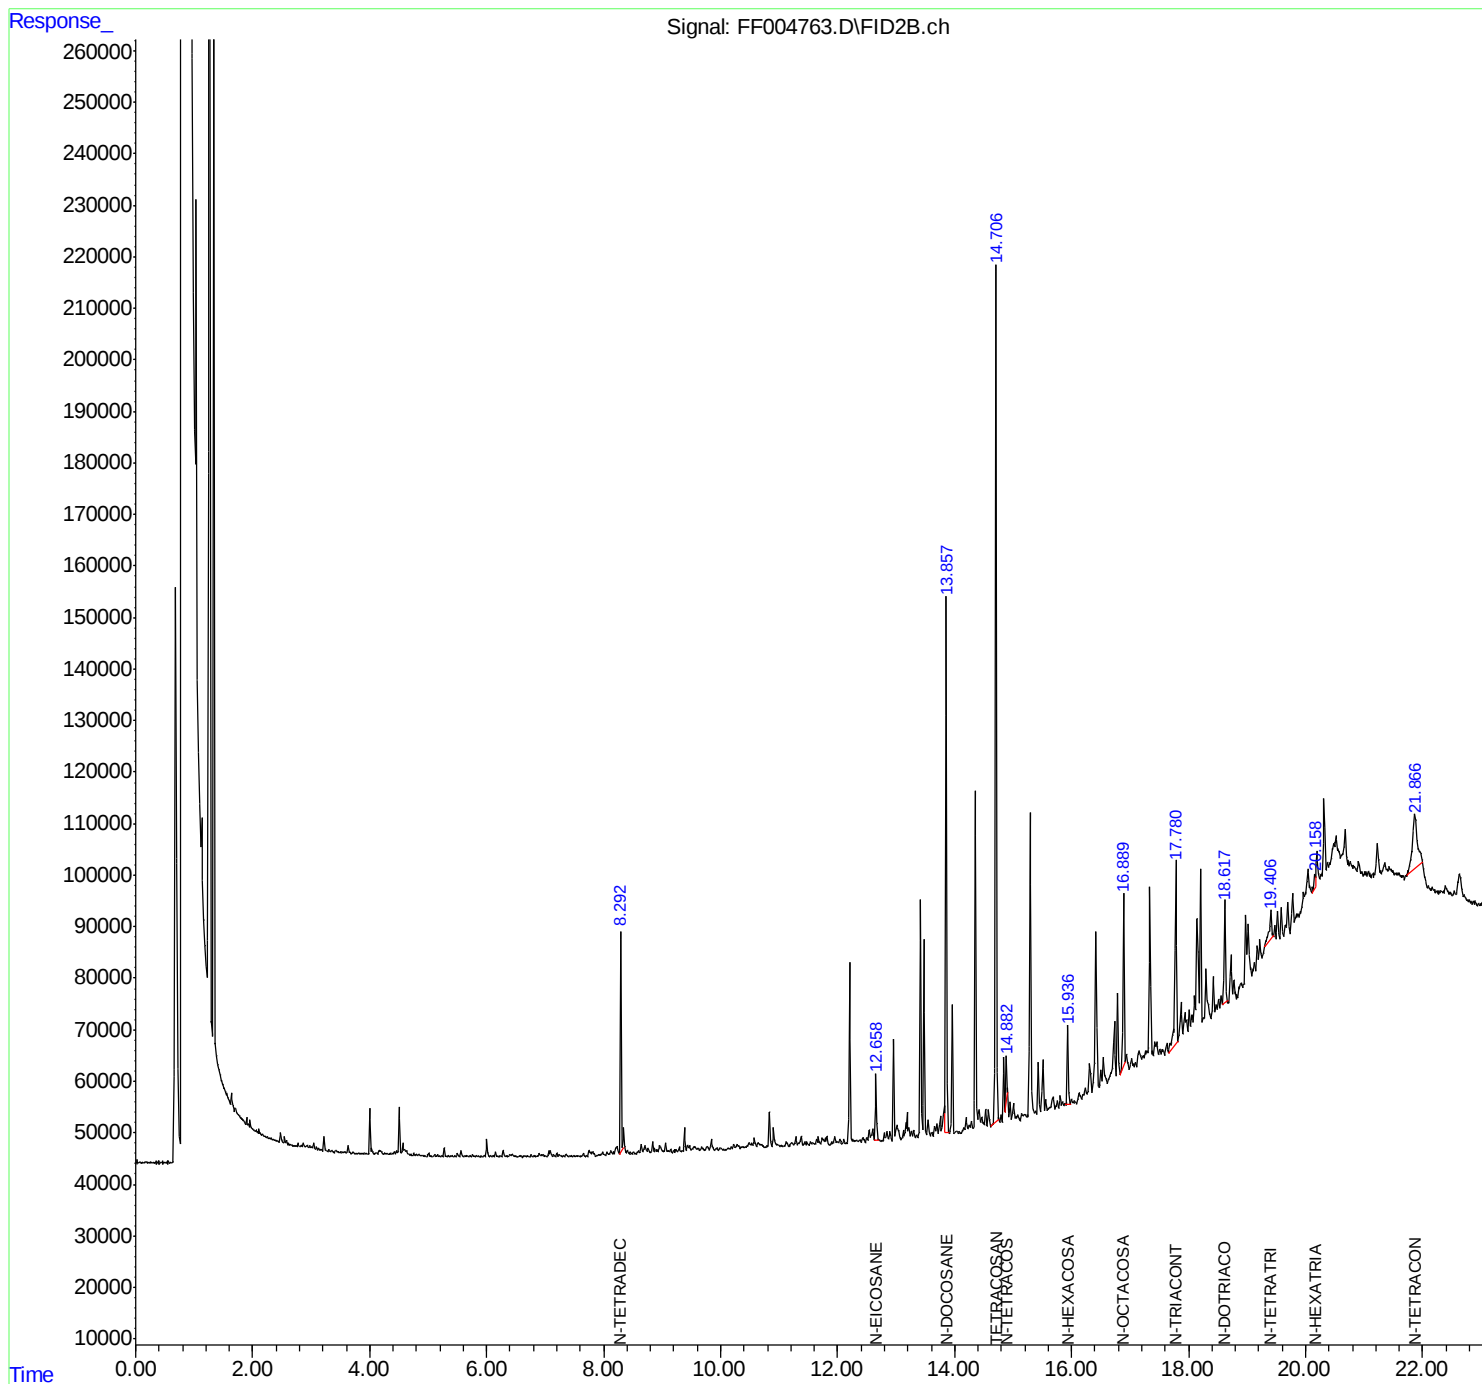

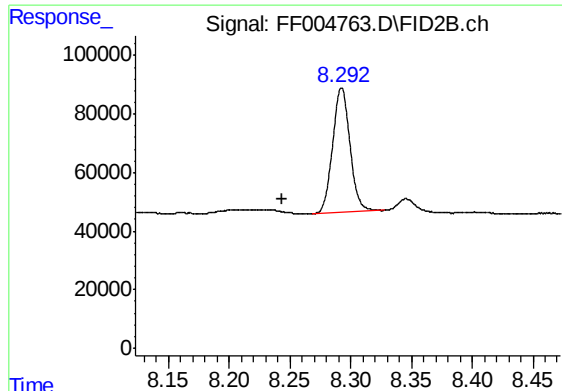


#4 N-TETRADECANE

R.T.: 8.293 min
Delta R.T.: 0.049 min
Response: 423700
Conc: 2.88 ug/ml

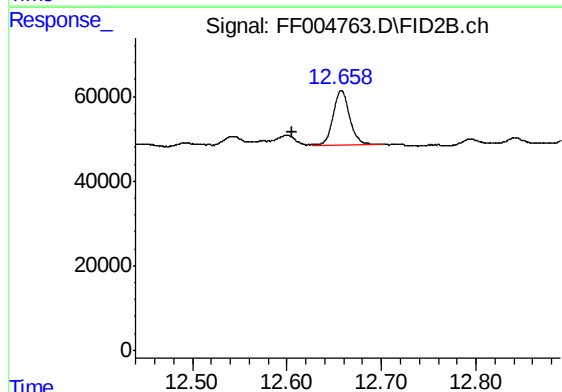


#7 N-EICOSANE

R.T.: 12.658 min
Delta R.T.: 0.052 min
Response: 155401
Conc: 1.07 ug/ml

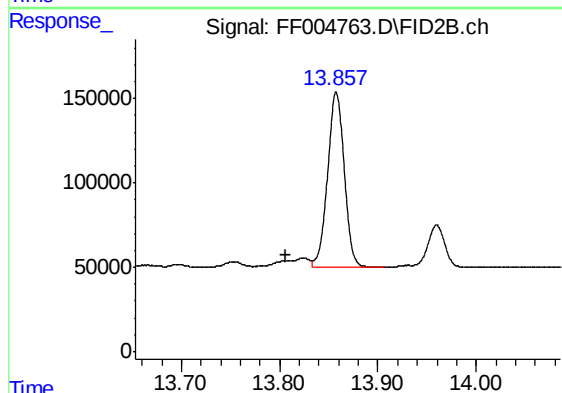


#8 N-DOCOSANE

R.T.: 13.858 min
Delta R.T.: 0.051 min
Response: 1226891
Conc: 8.68 ug/ml

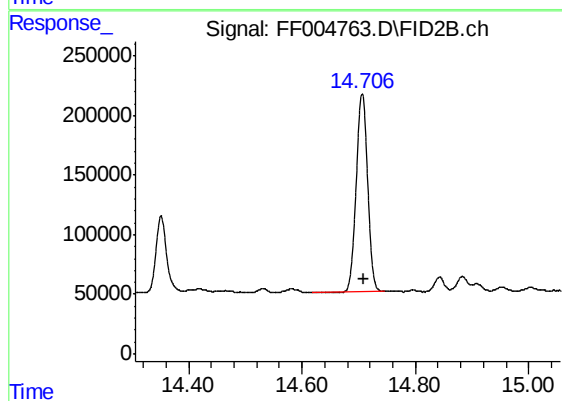


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.707 min
Delta R.T.: -0.002 min
Response: 2330166
Conc: 19.08 ug/ml

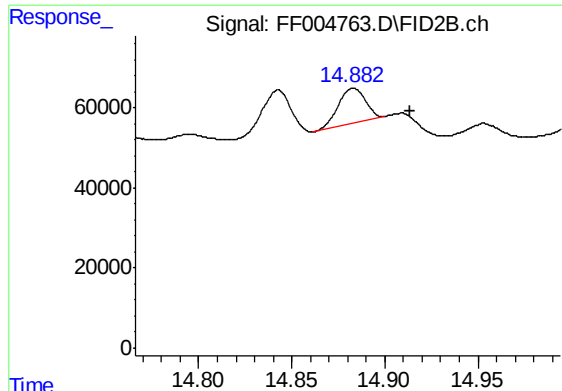


#10 N-TETRACOSANE

R.T.: 14.883 min
Delta R.T.: -0.030 min
Response: 87010
Conc: 0.63 ug/ml

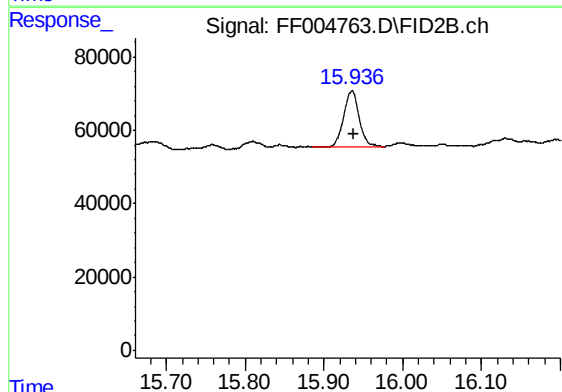


#11 N-HEXACOSANE

R.T.: 15.936 min
Delta R.T.: -0.002 min
Response: 206318
Conc: 1.51 ug/ml

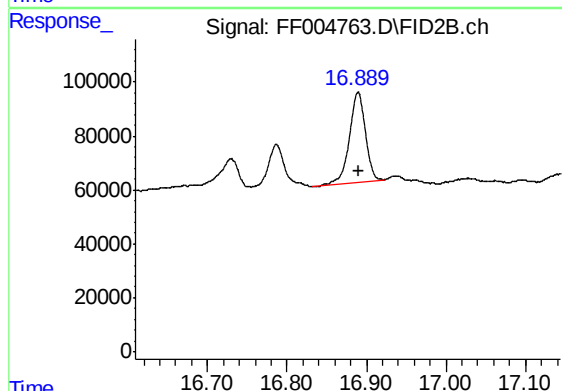


#12 N-OCTACOSANE

R.T.: 16.890 min
Delta R.T.: 0.000 min
Response: 466936
Conc: 3.43 ug/ml

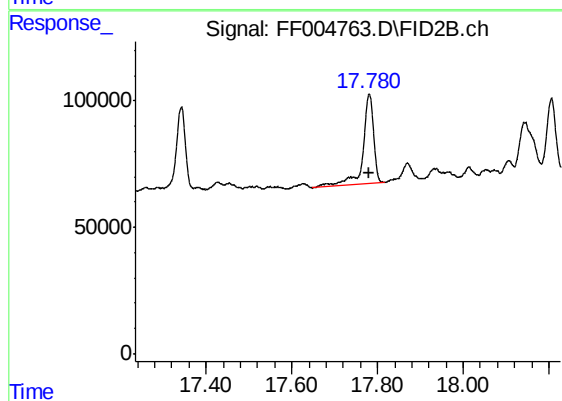


#13 N-TRIACONTANE

R.T.: 17.781 min
Delta R.T.: 0.000 min
Response: 621916
Conc: 4.50 ug/ml

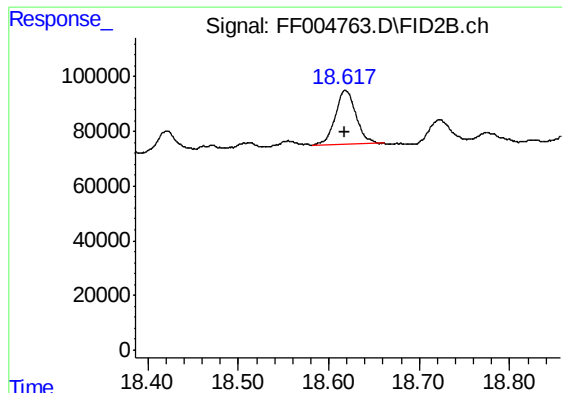


#14 N-DOTRIACONTANE

R.T.: 18.618 min
Delta R.T.: 0.000 min
Response: 316700
Conc: 2.29 ug/ml

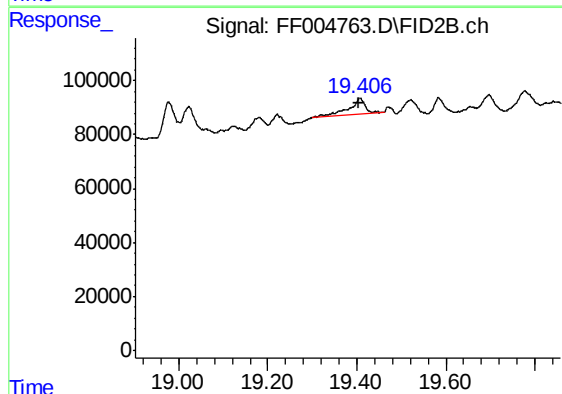


#15 N-TETRATRIACONTANE

R.T.: 19.407 min
Delta R.T.: 0.000 min
Response: 160601
Conc: 1.17 ug/ml

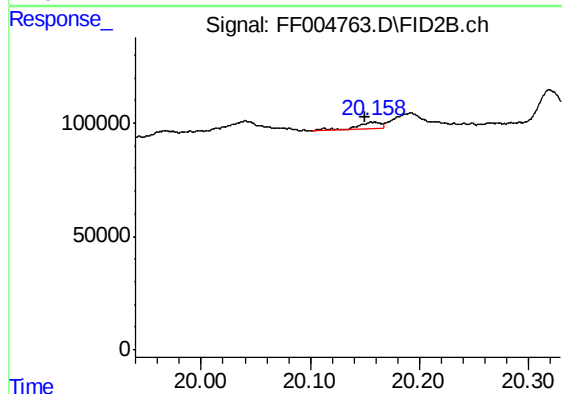

#16 N-HEXATRIACONTANE

R.T.: 20.158 min
Delta R.T.: 0.008 min
Response: 49725
Conc: 0.38 ug/ml

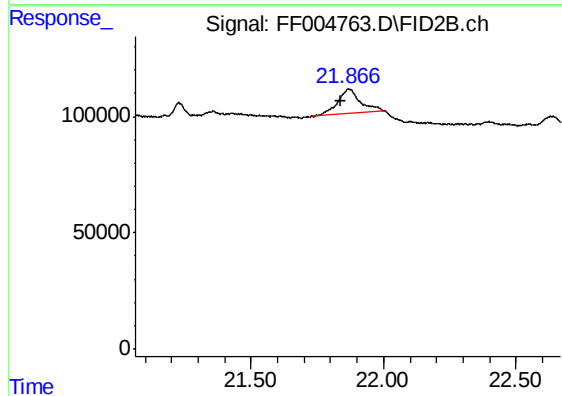

#18 N-TETRACONTANE

R.T.: 21.868 min
Delta R.T.: 0.031 min
Response: 635276
Conc: 5.16 ug/ml