

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061019\
 Data File : FF004767.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jun 2019 19:10
 Operator : DD\AJ
 Sample : K3265-08
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 11 01:42:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.708	2396747	19.628 ug/ml
Target Compounds			
2) N-DECANE	4.459	64534	0.441 ug/ml
4) N-TETRADECANE	8.292	399222	2.718 ug/ml
7) N-EICOSANE	12.601	119199	0.823 ug/ml
8) N-DOCOSANE	13.804	368024	2.604 ug/ml
10) N-TETRACOSANE	14.912	940979	6.790 ug/ml
11) N-HEXACOSANE	15.939	1920618	14.096 ug/ml
12) N-OCTACOSANE	16.893	1979071	14.556 ug/ml
13) N-TRIACONTANE	17.787	1763392	12.752 ug/ml
14) N-DOTRIACONTANE	18.623	1061037	7.670 ug/ml
15) N-TETRATRIACONTANE	19.413	572736	4.189 ug/ml
16) N-HEXATRIACONTANE	20.156	637486	4.842 ug/ml
17) N-OCTATRIACONTANE	20.914	408892	3.400 ug/ml
18) N-TETRACONTANE	21.860	432624	3.513 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061019\
Data File : FF004767.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2019 19:10
Operator : DD\AJ
Sample : K3265-08
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 11 01:42:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

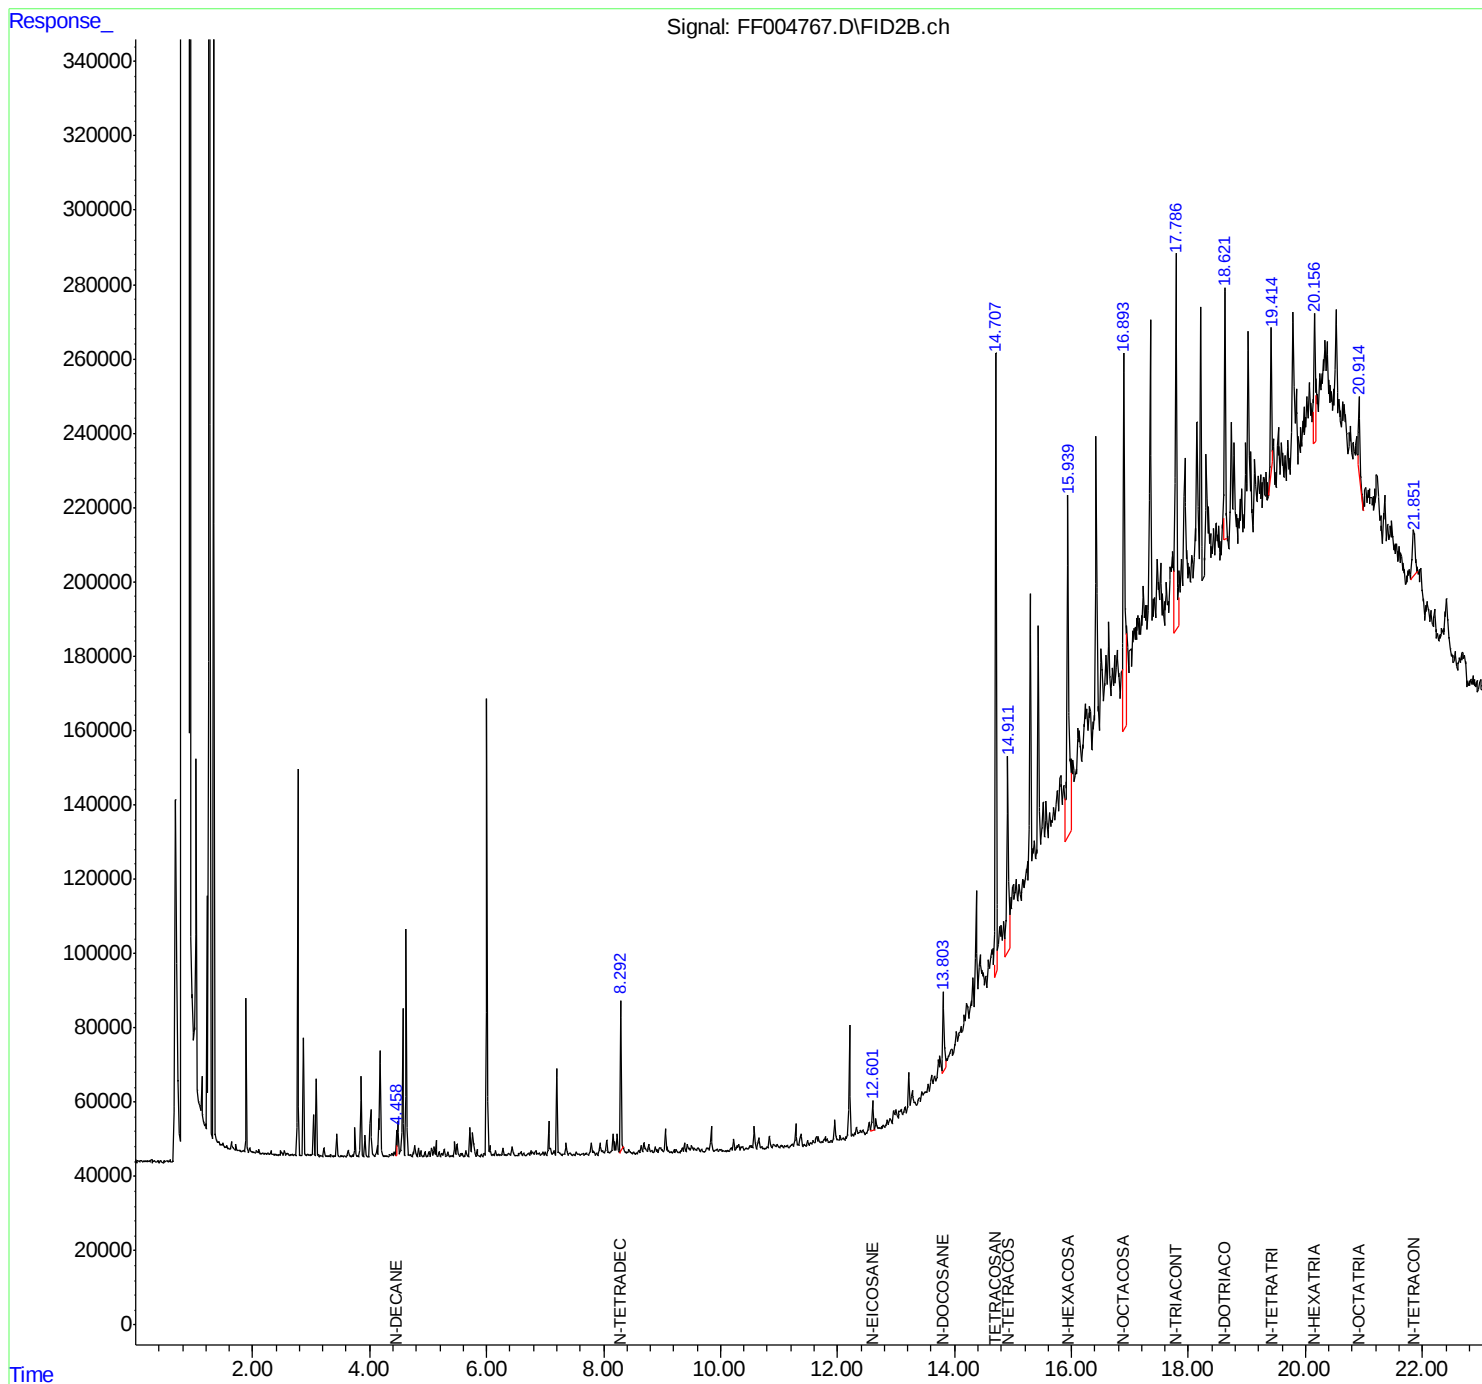

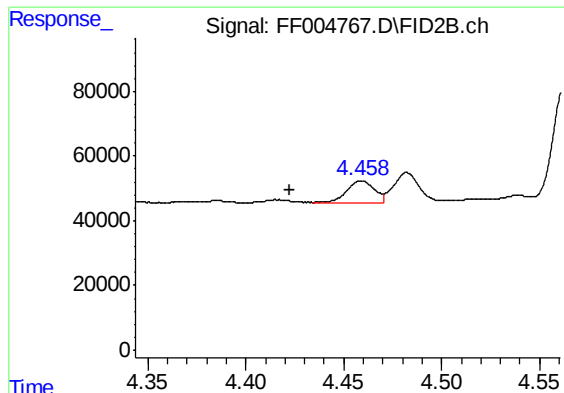


#2 N-DECANE

R.T.: 4.459 min
Delta R.T.: 0.036 min
Response: 64534
Conc: 0.44 ug/ml

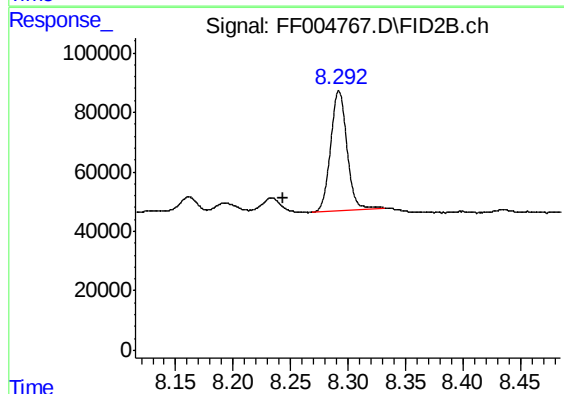


#4 N-TETRADECANE

R.T.: 8.292 min
Delta R.T.: 0.048 min
Response: 399222
Conc: 2.72 ug/ml

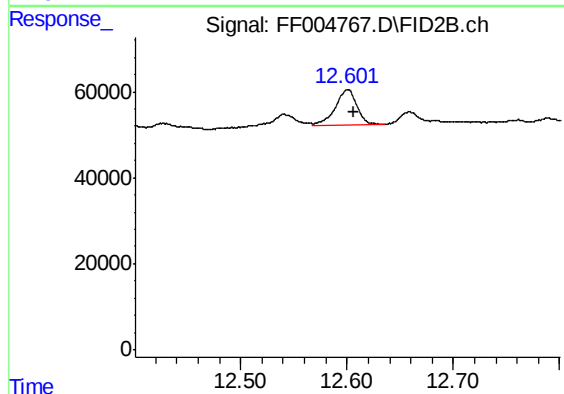


#7 N-EICOSANE

R.T.: 12.601 min
Delta R.T.: -0.005 min
Response: 119199
Conc: 0.82 ug/ml

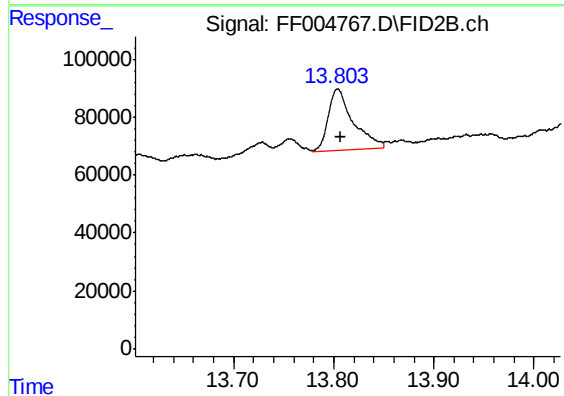


#8 N-DOCOSANE

R.T.: 13.804 min
Delta R.T.: -0.003 min
Response: 368024
Conc: 2.60 ug/ml

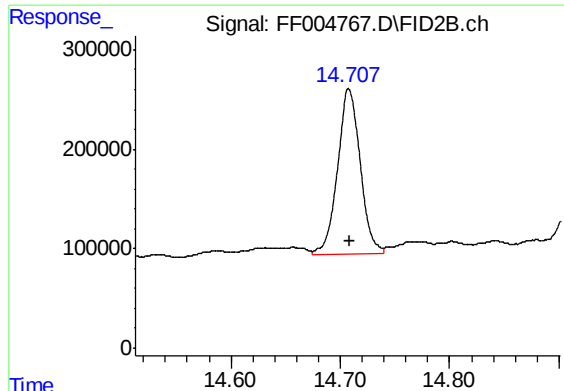


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.708 min
Delta R.T.: 0.000 min
Response: 2396747
Conc: 19.63 ug/ml

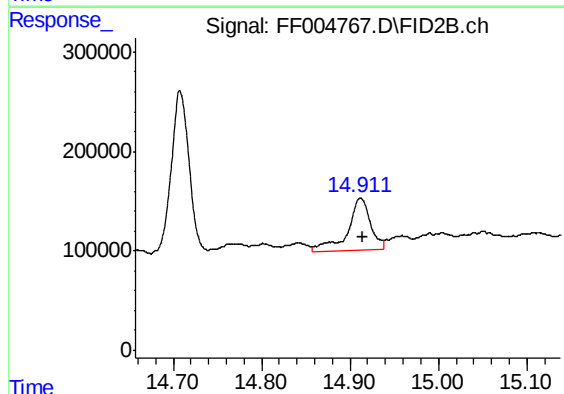


#10 N-TETRACOSANE

R.T.: 14.912 min
Delta R.T.: -0.002 min
Response: 940979
Conc: 6.79 ug/ml

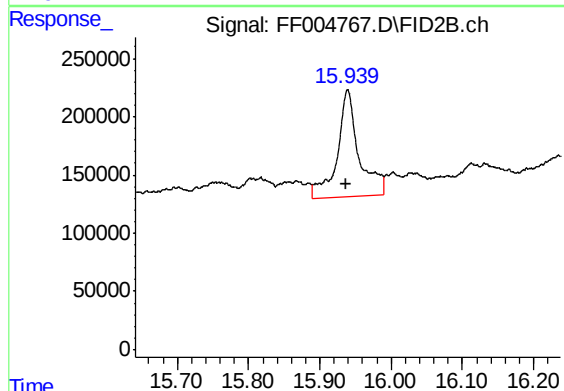


#11 N-HEXACOSANE

R.T.: 15.939 min
Delta R.T.: 0.001 min
Response: 1920618
Conc: 14.10 ug/ml

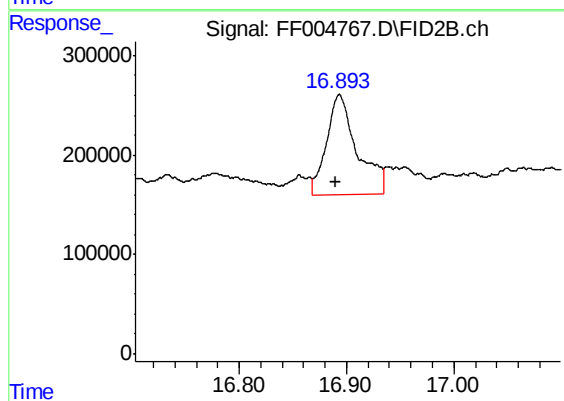


#12 N-OCTACOSANE

R.T.: 16.893 min
Delta R.T.: 0.004 min
Response: 1979071
Conc: 14.56 ug/ml

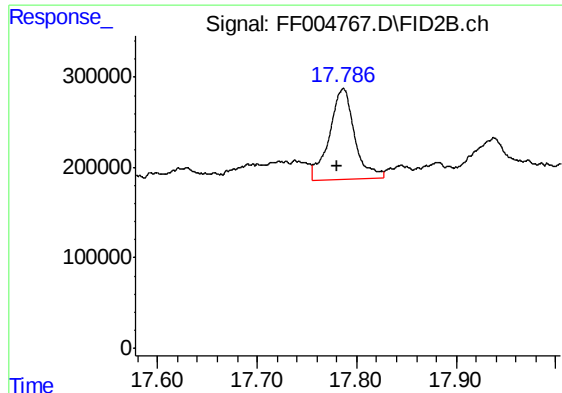


#13 N-TRIACONTANE

R.T.: 17.787 min
Delta R.T.: 0.006 min
Response: 1763392
Conc: 12.75 ug/ml

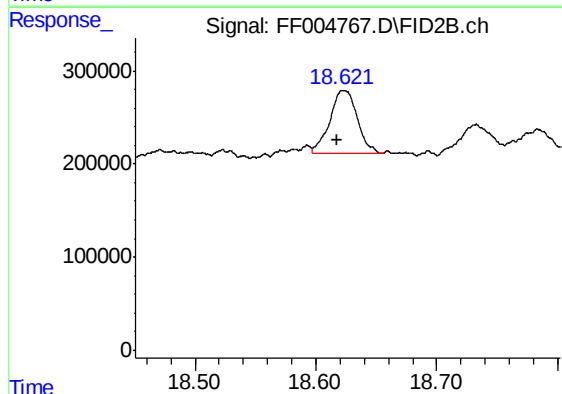


#14 N-DOTRIACONTANE

R.T.: 18.623 min
Delta R.T.: 0.006 min
Response: 1061037
Conc: 7.67 ug/ml

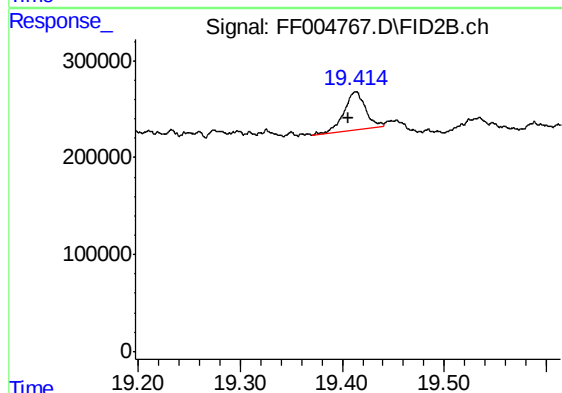


#15 N-TETRATRIACONTANE

R.T.: 19.413 min
Delta R.T.: 0.008 min
Response: 572736
Conc: 4.19 ug/ml

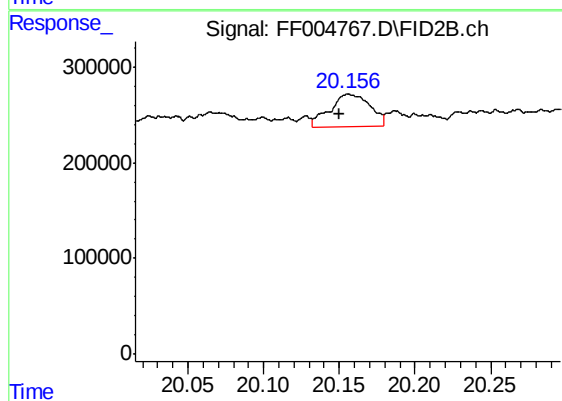


#16 N-HEXATRIACONTANE

R.T.: 20.156 min
Delta R.T.: 0.005 min
Response: 637486
Conc: 4.84 ug/ml

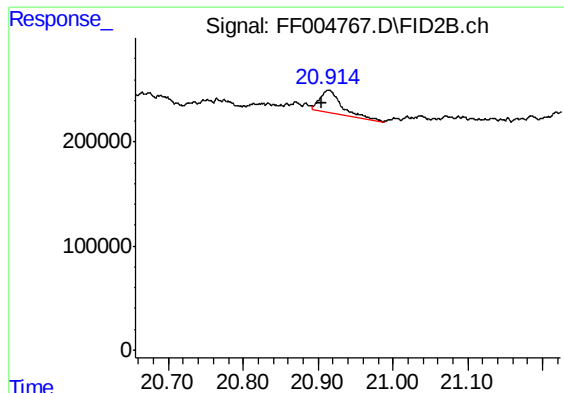

#17 N-OCTATRIACONTANE

R.T.: 20.914 min
Delta R.T.: 0.009 min
Response: 408892
Conc: 3.40 ug/ml

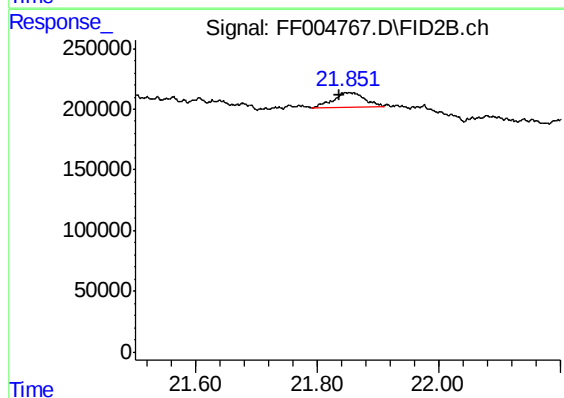

#18 N-TETRACONTANE

R.T.: 21.860 min
Delta R.T.: 0.023 min
Response: 432624
Conc: 3.51 ug/ml