

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061019\
 Data File : FF004768.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jun 2019 19:40
 Operator : DD\AJ
 Sample : K3163-05 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 11 01:42:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.706	223398	1.829 ug/ml
Target Compounds			
6) N-OCTADECANE	11.284	111043	0.765 ug/ml
7) N-EICOSANE	12.601	161039	1.112 ug/ml
8) N-DOCOSANE	13.803	83631	0.592 ug/ml
10) N-TETRACOSANE	14.885	481366	3.473 ug/ml
11) N-HEXACOSANE	15.937	149479	1.097 ug/ml
12) N-OCTACOSANE	16.892	434434	3.195 ug/ml
13) N-TRIACONTANE	17.785	457833	3.311 ug/ml
14) N-DOTRIACONTANE	18.623	328621	2.376 ug/ml
15) N-TETRATRIACONTANE	19.414	136023	0.995 ug/ml
16) N-HEXATRIACONTANE	20.155	87738	0.666 ug/ml
17) N-OCTATRIACONTANE	20.907	631296	5.250 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061019\
Data File : FF004768.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2019 19:40
Operator : DD\AJ
Sample : K3163-05 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 11 01:42:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

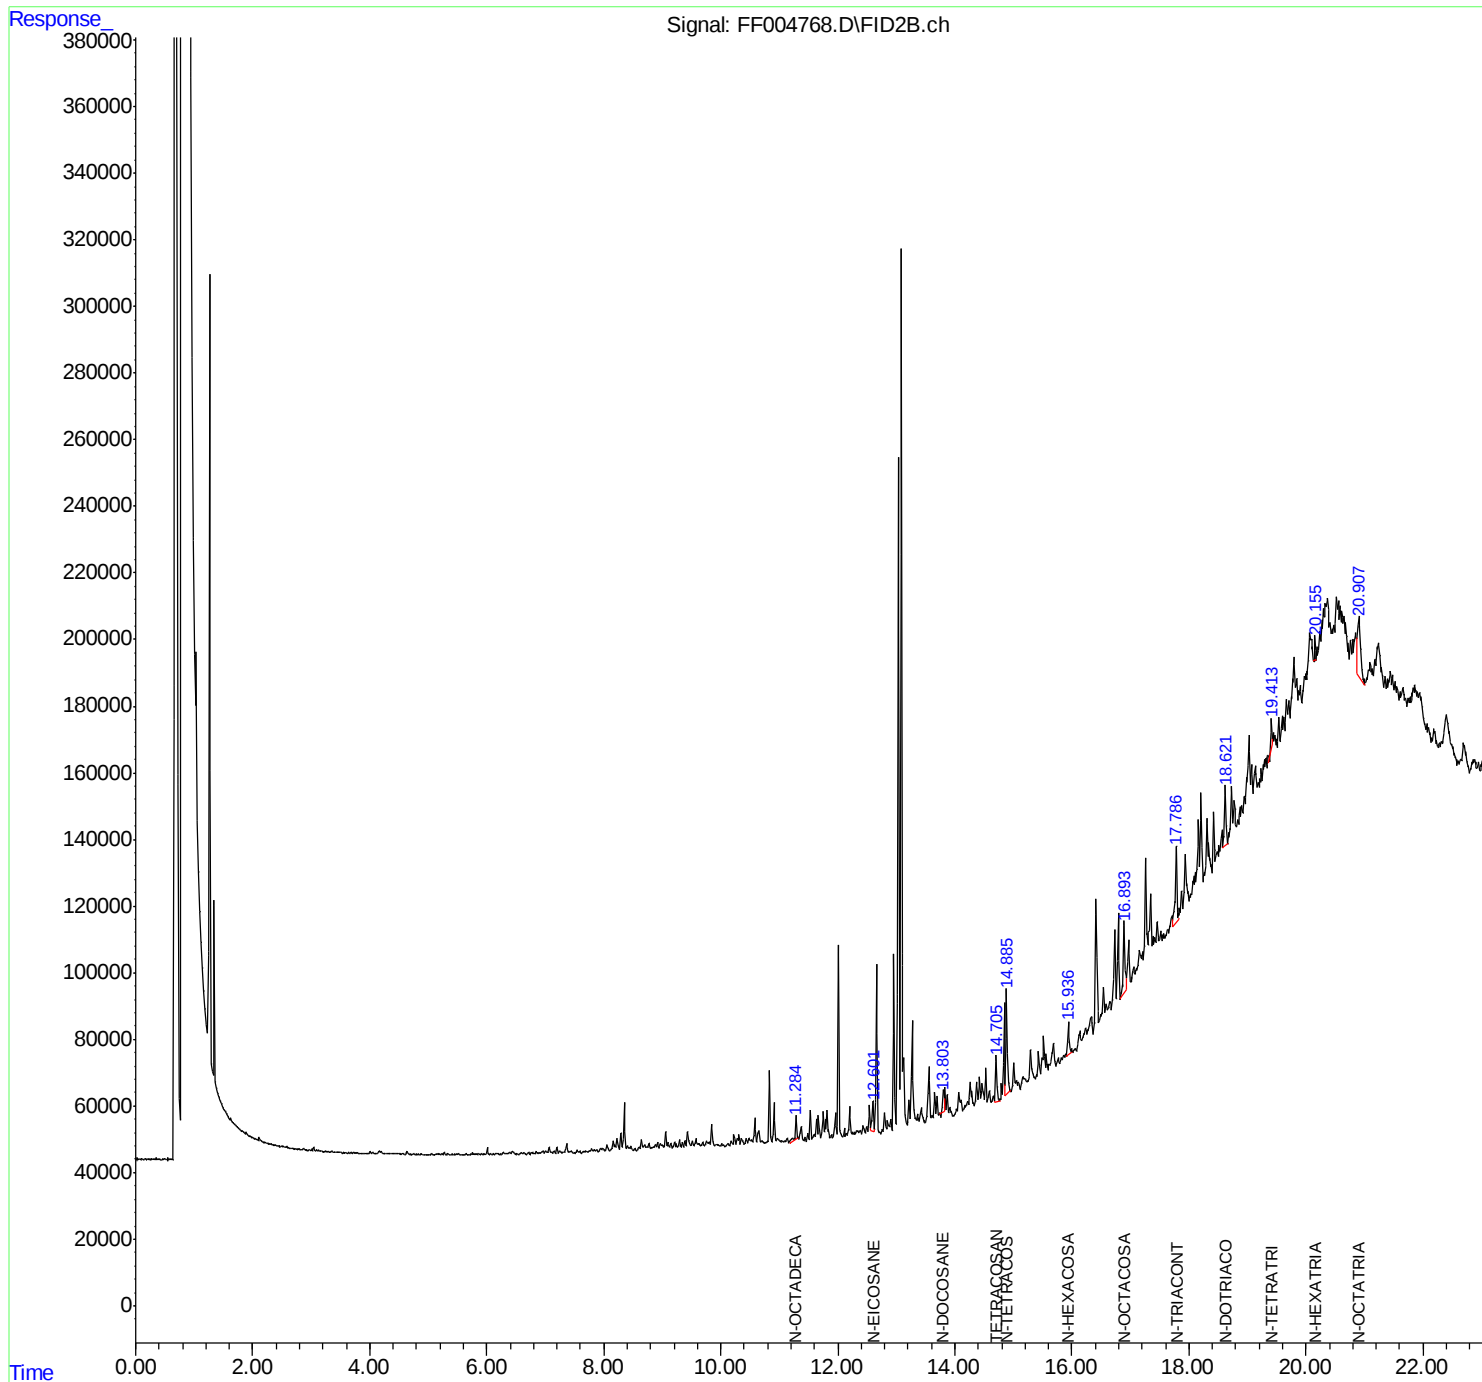

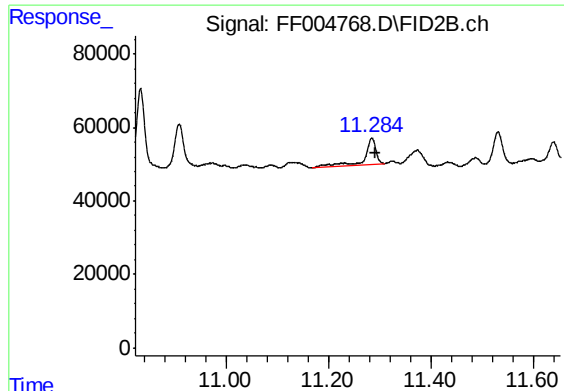


#6 N-OCTADECANE

R.T.: 11.284 min
Delta R.T.: -0.007 min
Response: 111043
Conc: 0.76 ug/ml

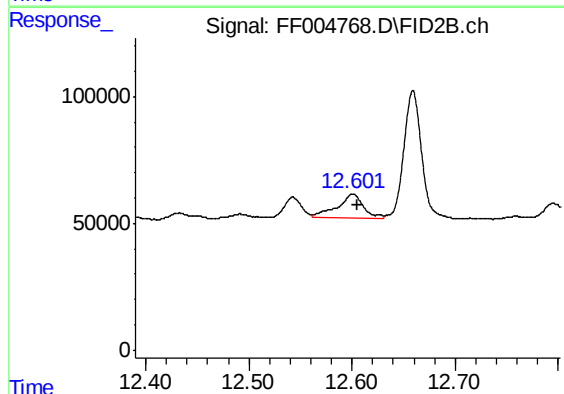


#7 N-EICOSANE

R.T.: 12.601 min
Delta R.T.: -0.005 min
Response: 161039
Conc: 1.11 ug/ml

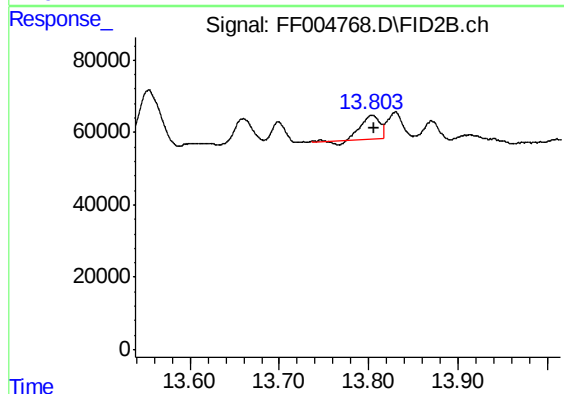


#8 N-DOCOSANE

R.T.: 13.803 min
Delta R.T.: -0.003 min
Response: 83631
Conc: 0.59 ug/ml

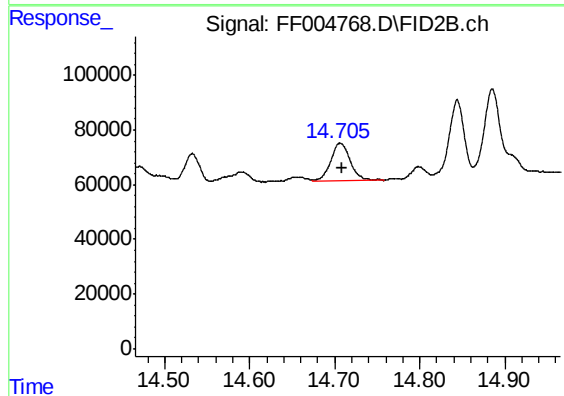


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.706 min
Delta R.T.: -0.002 min
Response: 223398
Conc: 1.83 ug/ml

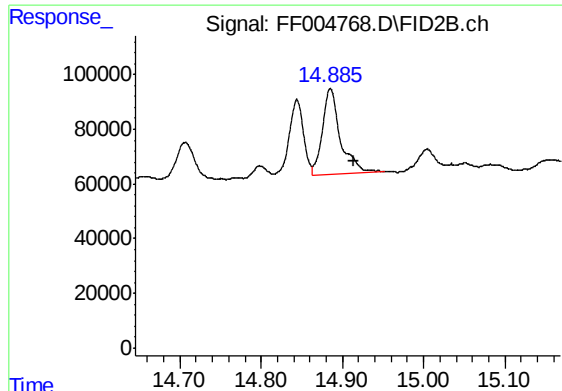


#10 N-TETRACOSANE

R.T.: 14.885 min
Delta R.T.: -0.028 min
Response: 481366
Conc: 3.47 ug/ml

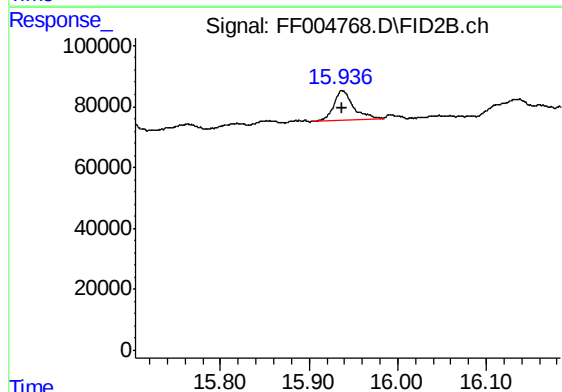


#11 N-HEXACOSANE

R.T.: 15.937 min
Delta R.T.: 0.000 min
Response: 149479
Conc: 1.10 ug/ml

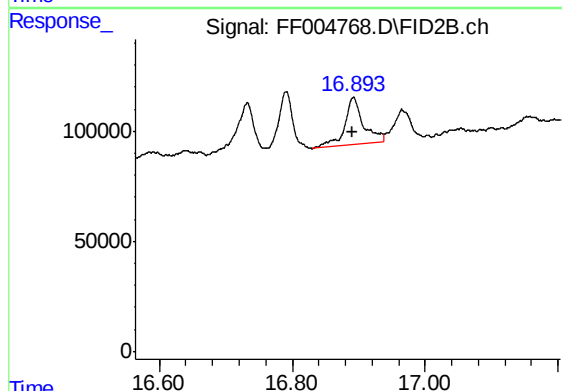


#12 N-OCTACOSANE

R.T.: 16.892 min
Delta R.T.: 0.002 min
Response: 434434
Conc: 3.20 ug/ml

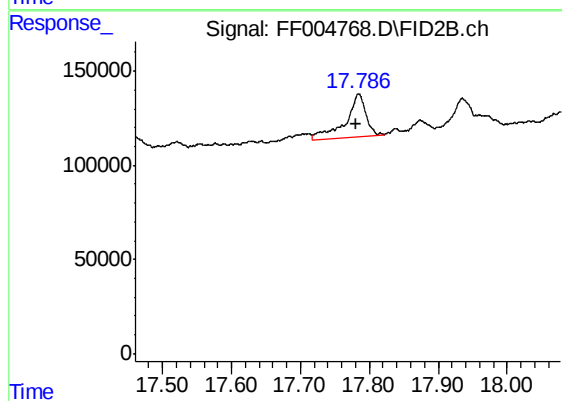


#13 N-TRIACONTANE

R.T.: 17.785 min
Delta R.T.: 0.004 min
Response: 457833
Conc: 3.31 ug/ml

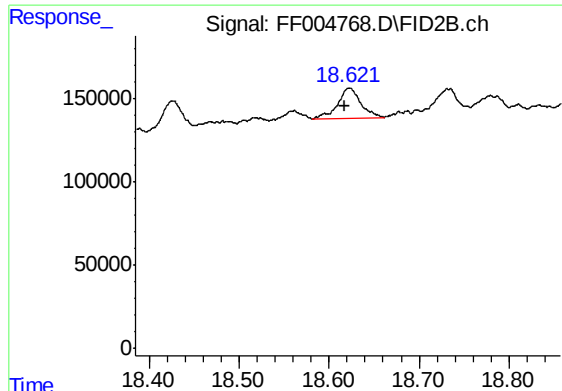


#14 N-DOTRIACONTANE

R.T.: 18.623 min
Delta R.T.: 0.005 min
Response: 328621
Conc: 2.38 ug/ml

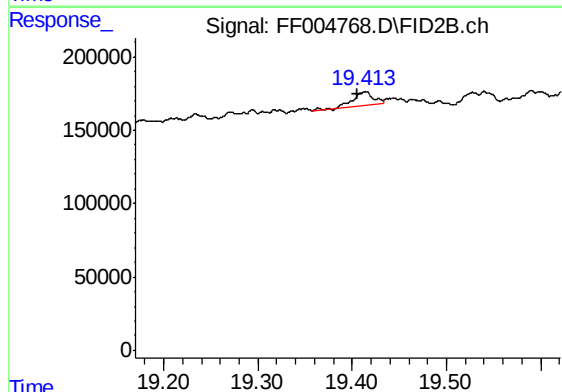


#15 N-TETRATRIACONTANE

R.T.: 19.414 min
Delta R.T.: 0.009 min
Response: 136023
Conc: 0.99 ug/ml

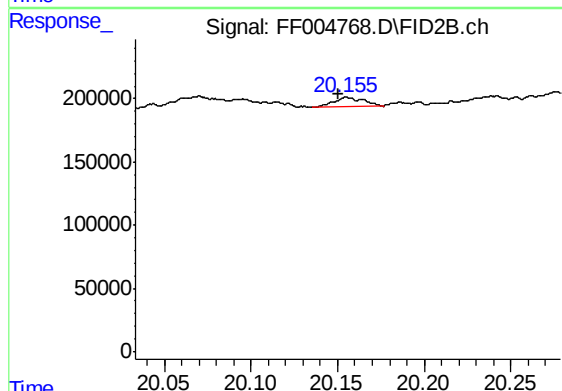

#16 N-HEXATRIACONTANE

R.T.: 20.155 min
Delta R.T.: 0.005 min
Response: 87738
Conc: 0.67 ug/ml

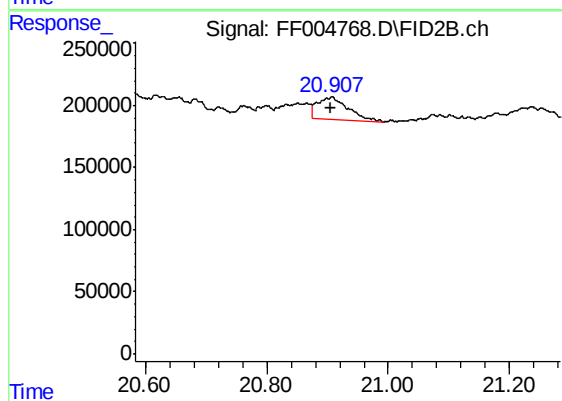

#17 N-OCTATRIACONTANE

R.T.: 20.907 min
Delta R.T.: 0.002 min
Response: 631296
Conc: 5.25 ug/ml