

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061019\
Data File : FF004770.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2019 20:39
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 11 01:42:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.707	2076272	17.003 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.781	101833	0.736 ug/ml
14)	N-DOTRIACONTANE	18.626	268098	1.938 ug/ml
16)	N-HEXATRIACONTANE	20.152	181054	1.375 ug/ml
18)	N-TETRACONTANE	21.870	509820	4.140 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061019\
Data File : FF004770.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2019 20:39
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 11 01:42:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

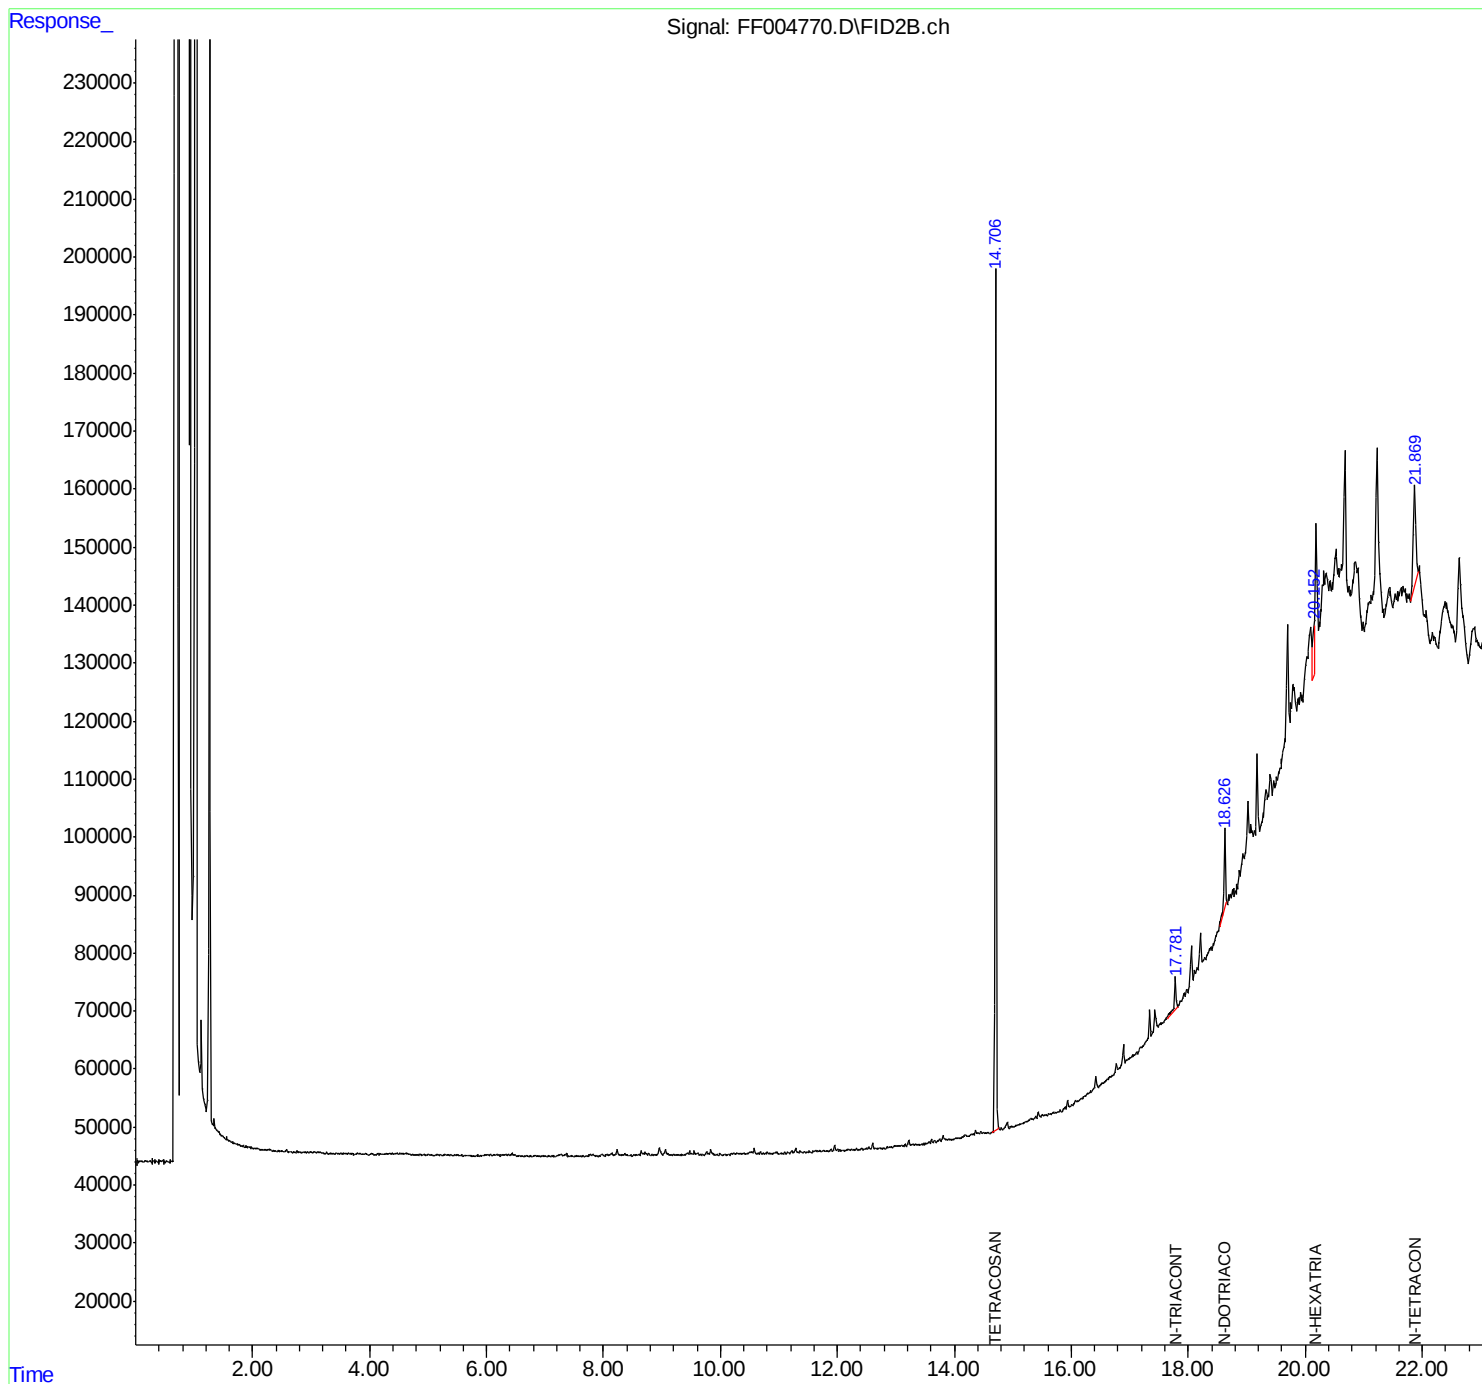

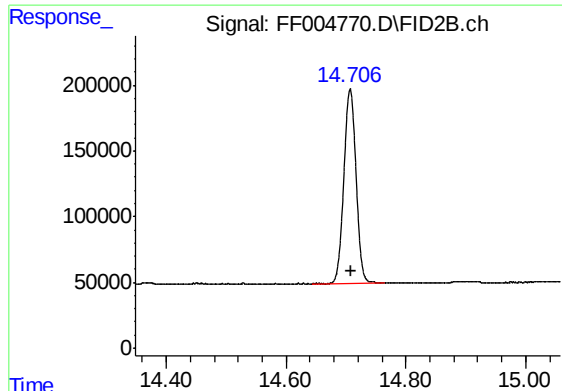


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.707 min
Delta R.T.: -0.001 min
Response: 2076272
Conc: 17.00 ug/ml

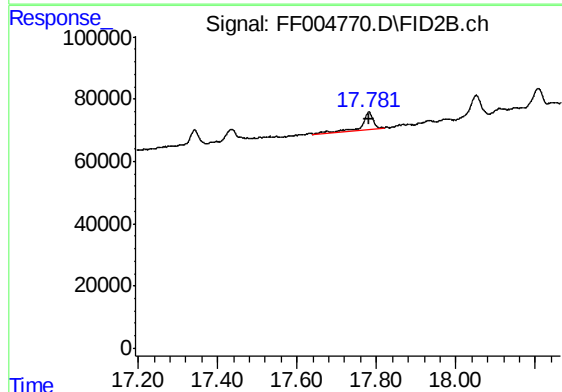


#13 N-TRIACONTANE

R.T.: 17.781 min
Delta R.T.: 0.000 min
Response: 101833
Conc: 0.74 ug/ml

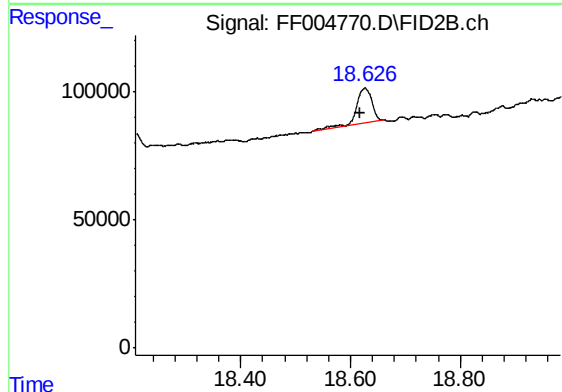


#14 N-DOTRIACONTANE

R.T.: 18.626 min
Delta R.T.: 0.009 min
Response: 268098
Conc: 1.94 ug/ml

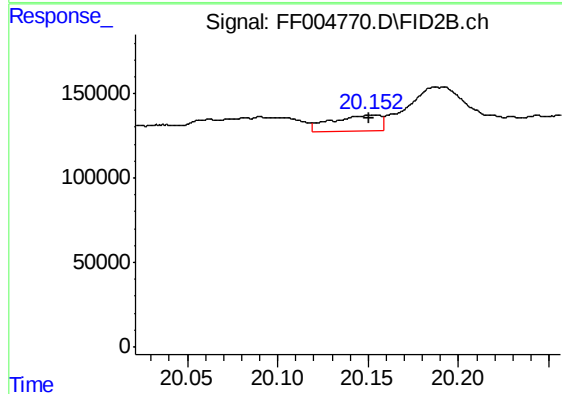

#16 N-HEXATRIACONTANE

R.T.: 20.152 min
Delta R.T.: 0.002 min
Response: 181054
Conc: 1.38 ug/ml

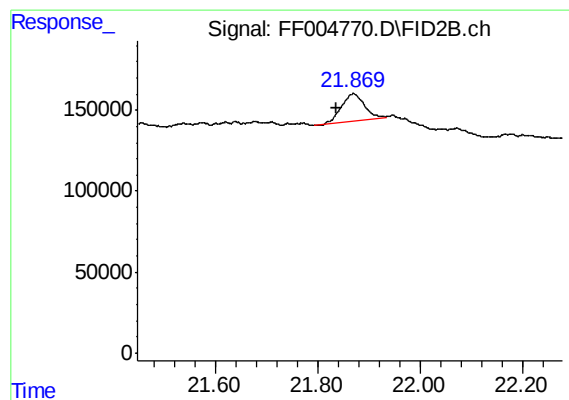

#18 N-TETRACONTANE

R.T.: 21.870 min
Delta R.T.: 0.033 min
Response: 509820
Conc: 4.14 ug/ml