

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061019\
 Data File : FF004758.D
 Signal(s) : FID2B.ch
 Acq On : 10 Jun 2019 14:25
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Jun 11 01:40:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.711	6106057	50.004 ug/ml
Target Compounds			
2) N-DECANE	4.417	8001141	54.641 ug/ml
3) N-DODECANE	6.442	7832822	52.931 ug/ml
4) N-TETRADECANE	8.239	7565230	51.503 ug/ml
5) N-HEXADECANE	9.844	7403134	50.141 ug/ml
6) N-OCTADECANE	11.290	7145289	49.216 ug/ml
7) N-EICOSANE	12.604	7056024	48.720 ug/ml
8) N-DOCOSANE	13.808	6943018	49.135 ug/ml
10) N-TETRACOSANE	14.916	6962413	50.239 ug/ml
11) N-HEXACOSANE	15.941	6983288	51.252 ug/ml
12) N-OCTACOSANE	16.896	7092360	52.165 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061019\
Data File : FF004758.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2019 14:25
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Jun 11 01:40:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

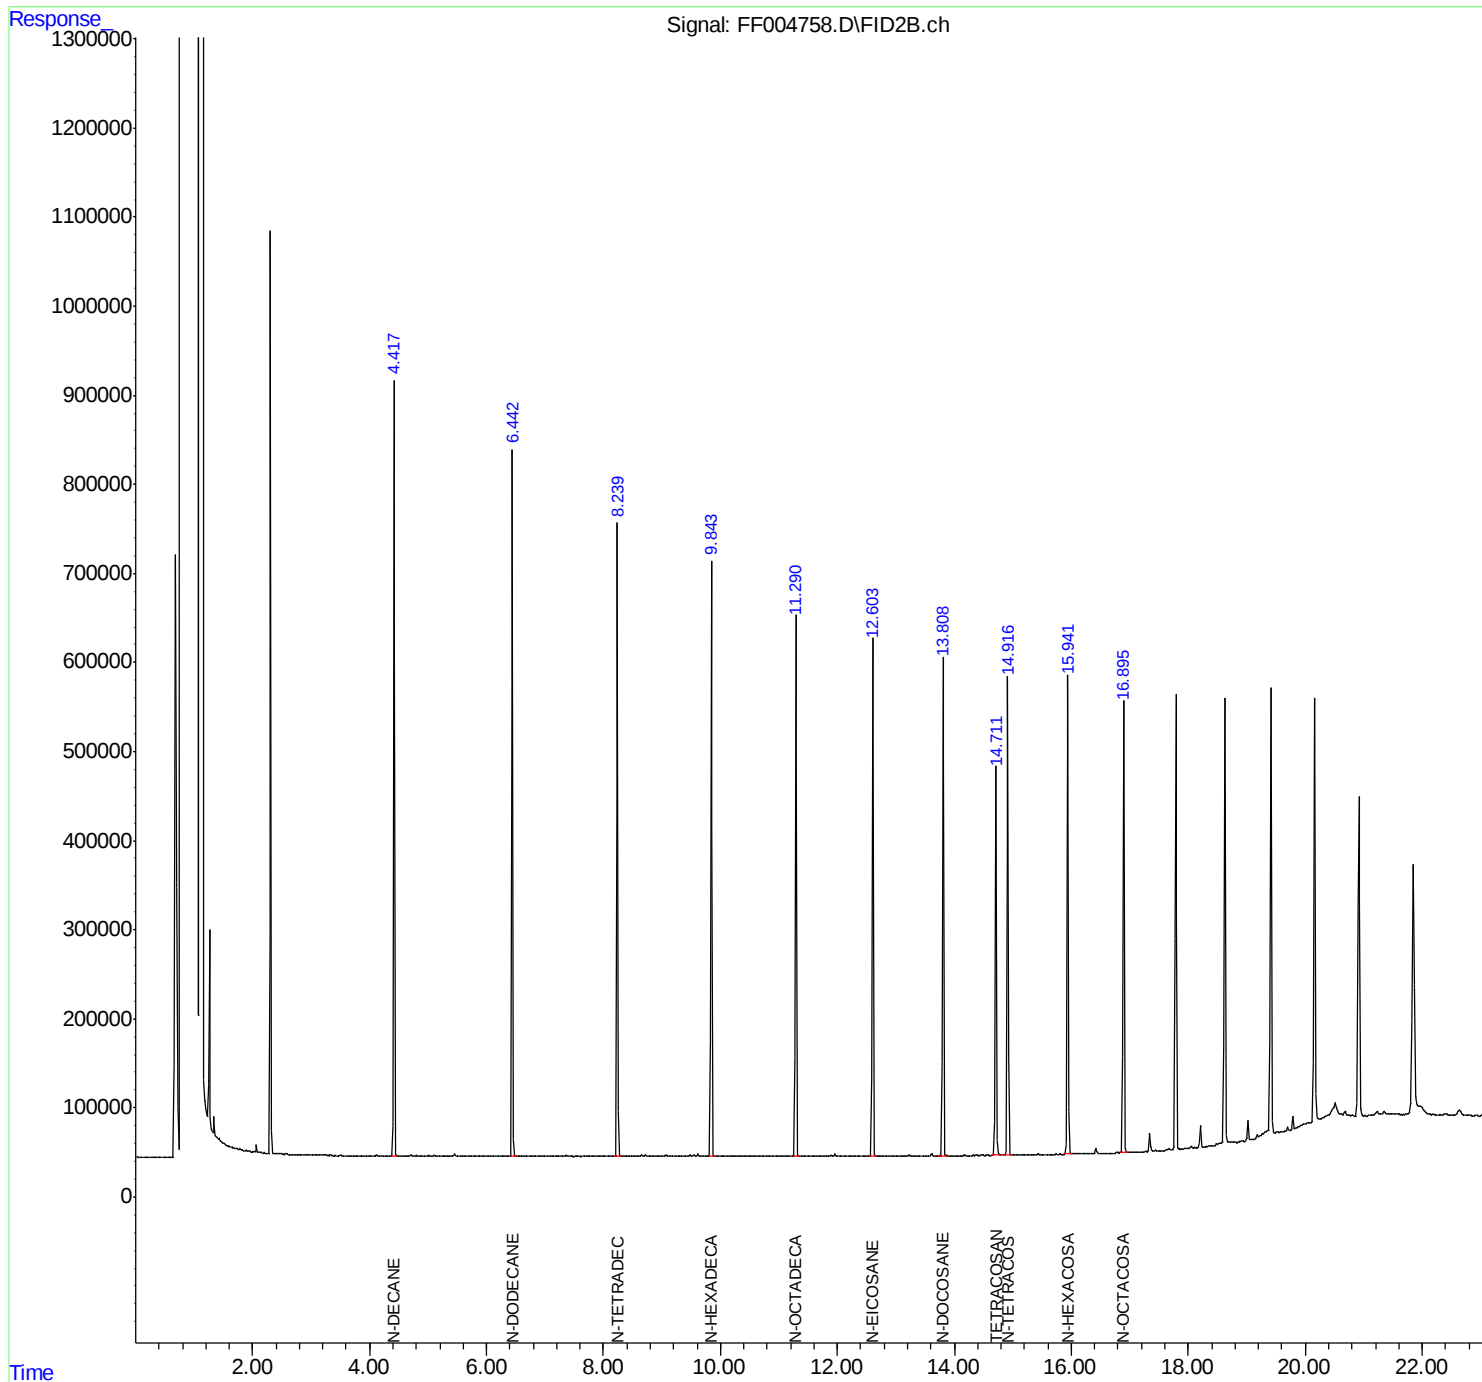

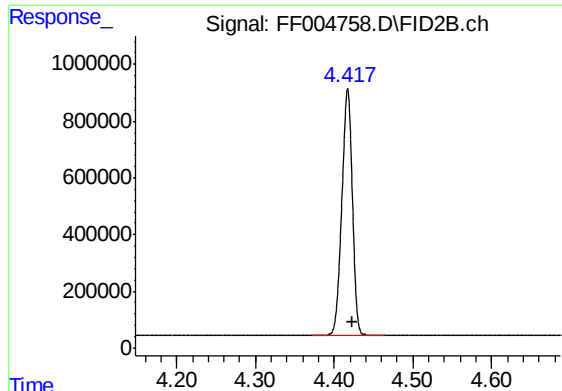


#2 N-DECANE

R.T.: 4.417 min
Delta R.T.: -0.005 min
Response: 8001141
Conc: 54.64 ug/ml

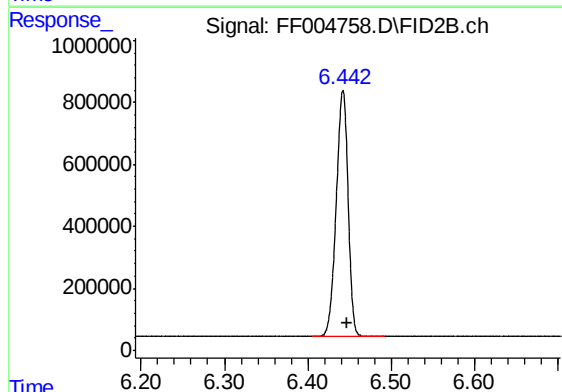


#3 N-DODECANE

R.T.: 6.442 min
Delta R.T.: -0.006 min
Response: 7832822
Conc: 52.93 ug/ml

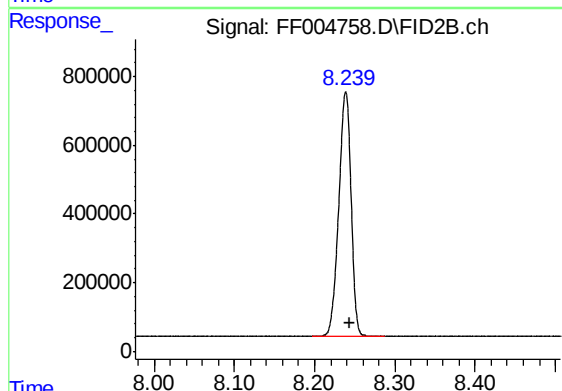


#4 N-TETRADECANE

R.T.: 8.239 min
Delta R.T.: -0.005 min
Response: 7565230
Conc: 51.50 ug/ml

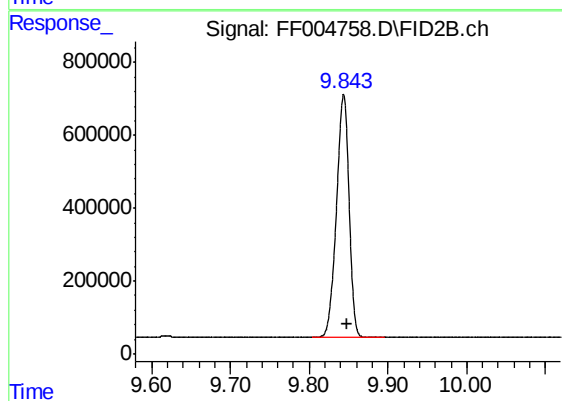


#5 N-HEXADECANE

R.T.: 9.844 min
Delta R.T.: -0.004 min
Response: 7403134
Conc: 50.14 ug/ml

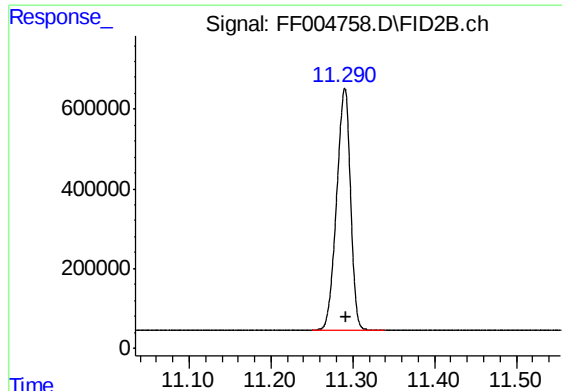


#6 N-OCTADECANE

R.T.: 11.290 min
Delta R.T.: -0.001 min
Response: 7145289
Conc: 49.22 ug/ml

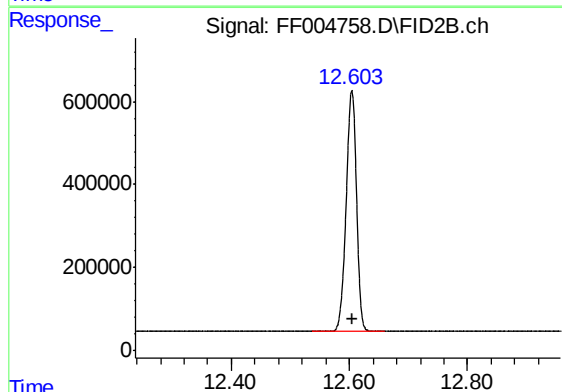


#7 N-EICOSANE

R.T.: 12.604 min
Delta R.T.: -0.002 min
Response: 7056024
Conc: 48.72 ug/ml

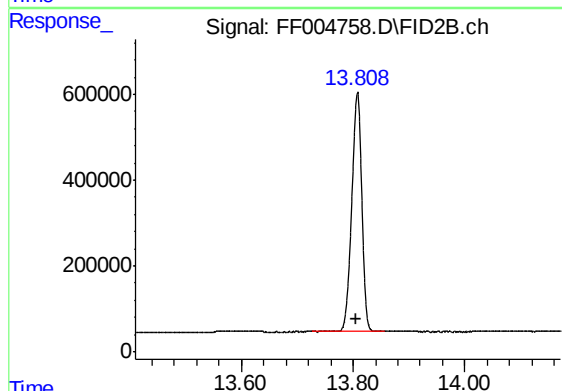


#8 N-DOCOSANE

R.T.: 13.808 min
Delta R.T.: 0.001 min
Response: 6943018
Conc: 49.13 ug/ml

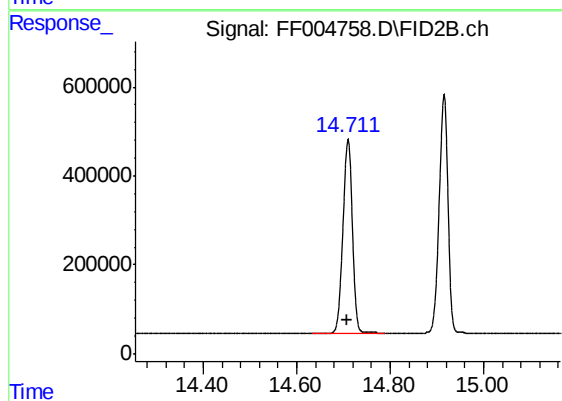


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.711 min
Delta R.T.: 0.002 min
Response: 6106057
Conc: 50.00 ug/ml

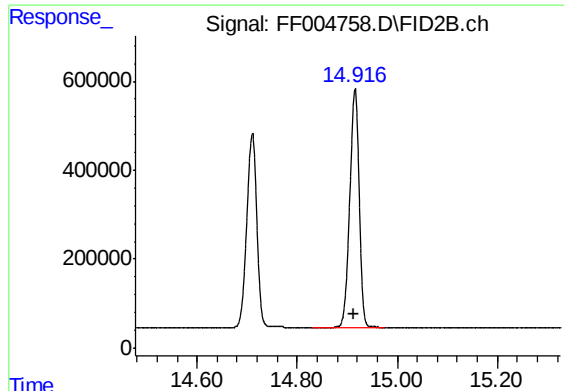


#10 N-TETRACOSANE

R.T.: 14.916 min
Delta R.T.: 0.002 min
Response: 6962413
Conc: 50.24 ug/ml

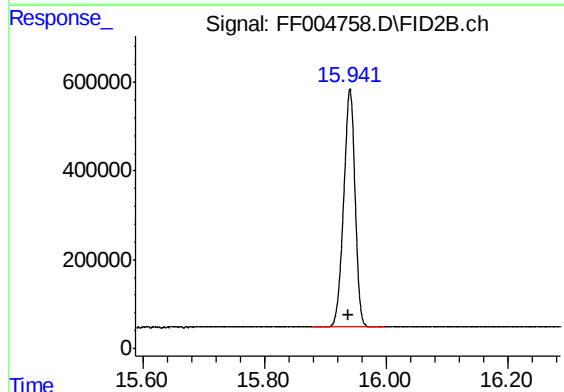

#11 N-HEXACOSANE

R.T.: 15.941 min
Delta R.T.: 0.003 min
Response: 6983288
Conc: 51.25 ug/ml

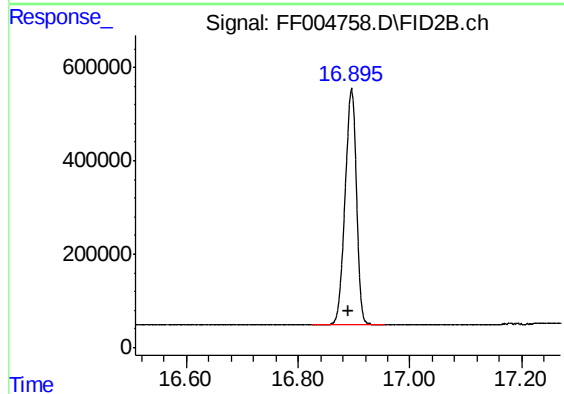

#12 N-OCTACOSANE

R.T.: 16.896 min
Delta R.T.: 0.006 min
Response: 7092360
Conc: 52.16 ug/ml