

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061022\
Data File : FF010744.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2022 12:14
Operator : AJ\MA
Sample : PB143240BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 10 23:33:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.823	2014630	17.823 ug/ml

Target Compounds


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061022\
Data File : FF010744.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2022 12:14
Operator : AJ\MA
Sample : PB143240BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 10 23:33:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

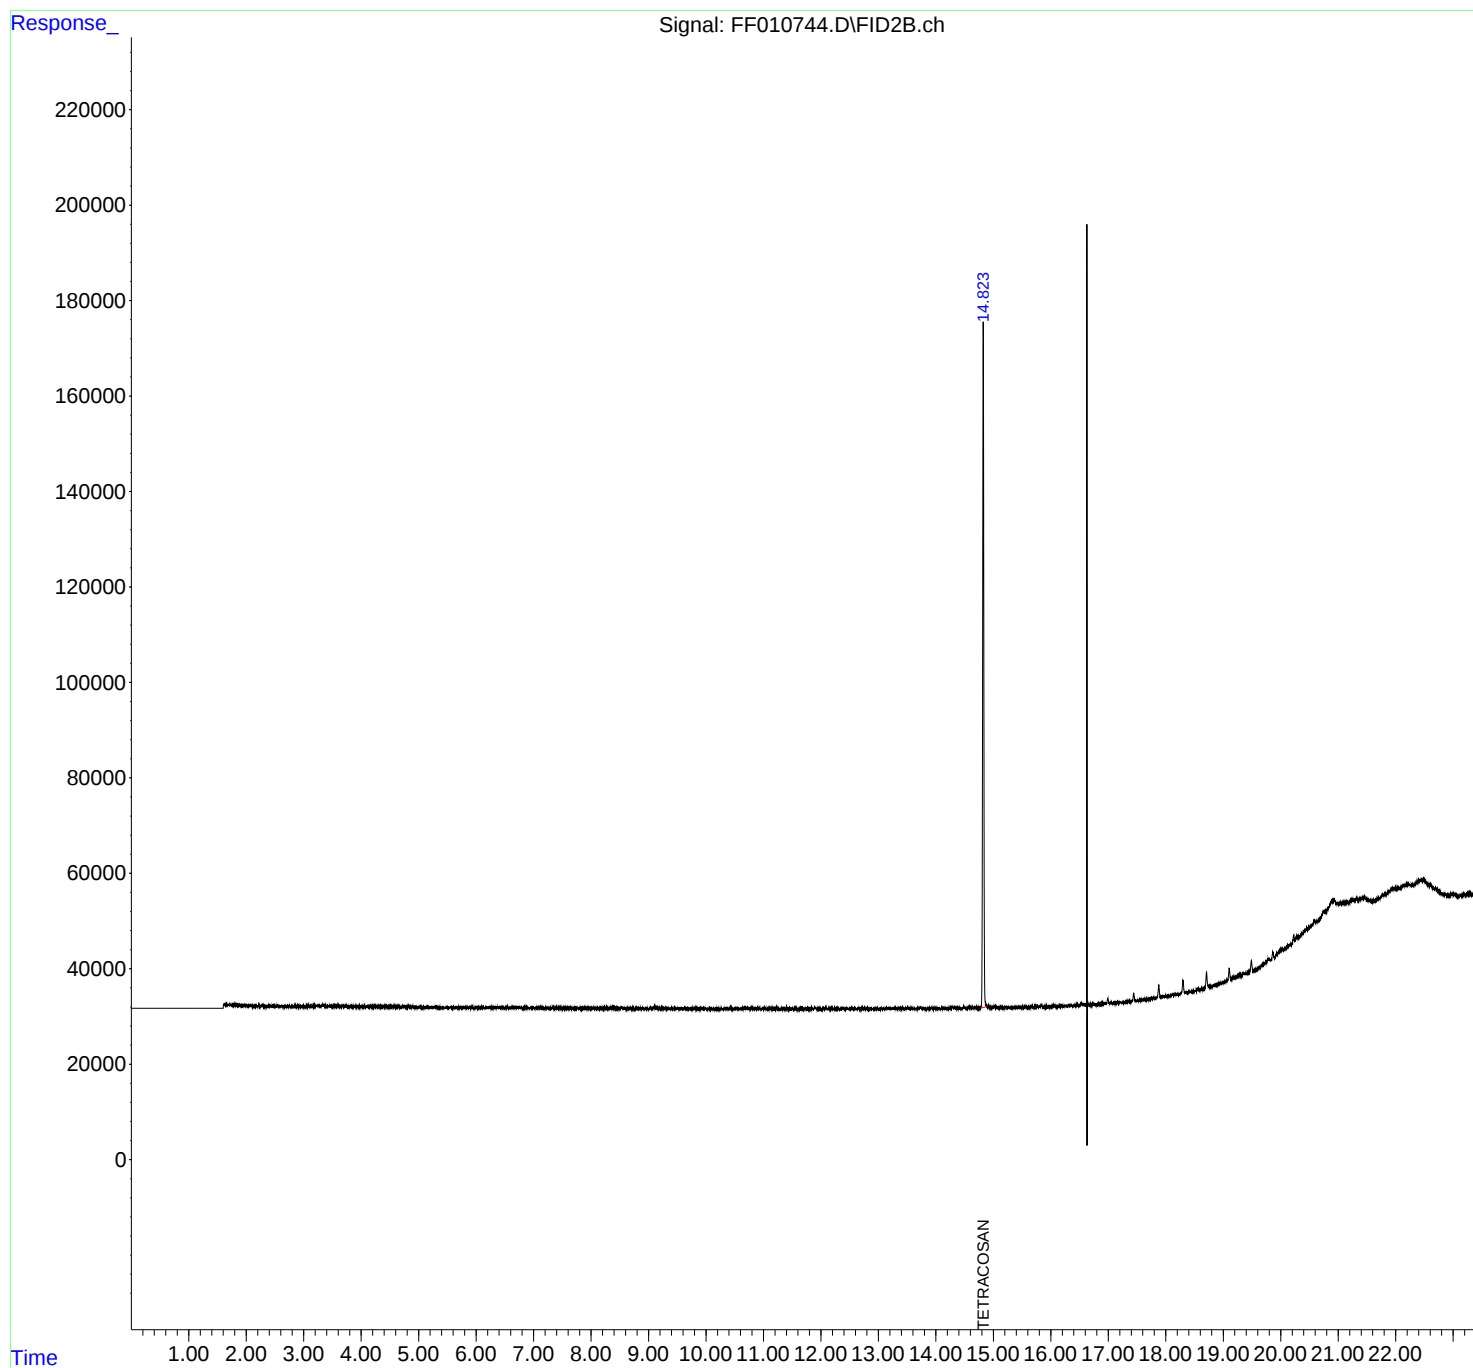

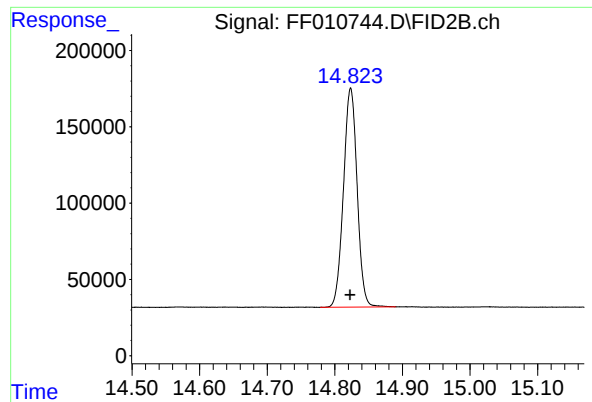

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.823 min
Delta R.T.: 0.000 min
Response: 2014630
Conc: 17.82 ug/ml