

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061025\
Data File : FF015922.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2025 17:04
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 11 04:44:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052125.M
Quant Title :
QLast Update : Wed May 21 12:32:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.028	1782043	14.591 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.939	68664	0.509 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061025\
Data File : FF015922.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2025 17:04
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 11 04:44:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052125.M
Quant Title :
QLast Update : Wed May 21 12:32:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

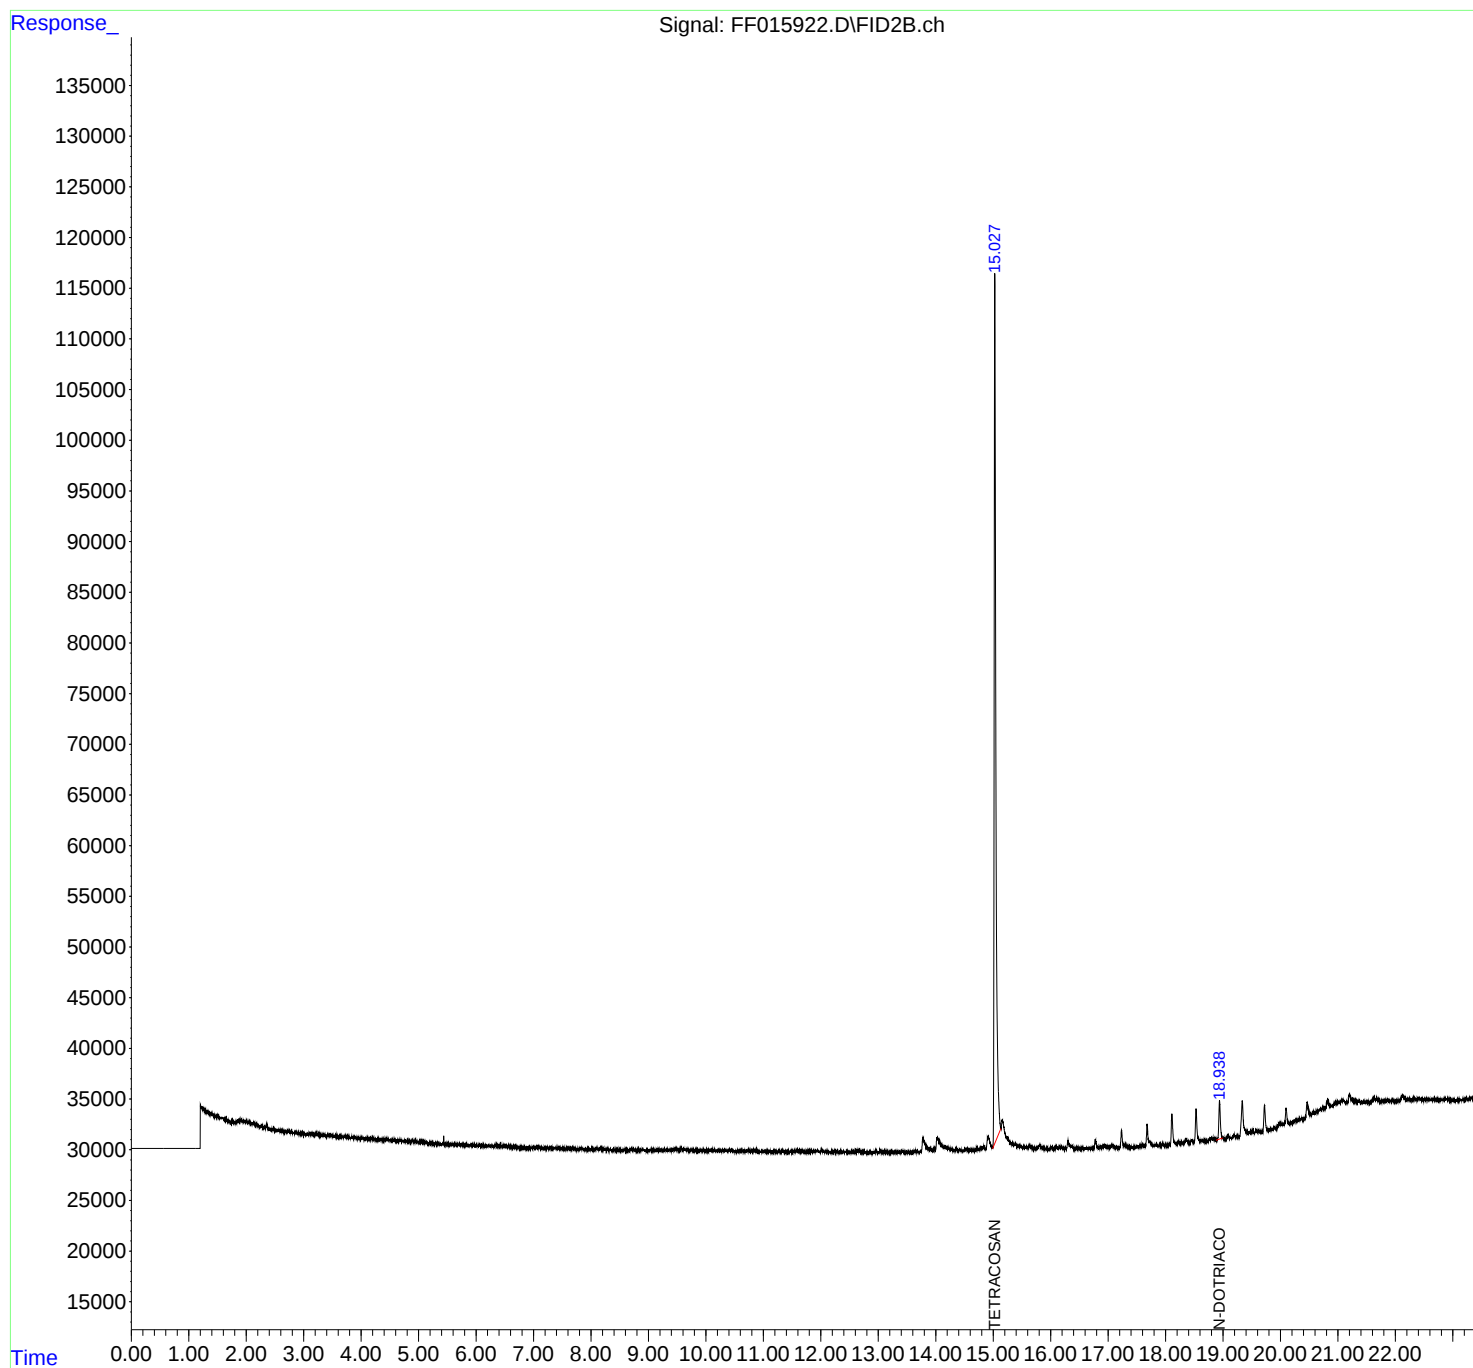


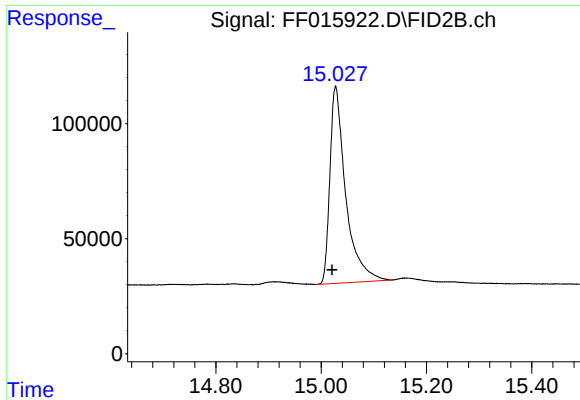

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.028 min
Delta R.T.: 0.007 min
Response: 1782043
Conc: 14.59 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

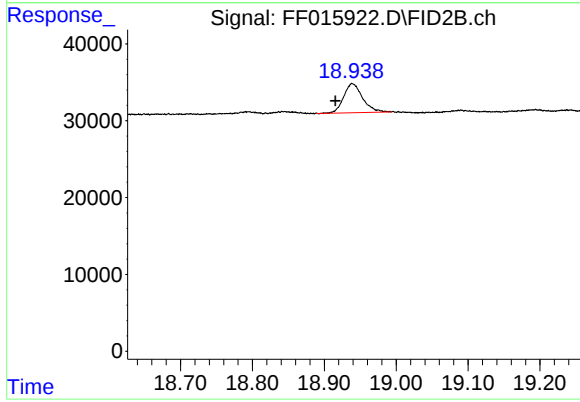

#14 N-DOTRIACONTANE

R.T.: 18.939 min
Delta R.T.: 0.023 min
Response: 68664
Conc: 0.51 ug/ml