

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061025\
Data File : FF015928.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2025 20:30
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 11 04:46:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052125.M
Quant Title :
QLast Update : Wed May 21 12:32:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.028	1824239	14.936 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.104	80504	0.578 ug/ml
14) N-DOTRIACONTANE	18.934	102429	0.759 ug/ml
15) N-TETRATRIACONTANE	19.718	71339	0.578 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061025\
Data File : FF015928.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2025 20:30
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 11 04:46:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052125.M
Quant Title :
QLast Update : Wed May 21 12:32:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

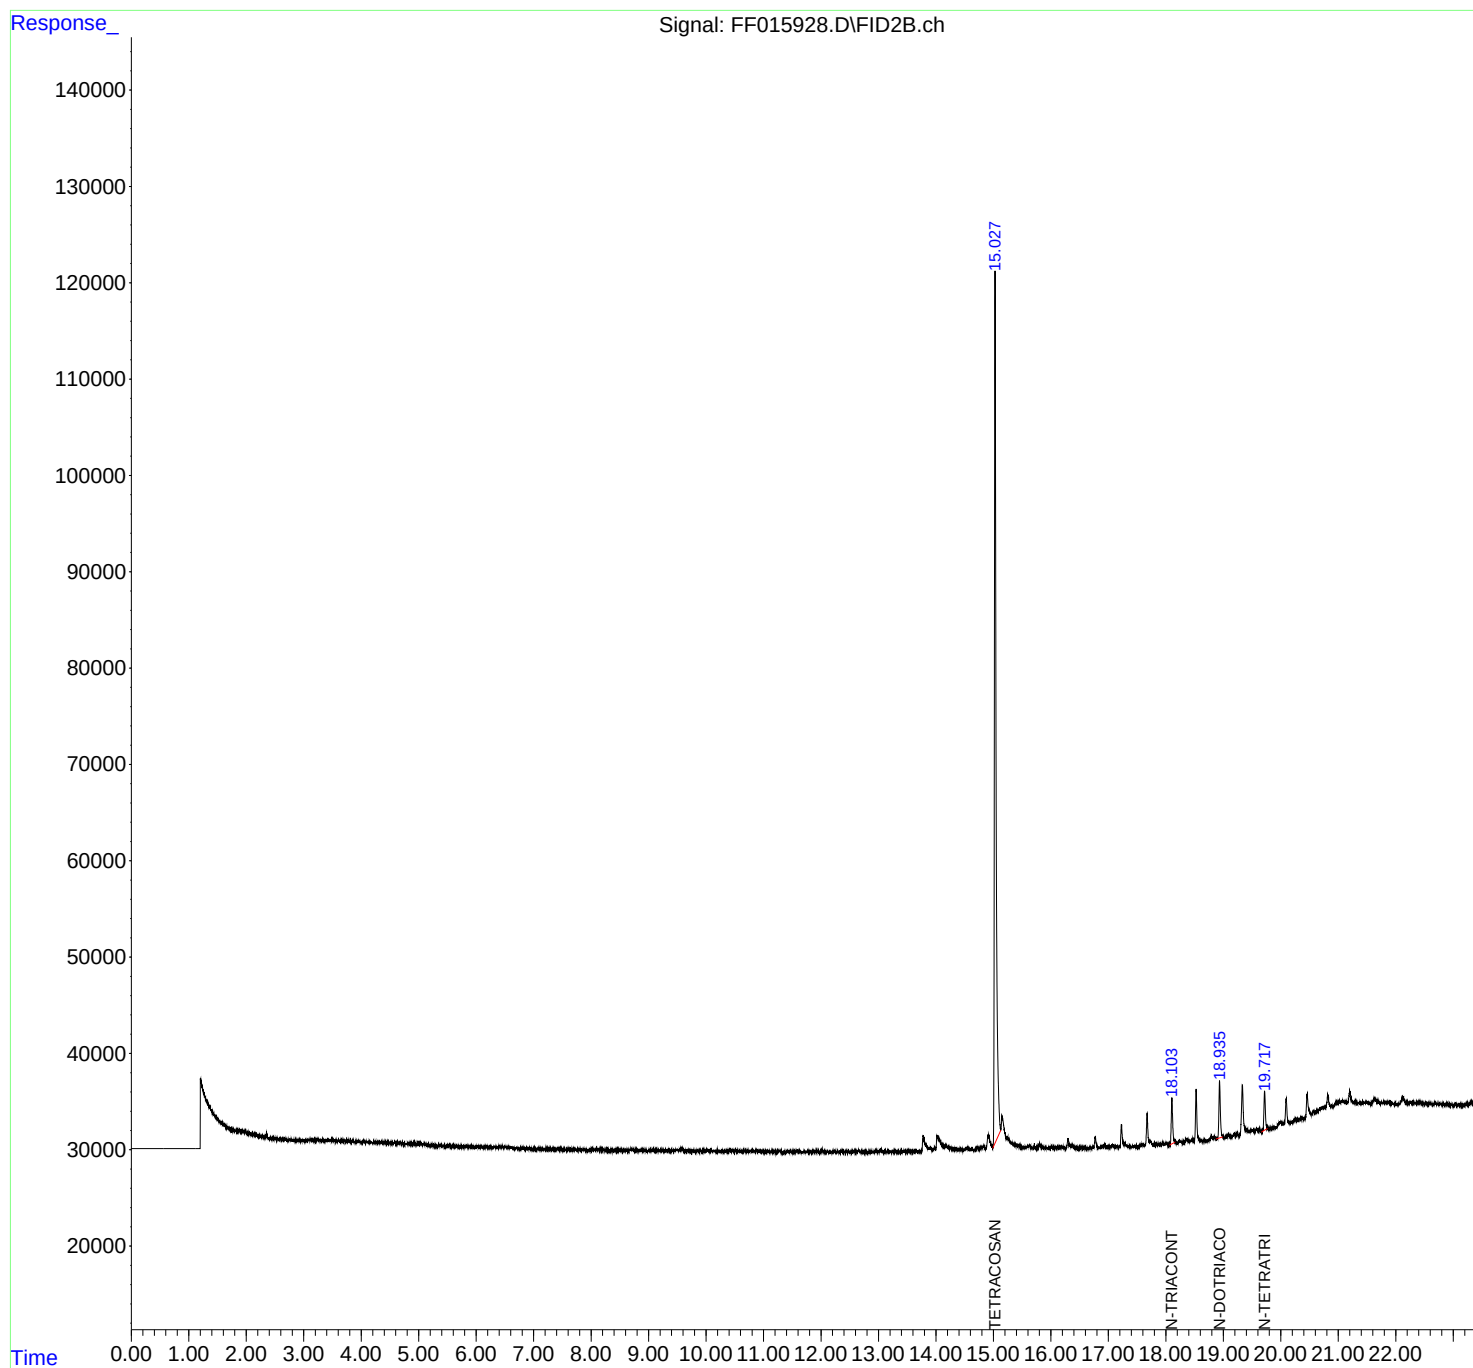


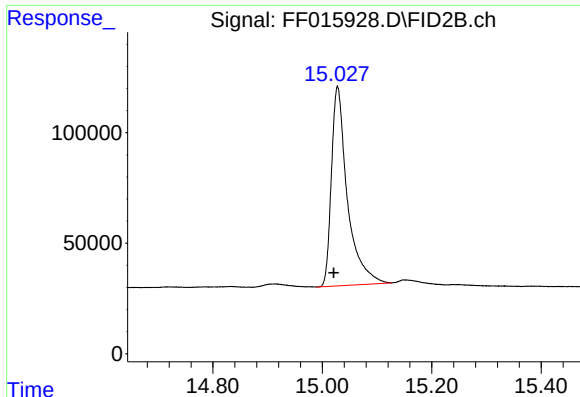

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.028 min
Delta R.T.: 0.007 min
Response: 1824239
Conc: 14.94 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

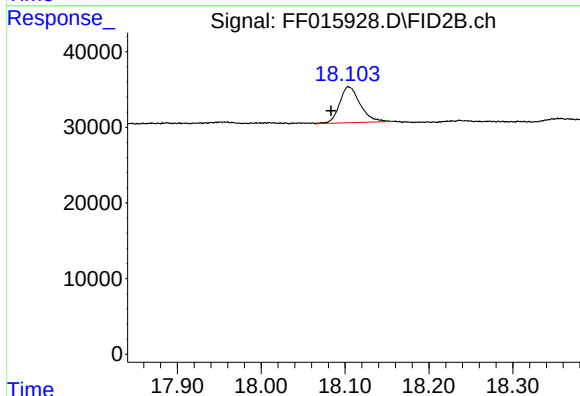


#13 N-TRIACONTANE

R.T.: 18.104 min
Delta R.T.: 0.021 min
Response: 80504
Conc: 0.58 ug/ml

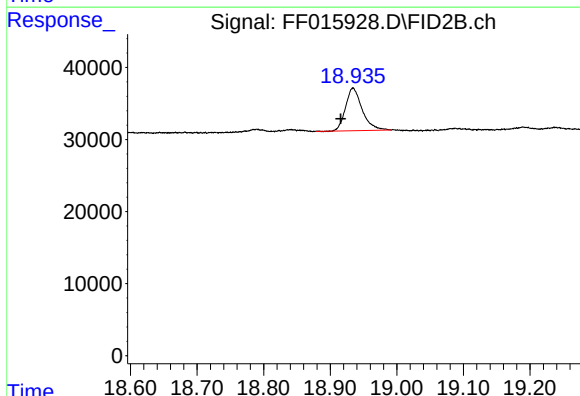

#14 N-DOTRIACONTANE

R.T.: 18.934 min
Delta R.T.: 0.019 min
Response: 102429
Conc: 0.76 ug/ml

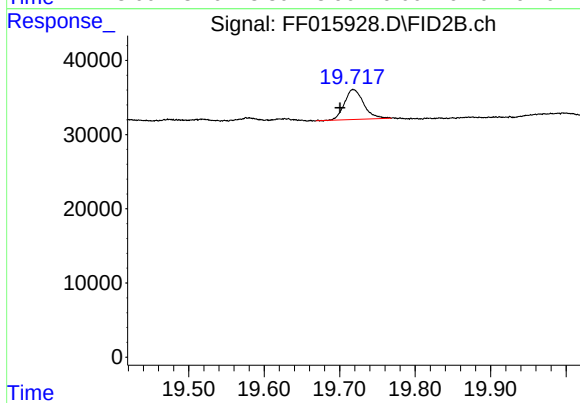

#15 N-TETRATRIACONTANE

R.T.: 19.718 min
Delta R.T.: 0.018 min
Response: 71339
Conc: 0.58 ug/ml