

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061025\
Data File : FF015924.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2025 18:32
Operator : YP\AJ
Sample : PB168382BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB168382BL

Integration File: autoint1.e
Quant Time: Jun 11 04:44:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052125.M
Quant Title :
QLast Update : Wed May 21 12:32:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.034	1658130	13.576 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061025\
Data File : FF015924.D
Signal(s) : FID2B.ch
Acq On : 10 Jun 2025 18:32
Operator : YP\AJ
Sample : PB168382BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB168382BL

Integration File: autoint1.e
Quant Time: Jun 11 04:44:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052125.M
Quant Title :
QLast Update : Wed May 21 12:32:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

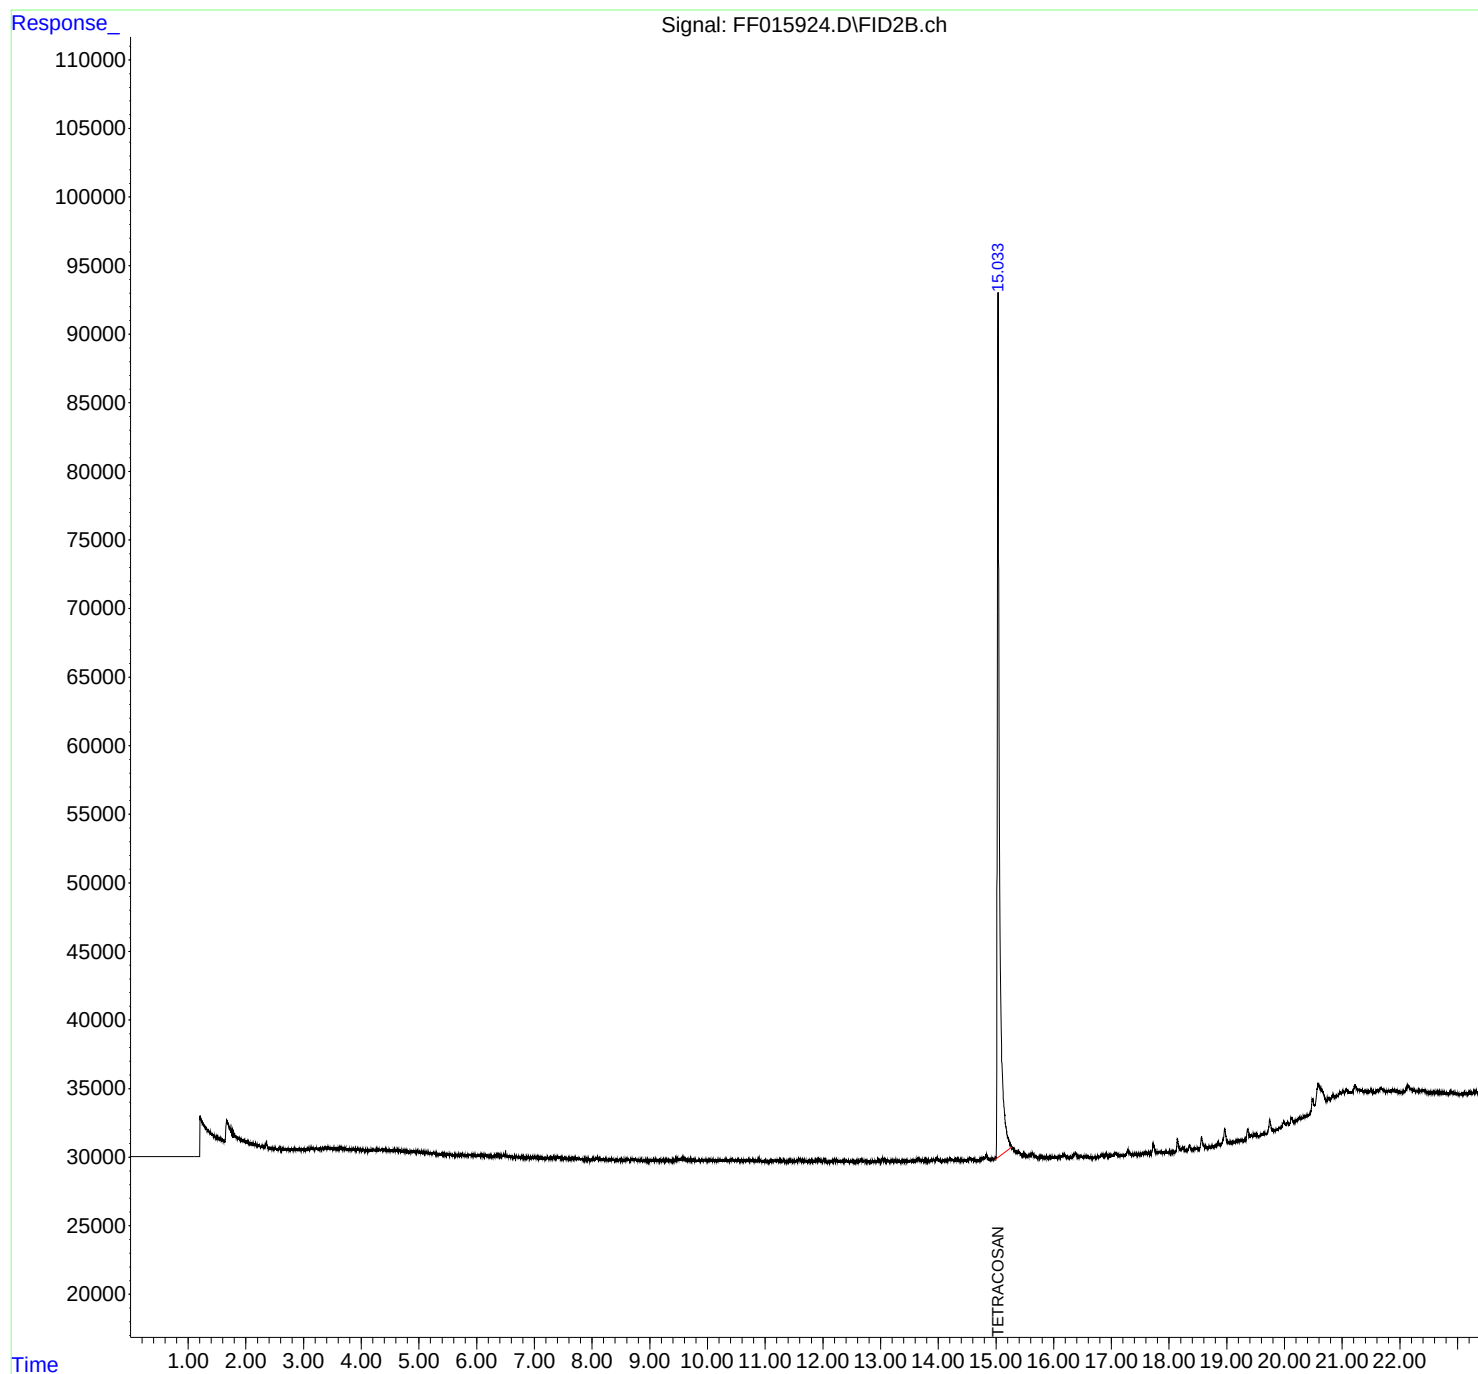

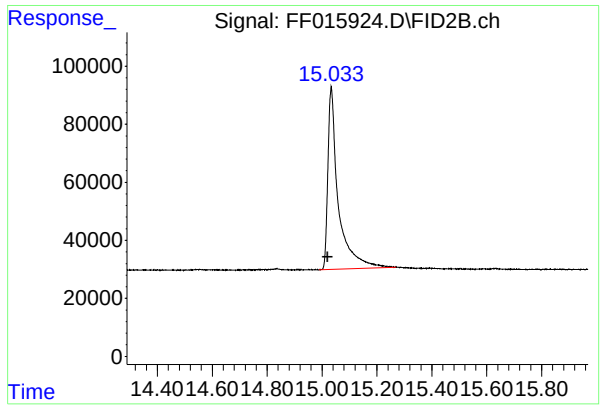

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.034 min
Delta R.T.: 0.013 min
Response: 1658130
Conc: 13.58 ug/ml

Instrument :
FID_F
ClientSampleId :
PB168382BL