

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061119\
 Data File : FF004776.D
 Signal(s) : FID2B.ch
 Acq On : 11 Jun 2019 11:06
 Operator : DD\AJ
 Sample : K3265-08 2X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 12 02:10:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.705	1070141	8.764 ug/ml
Target Compounds			
4) N-TETRADECANE	8.293	180624	1.230 ug/ml
8) N-DOCOSANE	13.802	160235	1.134 ug/ml
10) N-TETRACOSANE	14.910	277033	1.999 ug/ml
11) N-HEXACOSANE	15.936	571179	4.192 ug/ml
12) N-OCTACOSANE	16.890	886973	6.524 ug/ml
13) N-TRIACONTANE	17.783	767339	5.549 ug/ml
14) N-DOTRIACONTANE	18.623	764944	5.530 ug/ml
15) N-TETRATRIACONTANE	19.414	324502	2.373 ug/ml
16) N-HEXATRIACONTANE	20.159	426819	3.242 ug/ml
17) N-OCTATRIACONTANE	20.915	262172	2.180 ug/ml
18) N-TETRACONTANE	21.872	856267	6.954 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061119\
Data File : FF004776.D
Signal(s) : FID2B.ch
Acq On : 11 Jun 2019 11:06
Operator : DD\AJ
Sample : K3265-08 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 12 02:10:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

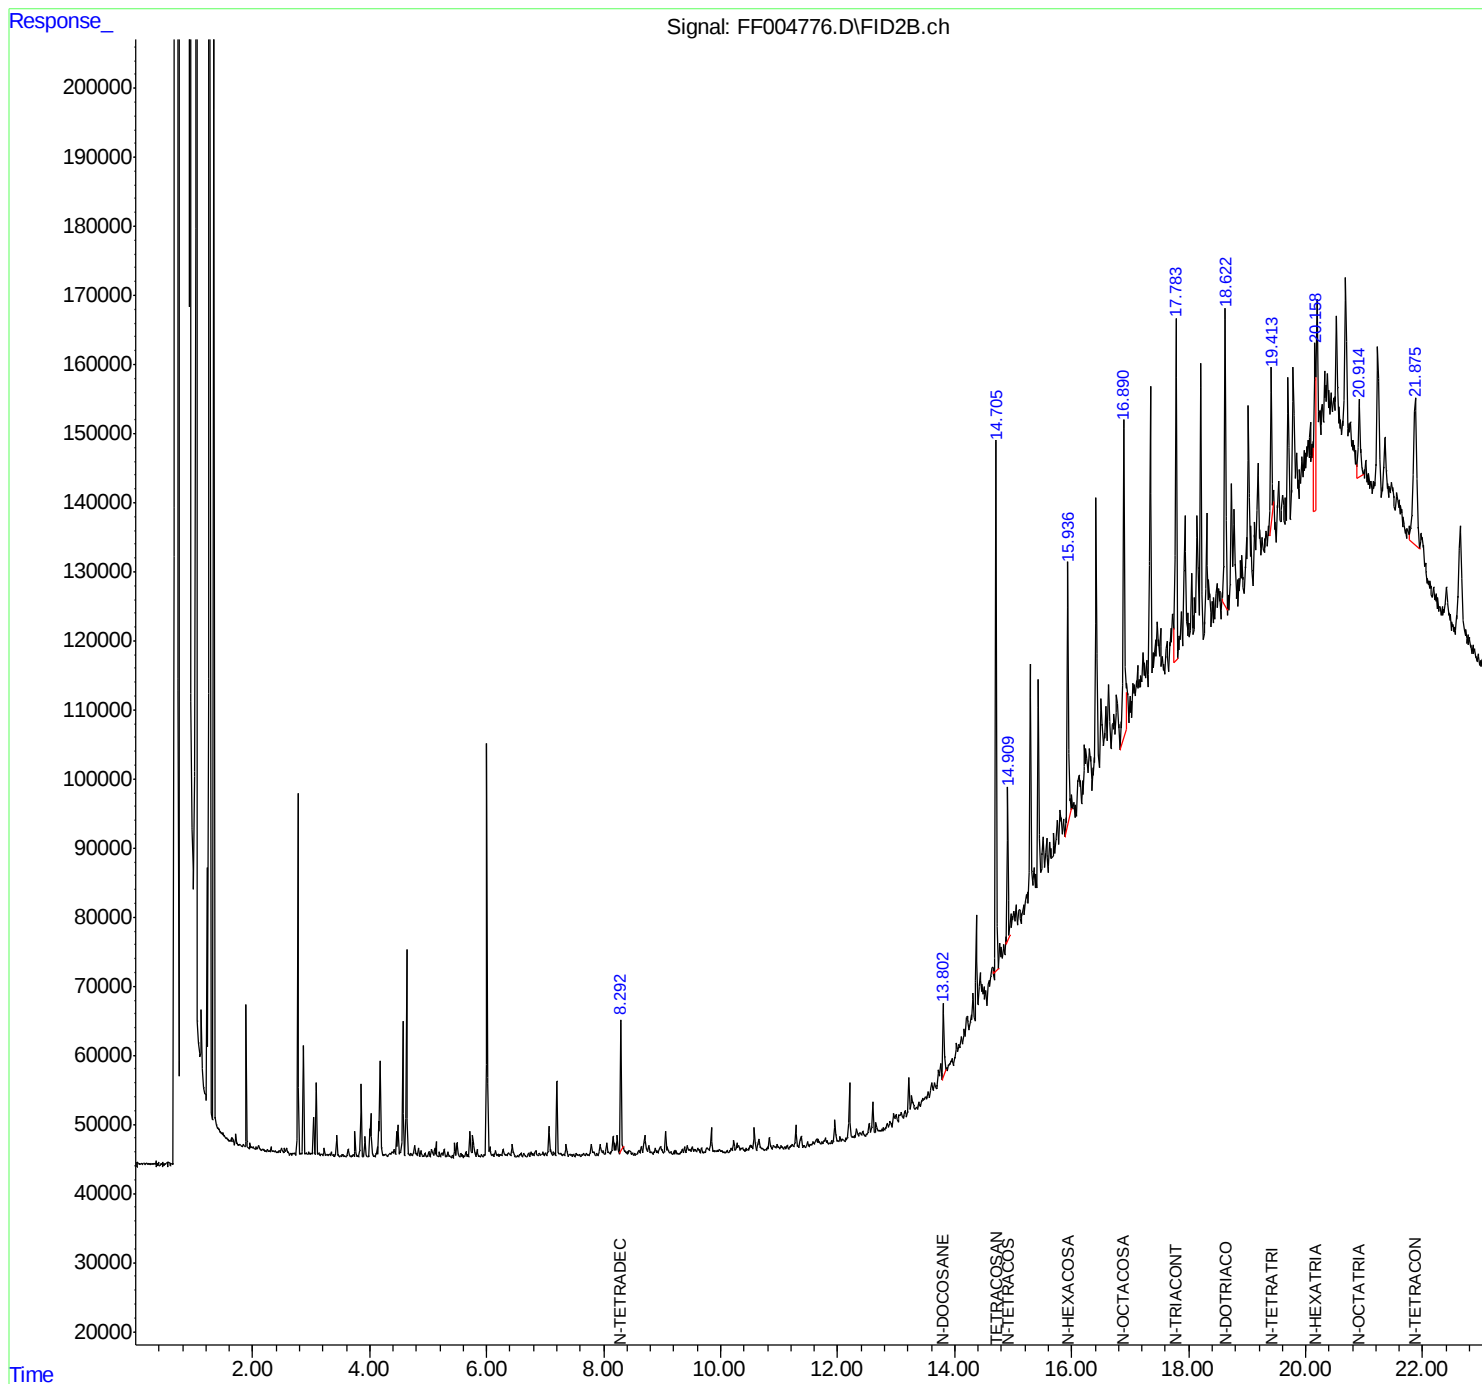

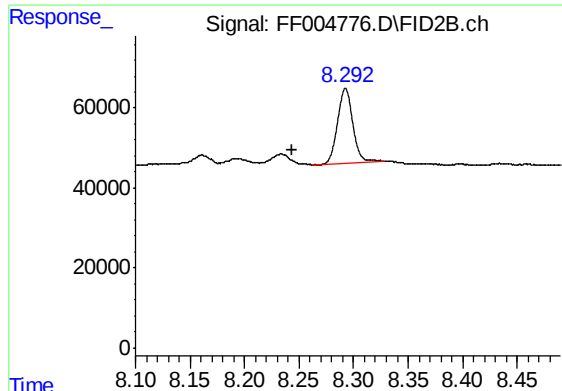


#4 N-TETRADECANE

R.T.: 8.293 min
Delta R.T.: 0.049 min
Response: 180624
Conc: 1.23 ug/ml

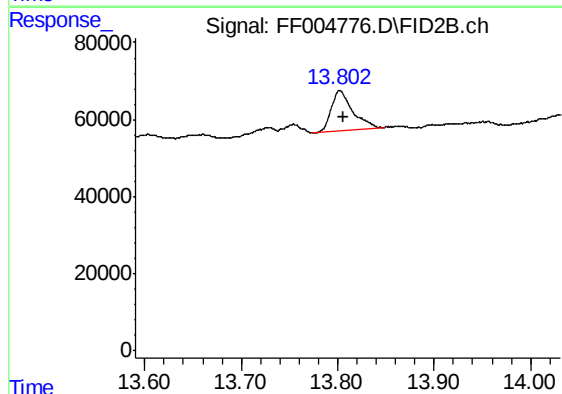


#8 N-DOCOSANE

R.T.: 13.802 min
Delta R.T.: -0.004 min
Response: 160235
Conc: 1.13 ug/ml

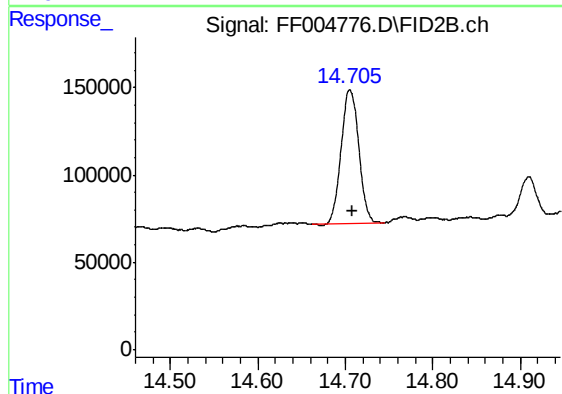


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.705 min
Delta R.T.: -0.003 min
Response: 1070141
Conc: 8.76 ug/ml

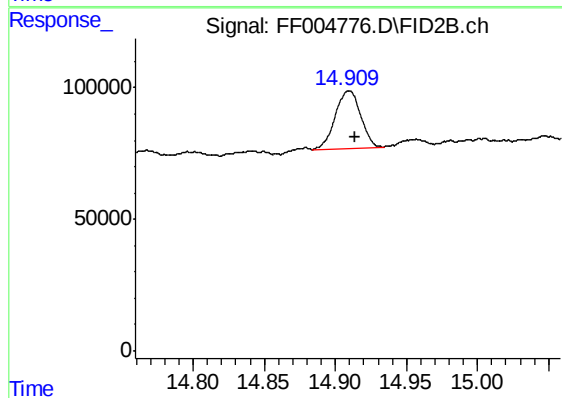


#10 N-TETRACOSANE

R.T.: 14.910 min
Delta R.T.: -0.004 min
Response: 277033
Conc: 2.00 ug/ml

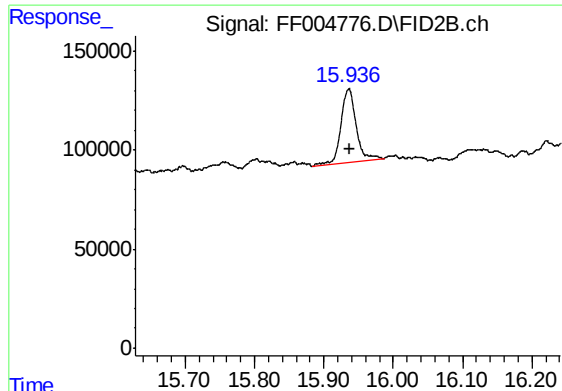


#11 N-HEXACOSANE

R.T.: 15.936 min
Delta R.T.: -0.001 min
Response: 571179
Conc: 4.19 ug/ml

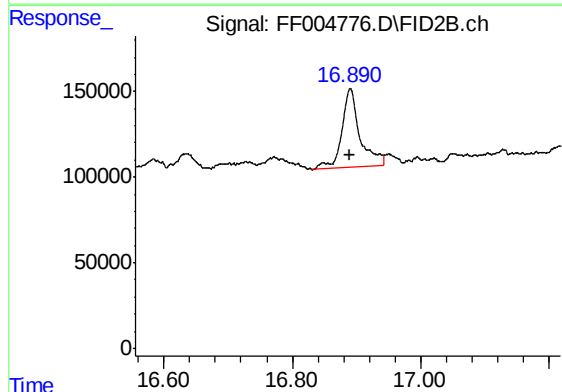


#12 N-OCTACOSANE

R.T.: 16.890 min
Delta R.T.: 0.000 min
Response: 886973
Conc: 6.52 ug/ml

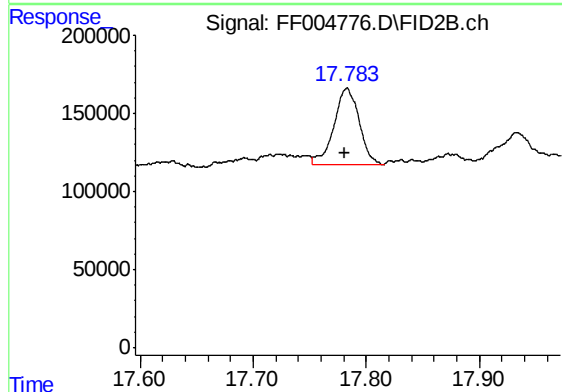


#13 N-TRIACONTANE

R.T.: 17.783 min
Delta R.T.: 0.002 min
Response: 767339
Conc: 5.55 ug/ml

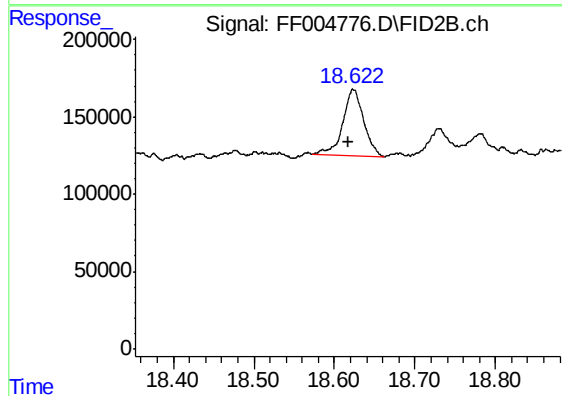


#14 N-DOTRIACONTANE

R.T.: 18.623 min
Delta R.T.: 0.006 min
Response: 764944
Conc: 5.53 ug/ml

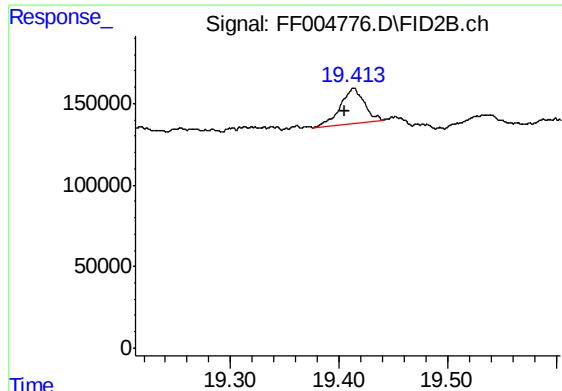


#15 N-TETRATRIACONTANE

R.T.: 19.414 min
Delta R.T.: 0.008 min
Response: 324502
Conc: 2.37 ug/ml

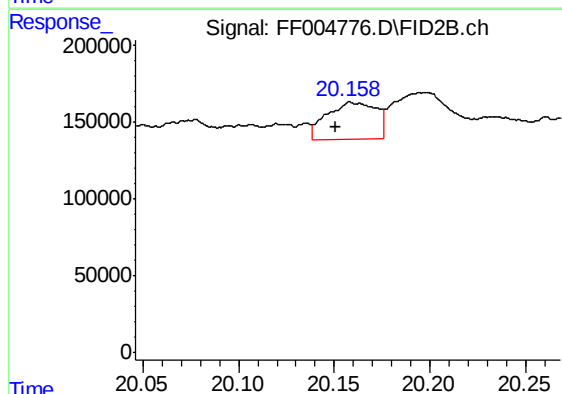


#16 N-HEXATRIACONTANE

R.T.: 20.159 min
Delta R.T.: 0.008 min
Response: 426819
Conc: 3.24 ug/ml

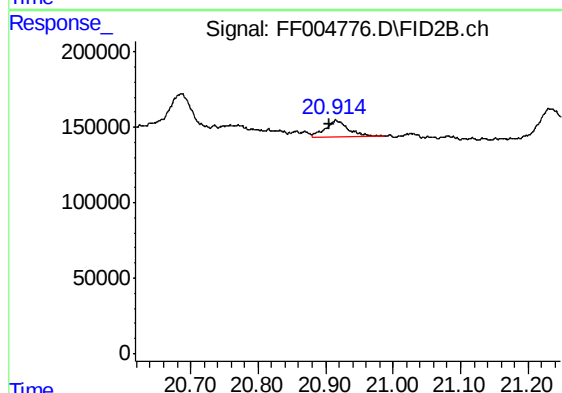

#17 N-OCTATRIACONTANE

R.T.: 20.915 min
Delta R.T.: 0.010 min
Response: 262172
Conc: 2.18 ug/ml

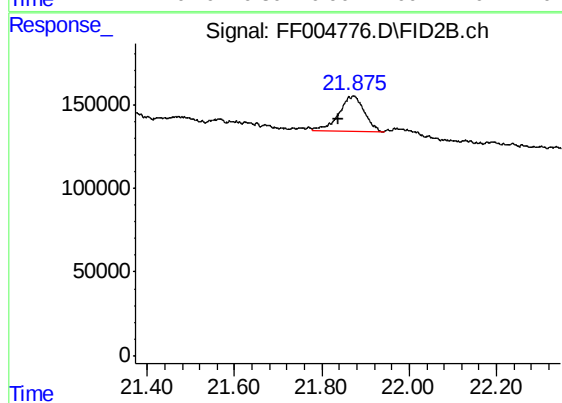

#18 N-TETRACONTANE

R.T.: 21.872 min
Delta R.T.: 0.035 min
Response: 856267
Conc: 6.95 ug/ml