

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061119\
 Data File : FF004780.D
 Signal(s) : FID2B.ch
 Acq On : 11 Jun 2019 13:21
 Operator : DD\AJ
 Sample : PB120507BS
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 12 02:10:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.704	1989521	16.293 ug/ml
Target Compounds			
2) N-DECANE	4.414	2606386	17.799 ug/ml
3) N-DODECANE	6.437	2560183	17.301 ug/ml
4) N-TETRADECANE	8.234	2480032	16.884 ug/ml
5) N-HEXADECANE	9.837	2406859	16.302 ug/ml
6) N-OCTADECANE	11.283	2337397	16.100 ug/ml
7) N-EICOSANE	12.598	2292528	15.829 ug/ml
8) N-DOCOSANE	13.801	2267178	16.045 ug/ml
10) N-TETRACOSANE	14.909	2304192	16.626 ug/ml
11) N-HEXACOSANE	15.935	2310535	16.958 ug/ml
12) N-OCTACOSANE	16.889	2349848	17.283 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061119\
Data File : FF004780.D
Signal(s) : FID2B.ch
Acq On : 11 Jun 2019 13:21
Operator : DD\AJ
Sample : PB120507BS
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 12 02:10:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

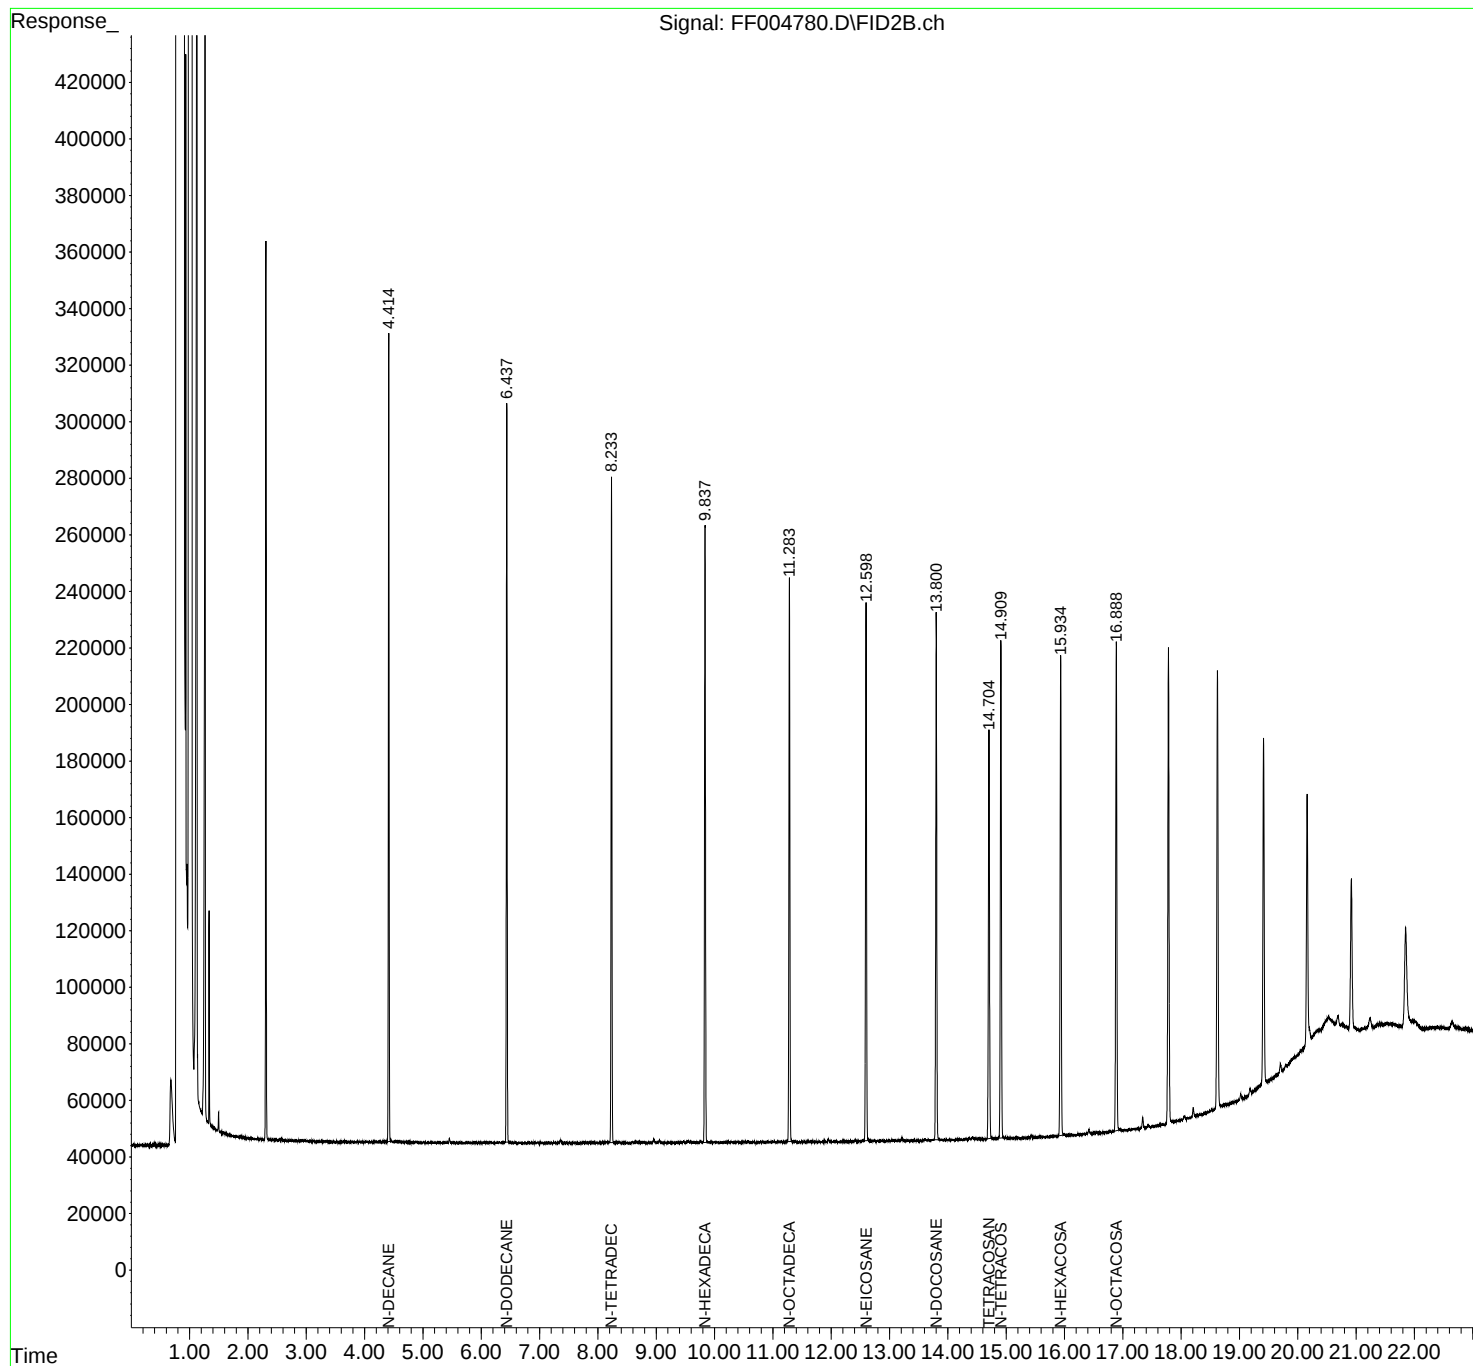

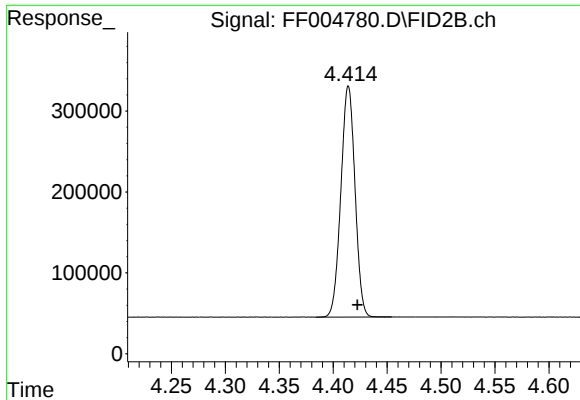


#2 N-DECANE

R.T.: 4.414 min
Delta R.T.: -0.008 min
Response: 2606386
Conc: 17.80 ug/ml

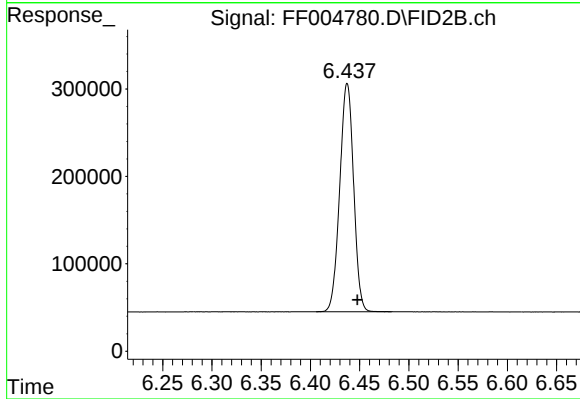


#3 N-DODECANE

R.T.: 6.437 min
Delta R.T.: -0.010 min
Response: 2560183
Conc: 17.30 ug/ml

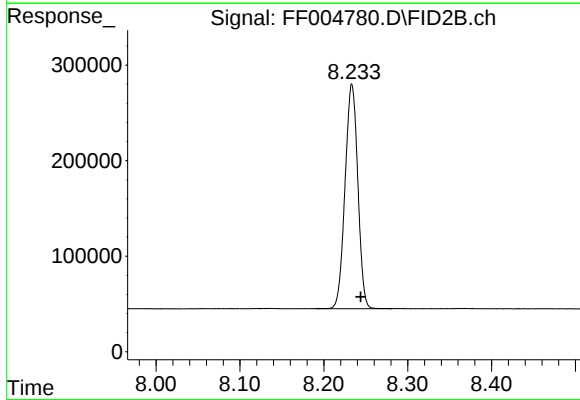


#4 N-TETRADECANE

R.T.: 8.234 min
Delta R.T.: -0.010 min
Response: 2480032
Conc: 16.88 ug/ml

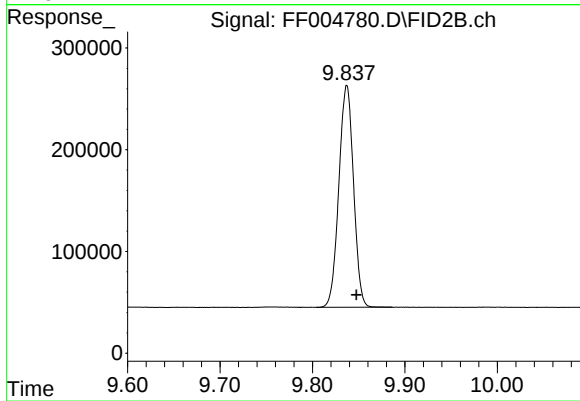


#5 N-HEXADECANE

R.T.: 9.837 min
Delta R.T.: -0.010 min
Response: 2406859
Conc: 16.30 ug/ml

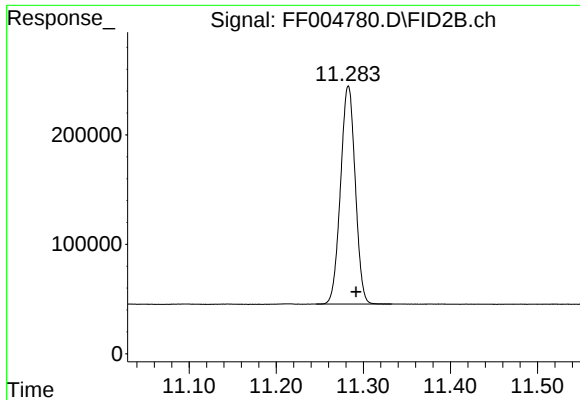


#6 N-OCTADECANE

R.T.: 11.283 min
Delta R.T.: -0.009 min
Response: 2337397
Conc: 16.10 ug/ml

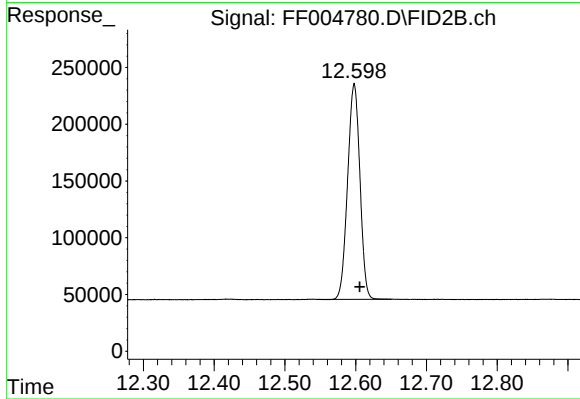


#7 N-EICOSANE

R.T.: 12.598 min
Delta R.T.: -0.008 min
Response: 2292528
Conc: 15.83 ug/ml

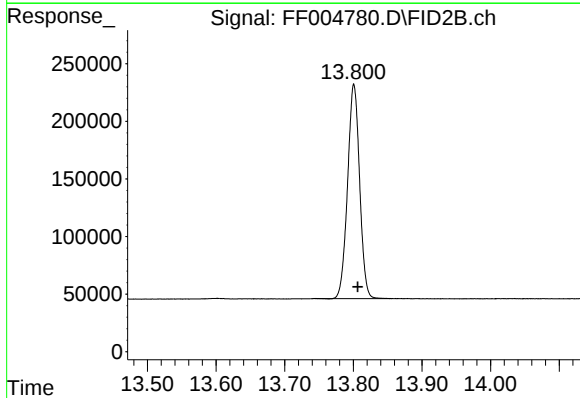


#8 N-DOCOSANE

R.T.: 13.801 min
Delta R.T.: -0.006 min
Response: 2267178
Conc: 16.04 ug/ml

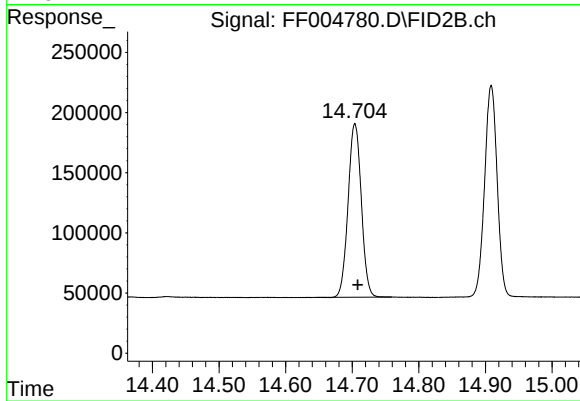


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.704 min
Delta R.T.: -0.004 min
Response: 1989521
Conc: 16.29 ug/ml

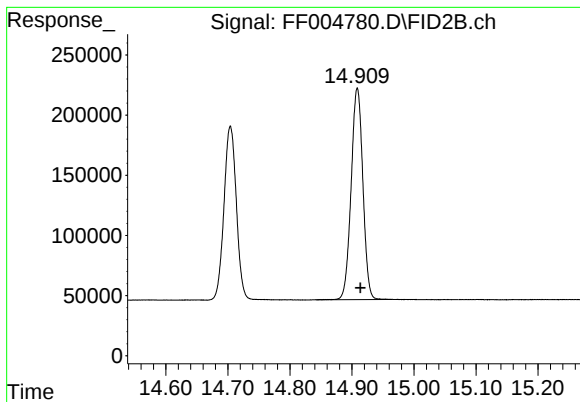


#10 N-TETRACOSANE

R.T.: 14.909 min
Delta R.T.: -0.005 min
Response: 2304192
Conc: 16.63 ug/ml

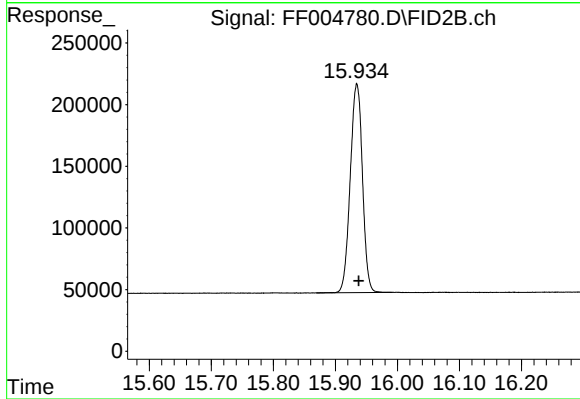

#11 N-HEXACOSANE

R.T.: 15.935 min
Delta R.T.: -0.003 min
Response: 2310535
Conc: 16.96 ug/ml

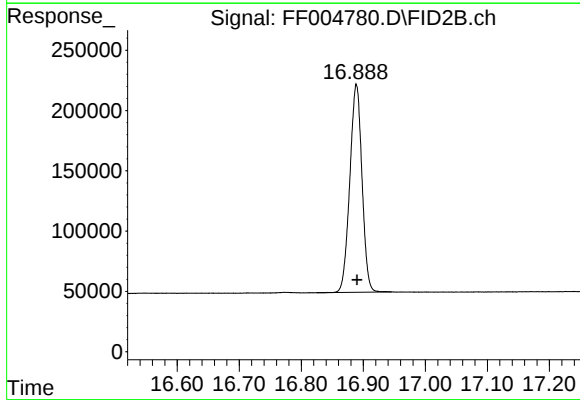

#12 N-OCTACOSANE

R.T.: 16.889 min
Delta R.T.: 0.000 min
Response: 2349848
Conc: 17.28 ug/ml