

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061119\
 Data File : FF004785.D
 Signal(s) : FID2B.ch
 Acq On : 11 Jun 2019 15:49
 Operator : DD\AJ
 Sample : K3283-02MSD
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 12 02:11:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.704	2174104	17.804 ug/ml
Target Compounds			
2) N-DECANE	4.414	2733494	18.667 ug/ml
3) N-DODECANE	6.438	2738355	18.505 ug/ml
4) N-TETRADECANE	8.234	2659354	18.105 ug/ml
5) N-HEXADECANE	9.837	2601887	17.623 ug/ml
6) N-OCTADECANE	11.284	2529152	17.420 ug/ml
7) N-EICOSANE	12.598	2474523	17.086 ug/ml
8) N-DOCOSANE	13.801	2469089	17.473 ug/ml
10) N-TETRACOSANE	14.909	2712399	19.572 ug/ml
11) N-HEXACOSANE	15.934	2564485	18.821 ug/ml
12) N-OCTACOSANE	16.889	2762013	20.315 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061119\
Data File : FF004785.D
Signal(s) : FID2B.ch
Acq On : 11 Jun 2019 15:49
Operator : DD\AJ
Sample : K3283-02MSD
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 12 02:11:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

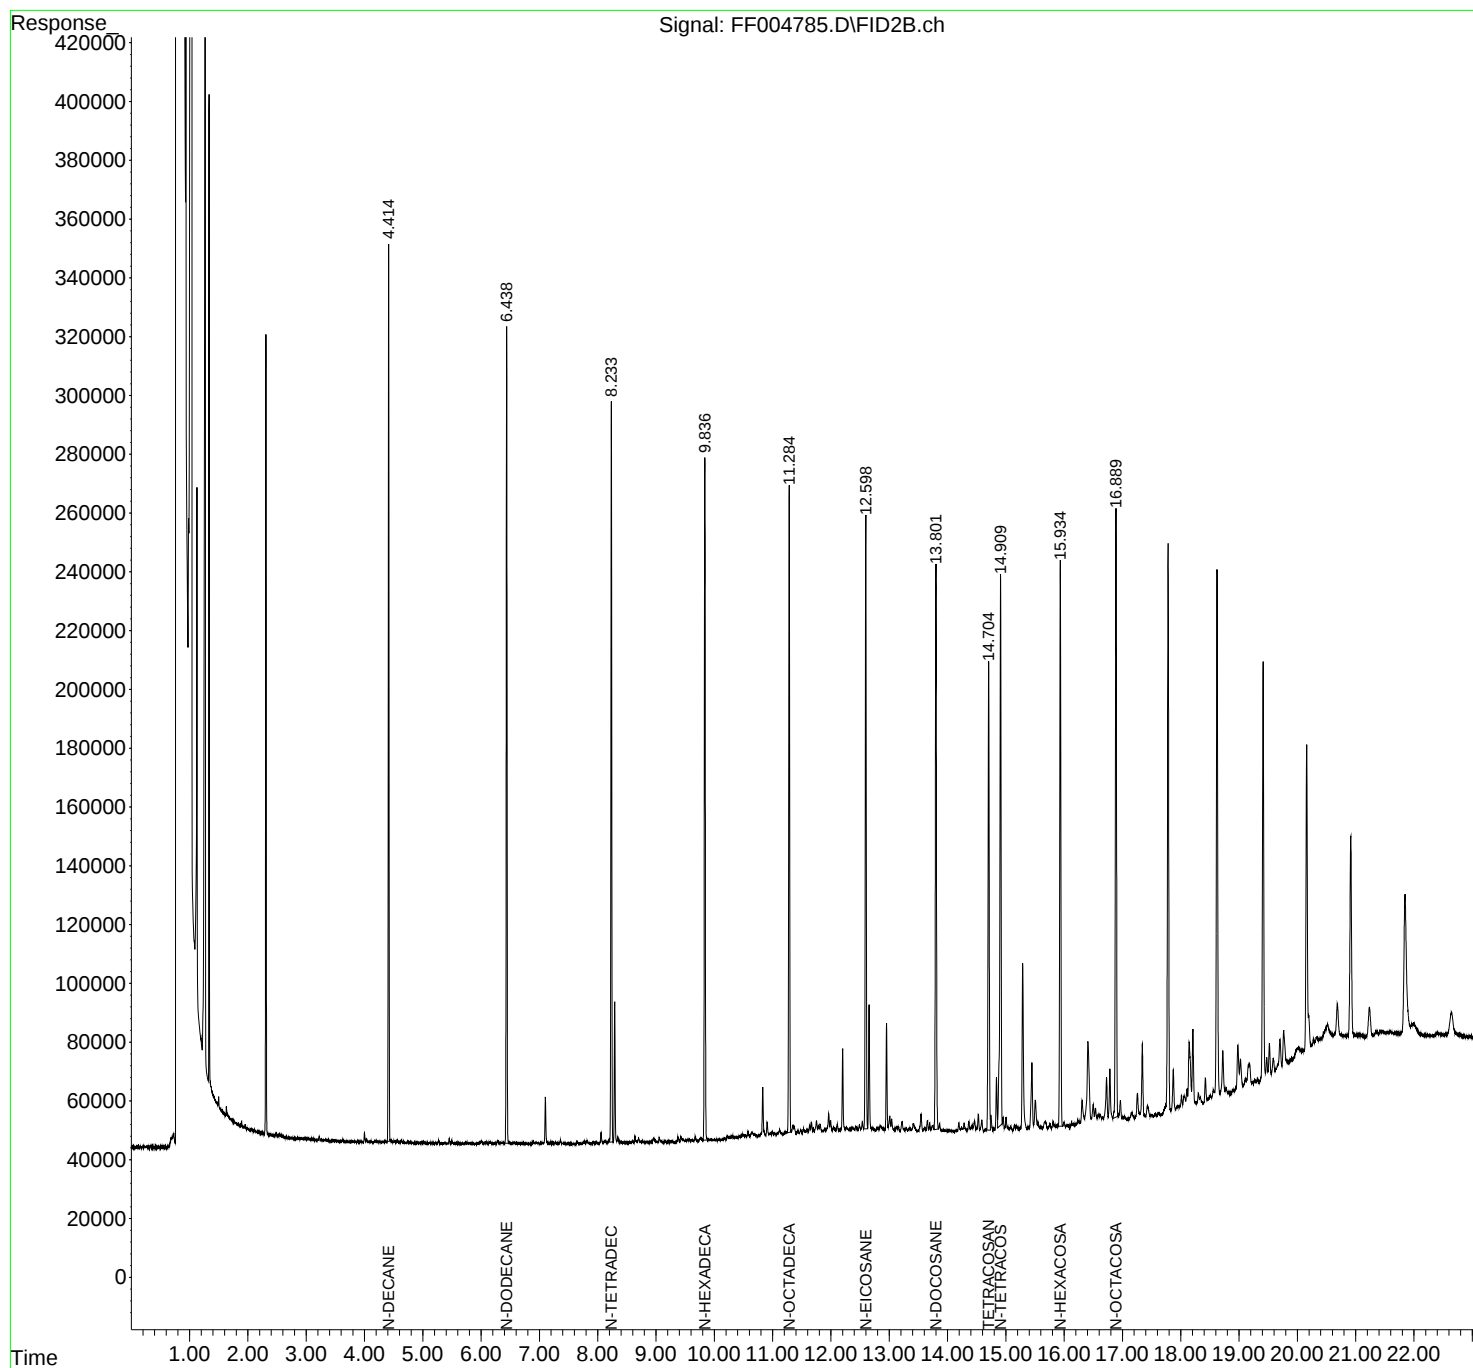

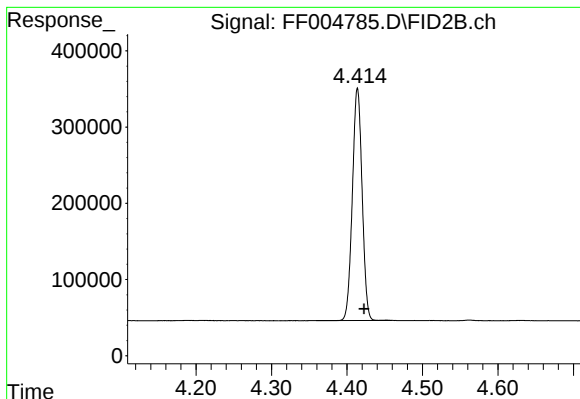


#2 N-DECANE

R.T.: 4.414 min
Delta R.T.: -0.009 min
Response: 2733494
Conc: 18.67 ug/ml

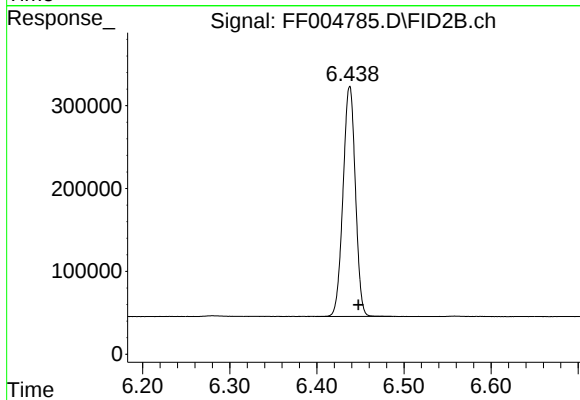


#3 N-DODECANE

R.T.: 6.438 min
Delta R.T.: -0.010 min
Response: 2738355
Conc: 18.50 ug/ml

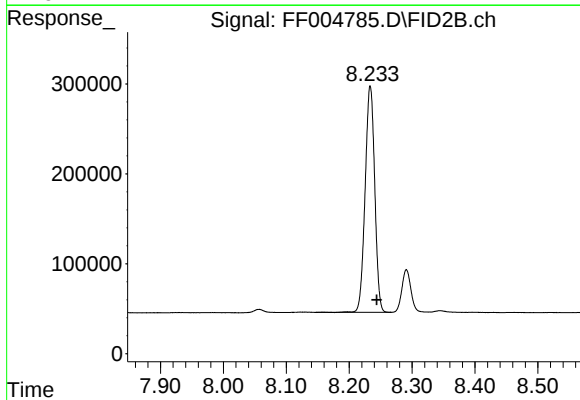


#4 N-TETRADECANE

R.T.: 8.234 min
Delta R.T.: -0.010 min
Response: 2659354
Conc: 18.10 ug/ml

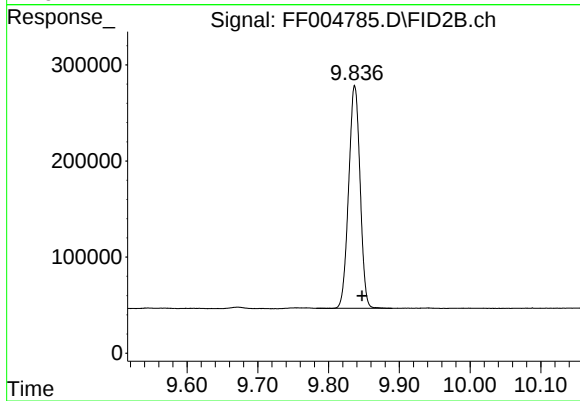


#5 N-HEXADECANE

R.T.: 9.837 min
Delta R.T.: -0.010 min
Response: 2601887
Conc: 17.62 ug/ml

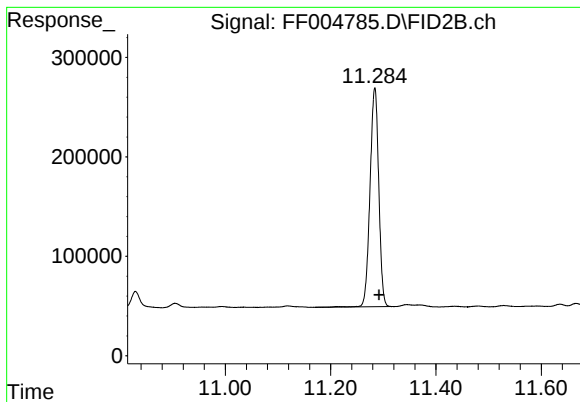


#6 N-OCTADECANE

R.T.: 11.284 min
Delta R.T.: -0.008 min
Response: 2529152
Conc: 17.42 ug/ml

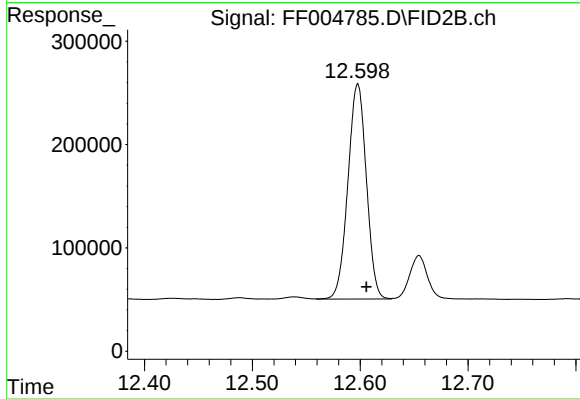


#7 N-EICOSANE

R.T.: 12.598 min
Delta R.T.: -0.008 min
Response: 2474523
Conc: 17.09 ug/ml

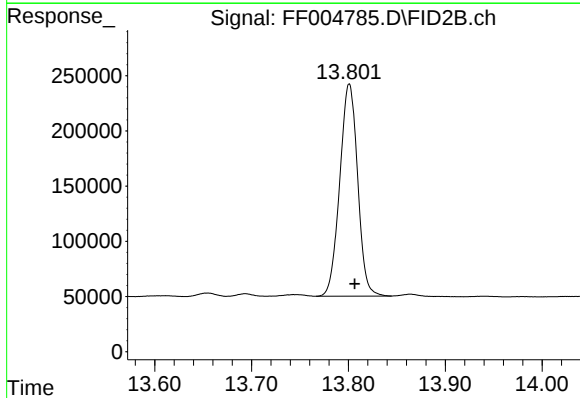


#8 N-DOCOSANE

R.T.: 13.801 min
Delta R.T.: -0.006 min
Response: 2469089
Conc: 17.47 ug/ml

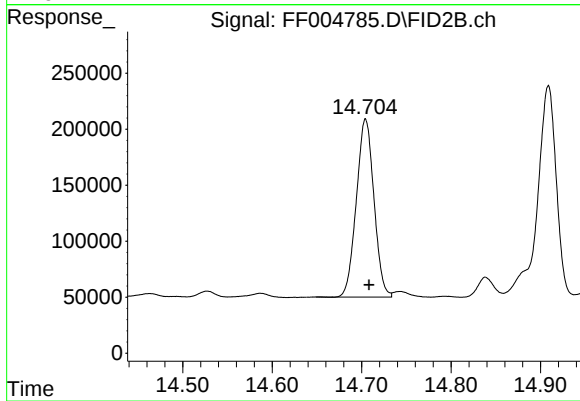


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.704 min
Delta R.T.: -0.004 min
Response: 2174104
Conc: 17.80 ug/ml

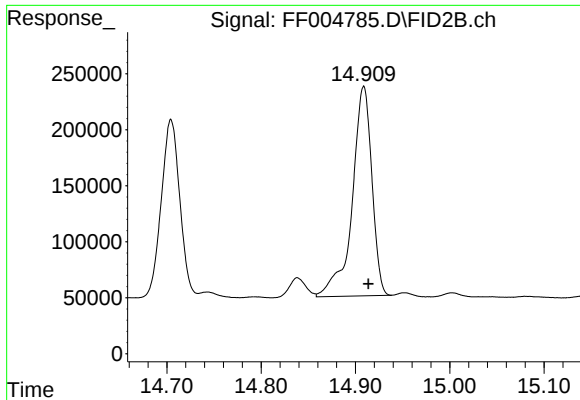


#10 N-TETRACOSANE

R.T.: 14.909 min
Delta R.T.: -0.005 min
Response: 2712399
Conc: 19.57 ug/ml

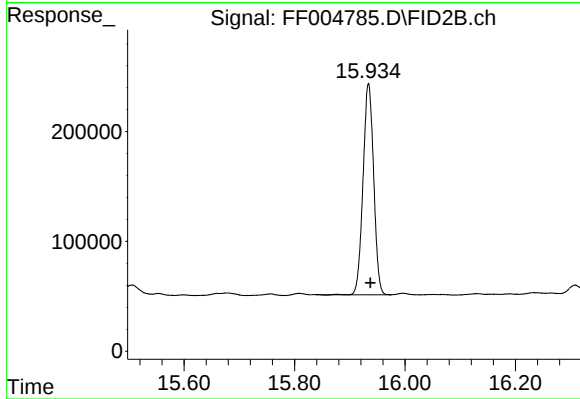

#11 N-HEXACOSANE

R.T.: 15.934 min
Delta R.T.: -0.004 min
Response: 2564485
Conc: 18.82 ug/ml

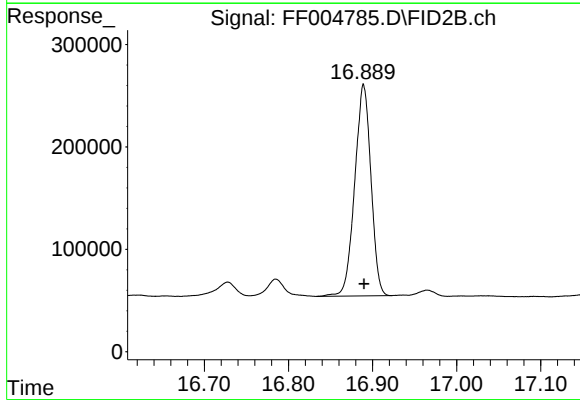

#12 N-OCTACOSANE

R.T.: 16.889 min
Delta R.T.: 0.000 min
Response: 2762013
Conc: 20.31 ug/ml