

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061219\
Data File : FF004789.D
Signal(s) : FID2B.ch
Acq On : 12 Jun 2019 10:54
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 13 01:30:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.701	2102020	17.214 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.777	100325	0.726 ug/ml
14) N-DOTRIACONTANE	18.615	159226	1.151 ug/ml
15) N-TETRATRIACONTANE	19.403	107565	0.787 ug/ml
16) N-HEXATRIACONTANE	20.153	81042	0.616 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061219\
Data File : FF004789.D
Signal(s) : FID2B.ch
Acq On : 12 Jun 2019 10:54
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 13 01:30:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

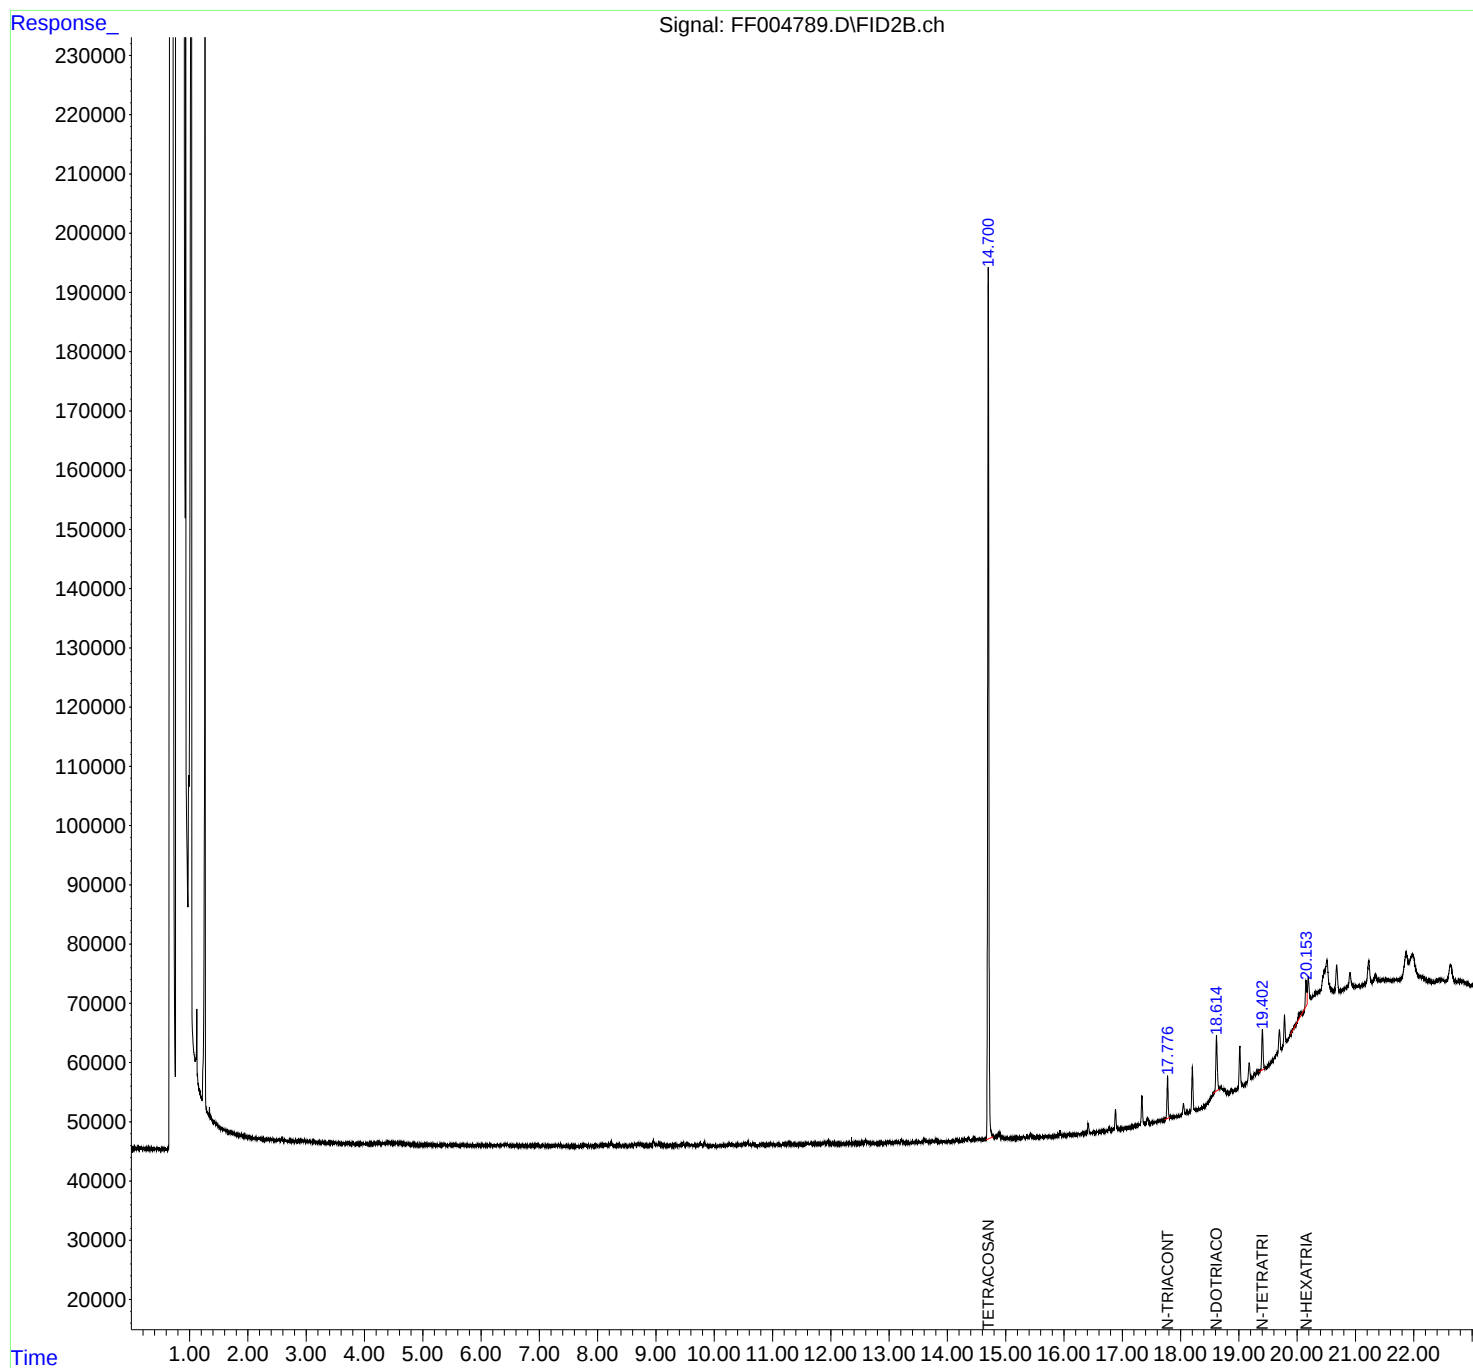

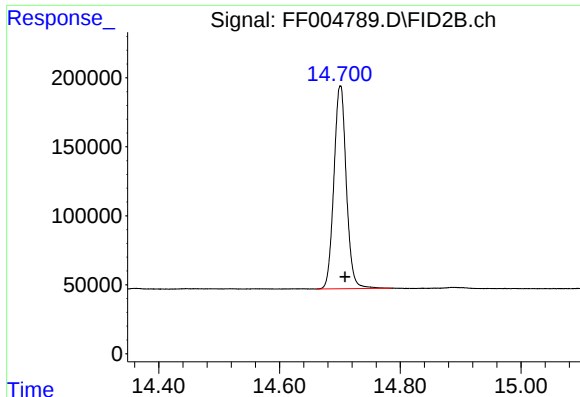


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.701 min
Delta R.T.: -0.008 min
Response: 2102020
Conc: 17.21 ug/ml

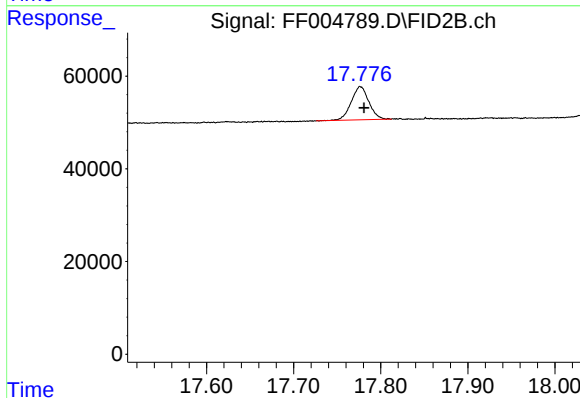


#13 N-TRIACONTANE

R.T.: 17.777 min
Delta R.T.: -0.004 min
Response: 100325
Conc: 0.73 ug/ml

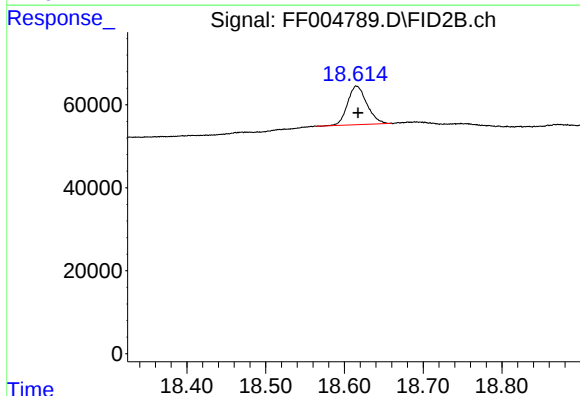


#14 N-DOTRIACONTANE

R.T.: 18.615 min
Delta R.T.: -0.002 min
Response: 159226
Conc: 1.15 ug/ml

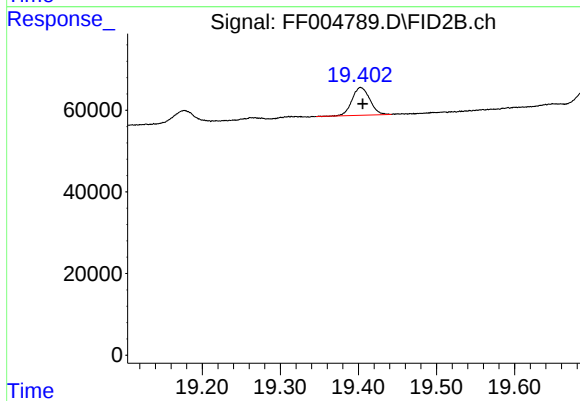

#15 N-TETRATRIACONTANE

R.T.: 19.403 min
Delta R.T.: -0.003 min
Response: 107565
Conc: 0.79 ug/ml

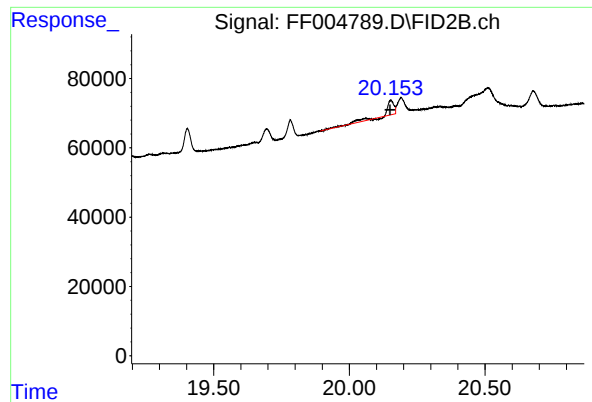

#16 N-HEXATRIACONTANE

R.T.: 20.153 min
Delta R.T.: 0.002 min
Response: 81042
Conc: 0.62 ug/ml