

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061219\
 Data File : FF004792.D
 Signal(s) : FID2B.ch
 Acq On : 12 Jun 2019 12:33
 Operator : DD\AJ
 Sample : PB120529BS
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 13 01:31:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.702	2963176	24.266 ug/ml
Target Compounds			
2) N-DECANE	4.409	3737514	25.524 ug/ml
3) N-DODECANE	6.431	3718554	25.128 ug/ml
4) N-TETRADECANE	8.228	3643801	24.806 ug/ml
5) N-HEXADECANE	9.833	3549339	24.040 ug/ml
6) N-OCTADECANE	11.280	3470829	23.907 ug/ml
7) N-EICOSANE	12.595	3408331	23.534 ug/ml
8) N-DOCOSANE	13.798	3346528	23.683 ug/ml
10) N-TETRACOSANE	14.907	3381973	24.403 ug/ml
11) N-HEXACOSANE	15.931	3338941	24.505 ug/ml
12) N-OCTACOSANE	16.887	3415350	25.120 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061219\
Data File : FF004792.D
Signal(s) : FID2B.ch
Acq On : 12 Jun 2019 12:33
Operator : DD\AJ
Sample : PB120529BS
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 13 01:31:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

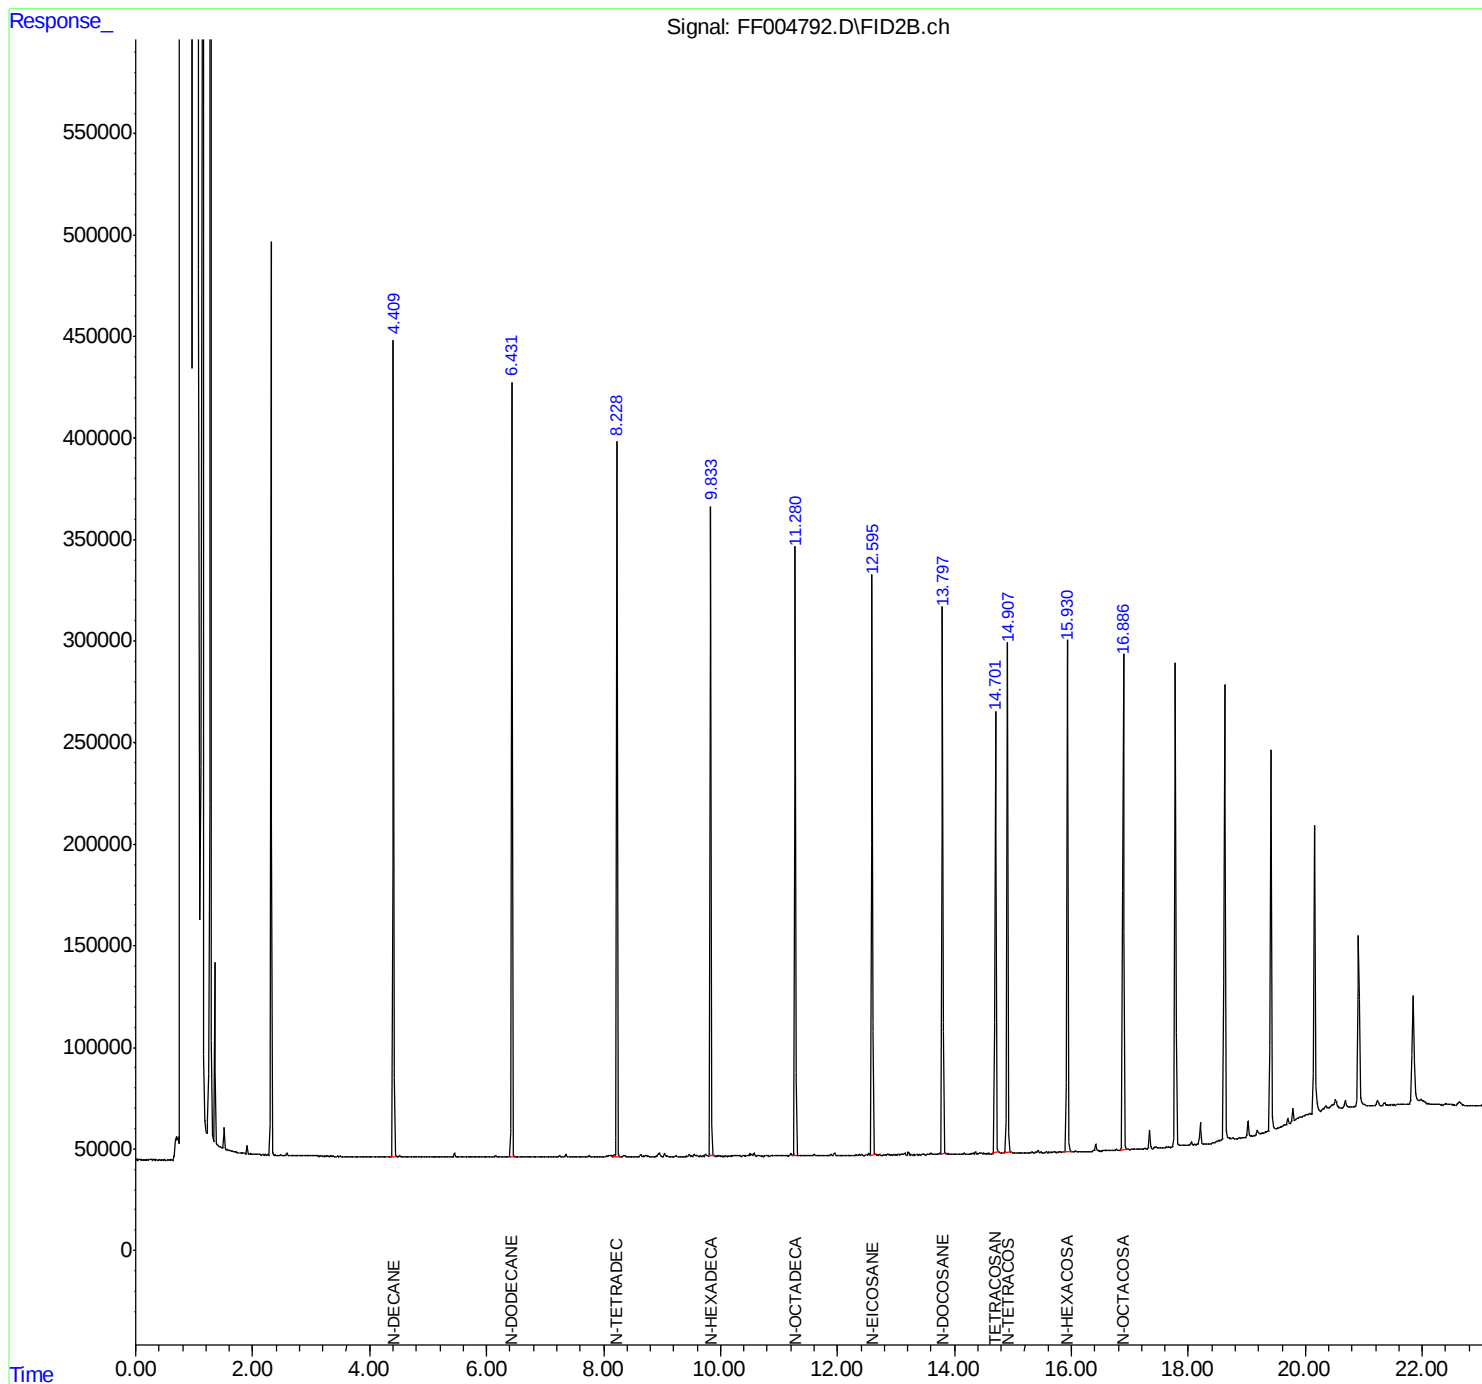

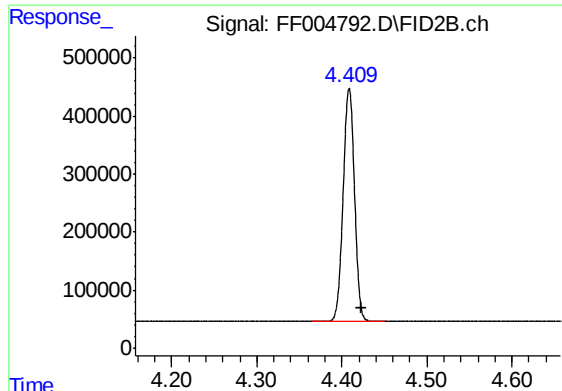


#2 N-DECANE

R.T.: 4.409 min
Delta R.T.: -0.014 min
Response: 3737514
Conc: 25.52 ug/ml

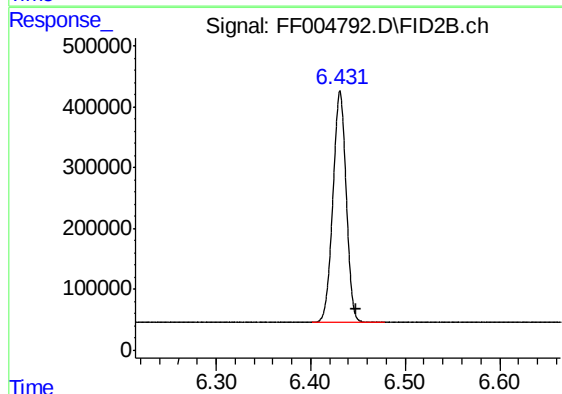


#3 N-DODECANE

R.T.: 6.431 min
Delta R.T.: -0.017 min
Response: 3718554
Conc: 25.13 ug/ml

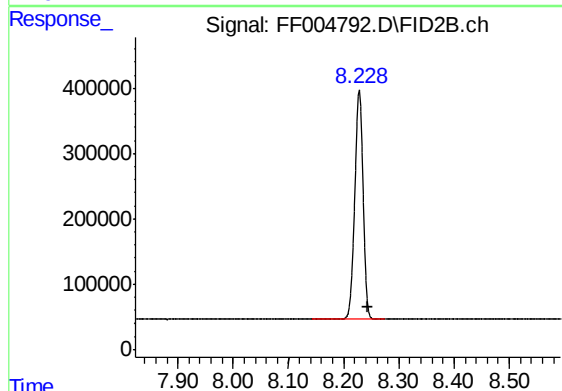


#4 N-TETRADECANE

R.T.: 8.228 min
Delta R.T.: -0.015 min
Response: 3643801
Conc: 24.81 ug/ml

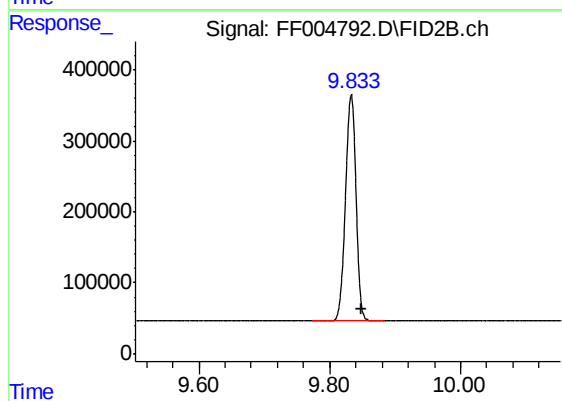


#5 N-HEXADECANE

R.T.: 9.833 min
Delta R.T.: -0.015 min
Response: 3549339
Conc: 24.04 ug/ml

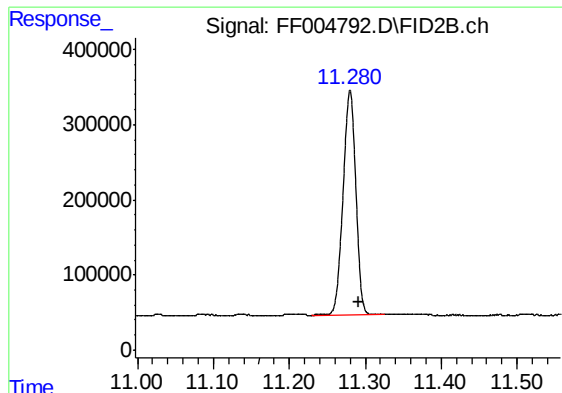


#6 N-OCTADECANE

R.T.: 11.280 min
Delta R.T.: -0.012 min
Response: 3470829
Conc: 23.91 ug/ml

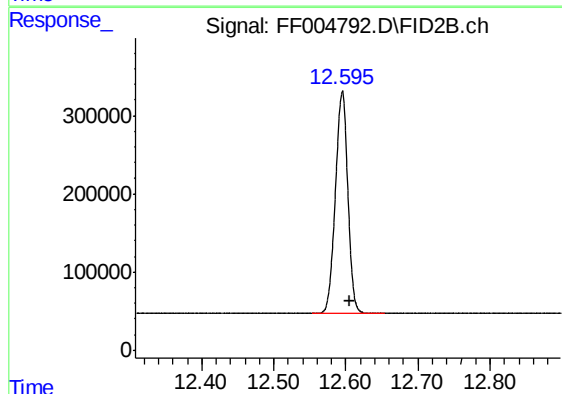


#7 N-EICOSANE

R.T.: 12.595 min
Delta R.T.: -0.011 min
Response: 3408331
Conc: 23.53 ug/ml

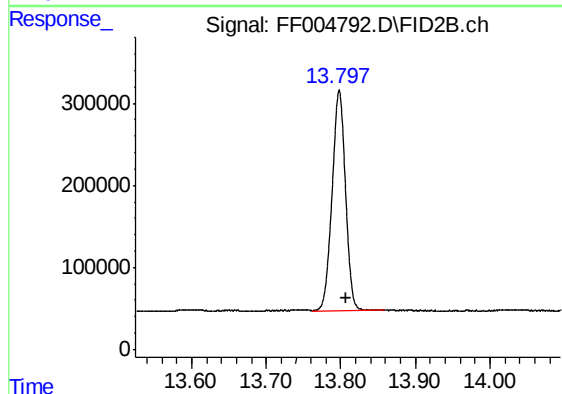


#8 N-DOCOSANE

R.T.: 13.798 min
Delta R.T.: -0.009 min
Response: 3346528
Conc: 23.68 ug/ml

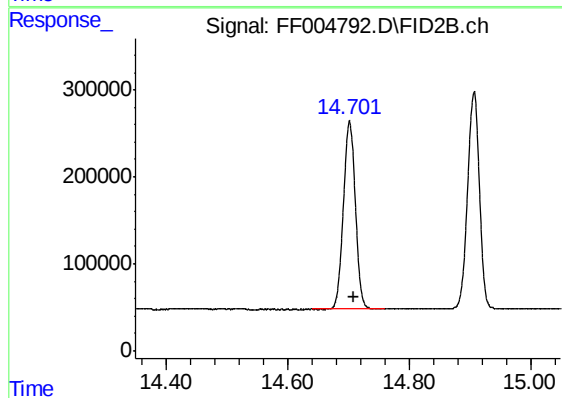


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.702 min
Delta R.T.: -0.007 min
Response: 2963176
Conc: 24.27 ug/ml

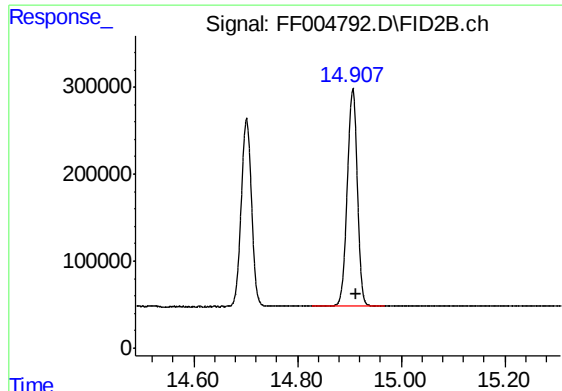


#10 N-TETRACOSANE

R.T.: 14.907 min
Delta R.T.: -0.007 min
Response: 3381973
Conc: 24.40 ug/ml

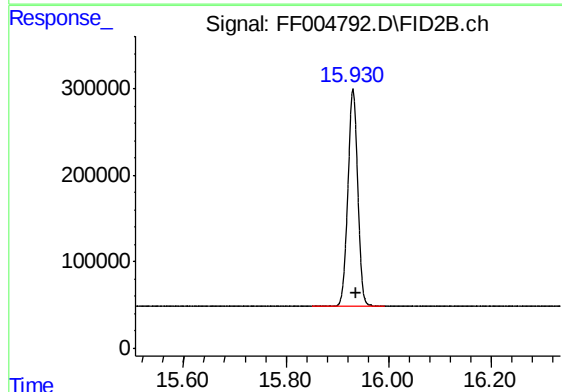

#11 N-HEXACOSANE

R.T.: 15.931 min
Delta R.T.: -0.007 min
Response: 3338941
Conc: 24.51 ug/ml

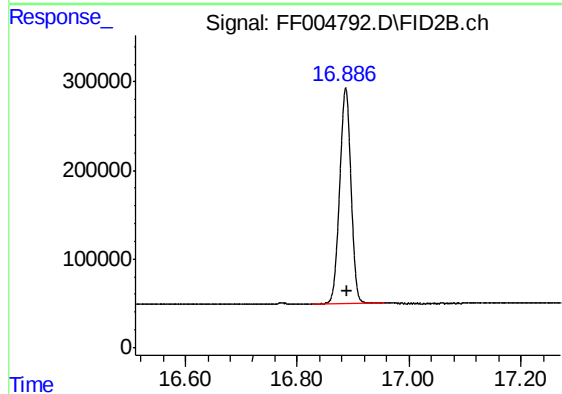

#12 N-OCTACOSANE

R.T.: 16.887 min
Delta R.T.: -0.003 min
Response: 3415350
Conc: 25.12 ug/ml