

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061223AL\
 Data File : FF012866.D
 Signal(s) : FID2B.ch
 Acq On : 12 Jun 2023 11:48
 Operator : YP\AJ
 Sample : PB151929BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 13 00:48:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 051923.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 12 16:29:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.316	3845329	32.536 ug/ml
Spiked Amount 50.000		Recovery =	65.07%
Target Compounds			
10) T n-Eicosane (C20)	11.868	179420	1.305 ug/ml
11) T n-Heneicosane (C21)	12.479	172524	1.276 ug/ml
13) T n-Docosane (C22)	13.064	187257	1.399 ug/ml
14) T n-Tetracosane (C24)	14.166	196965	1.498 ug/ml
15) T n-Hexacosane (C26)	15.186	201154	1.582 ug/ml
16) T n-Octacosane (C28)	16.133	206969	1.683 ug/ml
17) T n-Tricontane (C30)	17.020	221750	1.796 ug/ml
18) T n-Dotriacontane (C32)	17.850	234283	1.936 ug/ml
19) T n-Tetratriacontane (C34)	18.633	233448	1.995 ug/ml
20) T n-Hexatriacontane (C36)	19.372	224631	1.994 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061223AL\
Data File : FF012866.D
Signal(s) : FID2B.ch
Acq On : 12 Jun 2023 11:48
Operator : YP\AJ
Sample : PB151929BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 13 00:48:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 051923.M
Quant Title : GC Extractables
QLast Update : Mon Jun 12 16:29:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

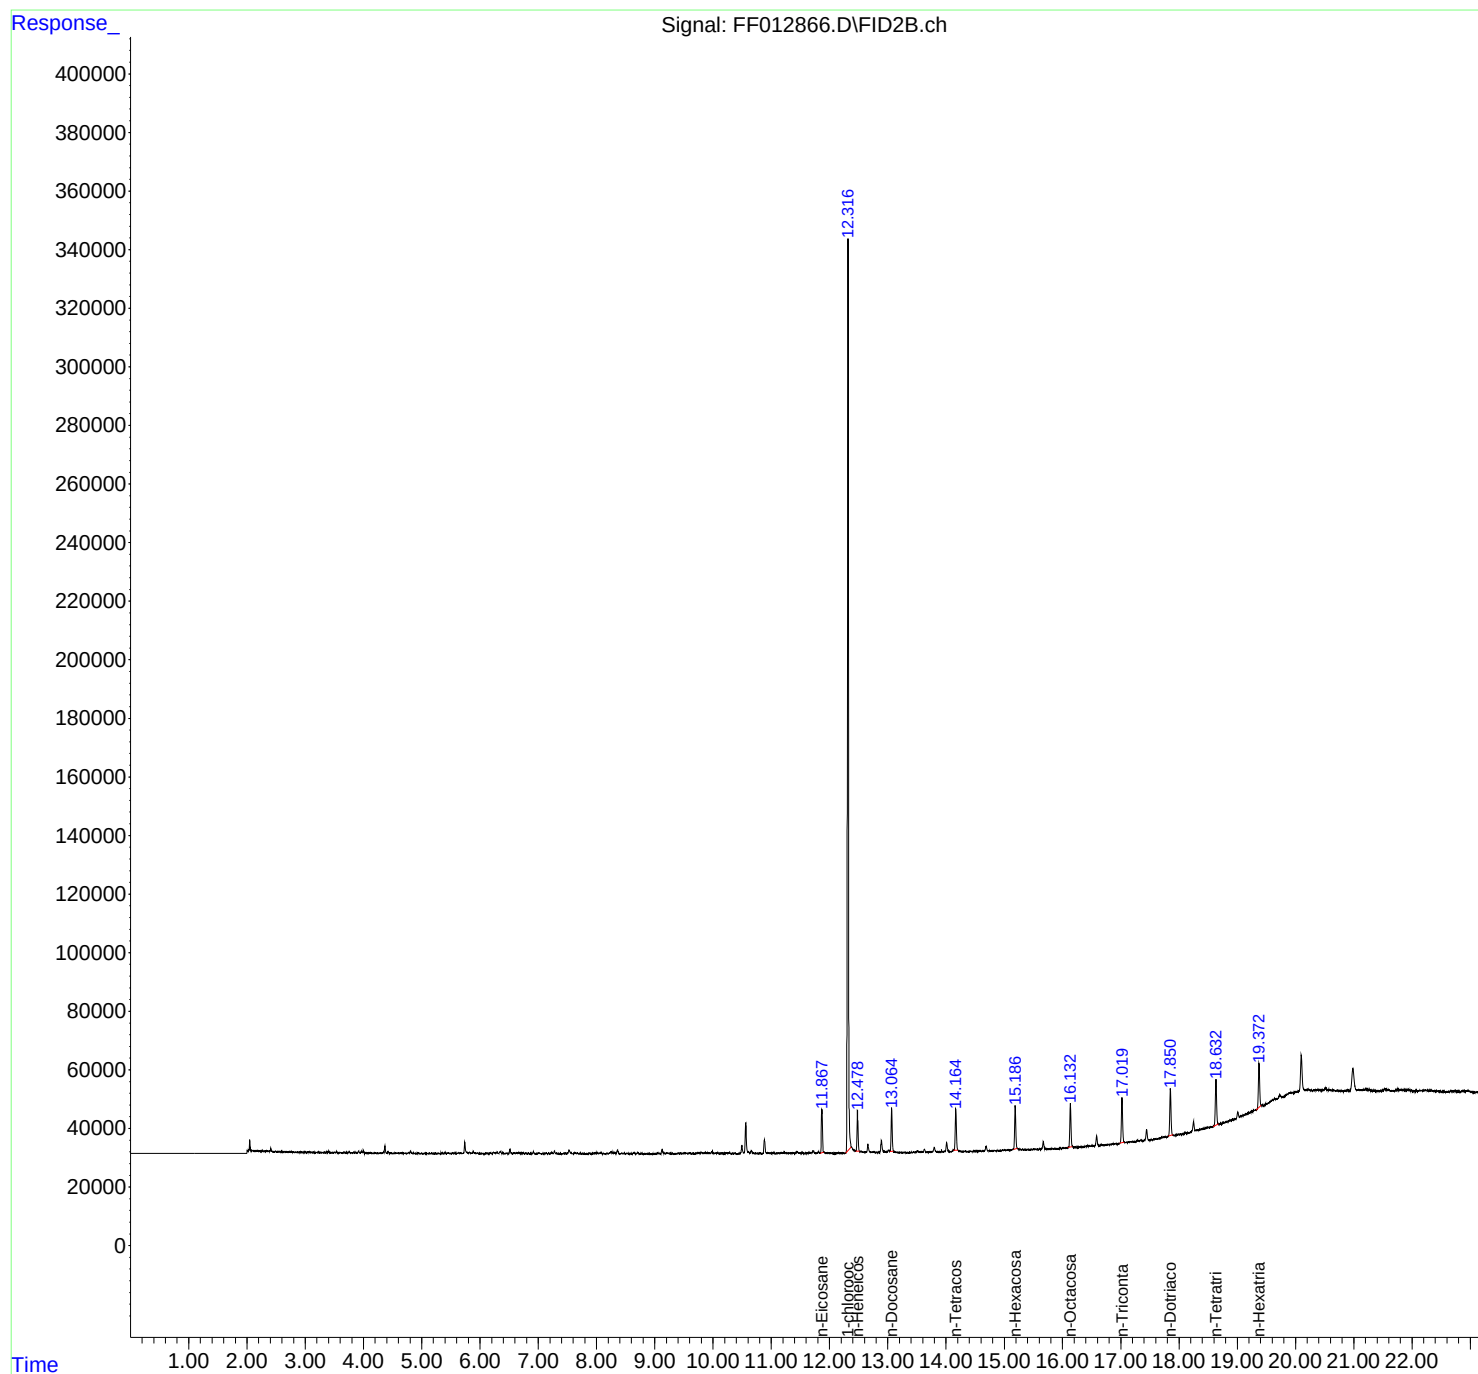


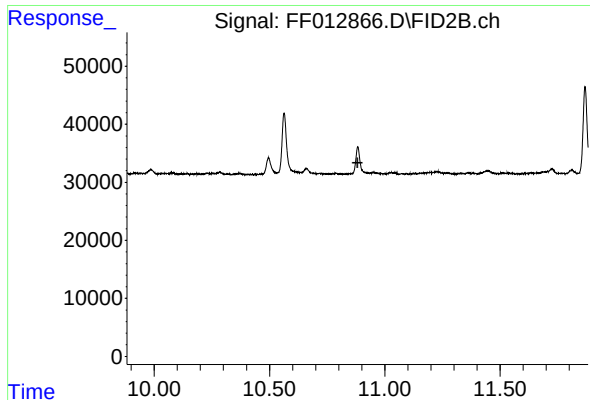

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.882 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

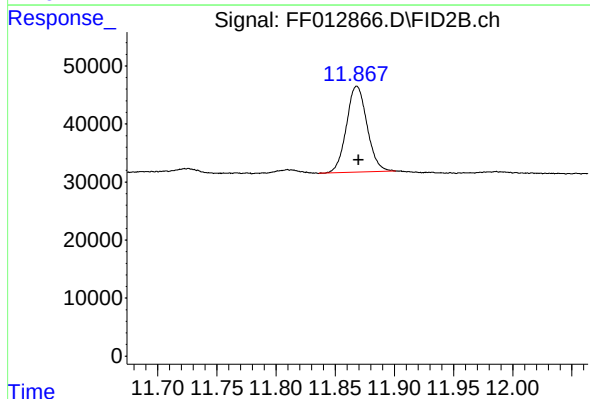


#10 n-Eicosane (C20)

R.T.: 11.868 min
Delta R.T.: -0.002 min
Response: 179420
Conc: 1.30 ug/ml

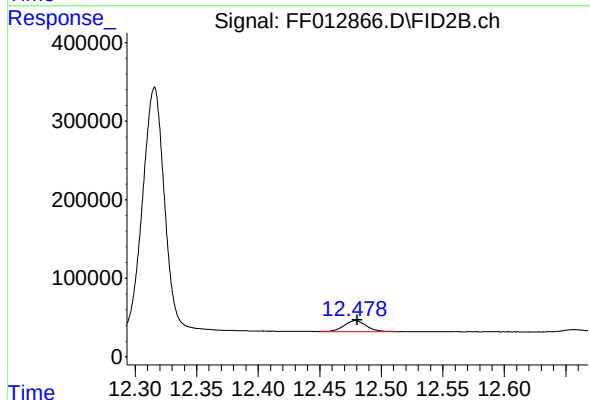


#11 n-Heneicosane (C21)

R.T.: 12.479 min
Delta R.T.: -0.001 min
Response: 172524
Conc: 1.28 ug/ml

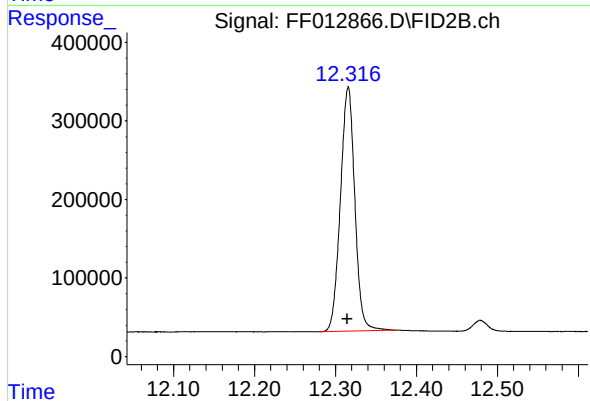

#12 1-chlorooctadecane (SURR)


R.T.: 12.316 min
Delta R.T.: 0.001 min
Response: 3845329
Conc: 32.54 ug/ml

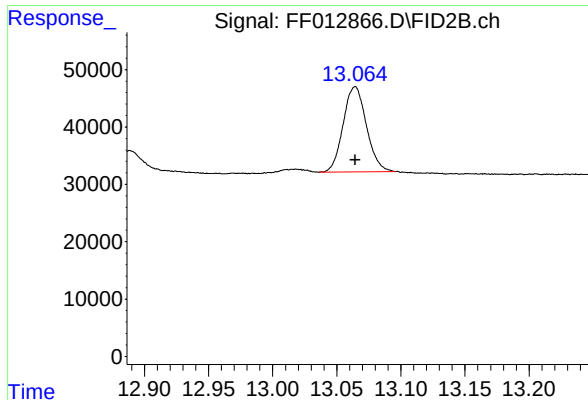

#13 n-Docosane (C22)


R.T.: 13.064 min
Delta R.T.: 0.000 min
Response: 187257
Conc: 1.40 ug/ml

Instrument :
FID_F
ClientSampleId :

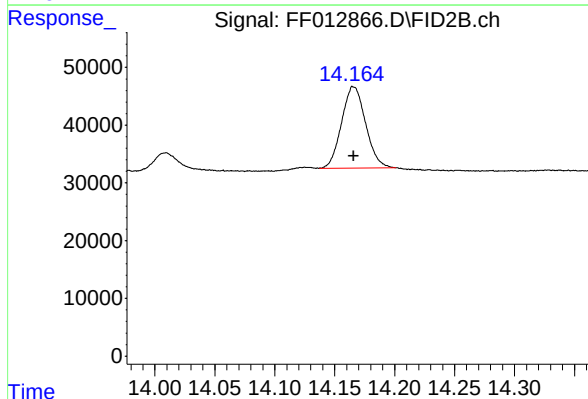


#14 n-Tetracosane (C24)

R.T.: 14.166 min
Delta R.T.: 0.000 min
Response: 196965
Conc: 1.50 ug/ml

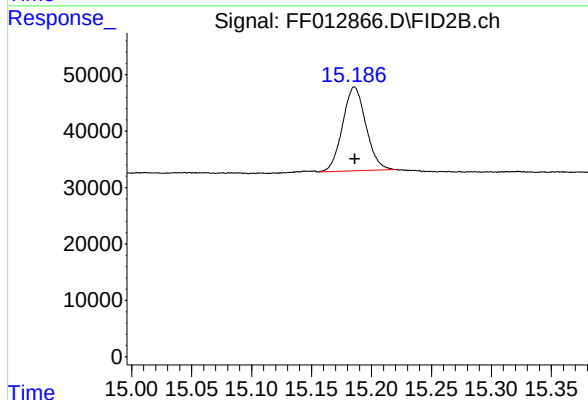


#15 n-Hexacosane (C26)

R.T.: 15.186 min
Delta R.T.: 0.000 min
Response: 201154
Conc: 1.58 ug/ml

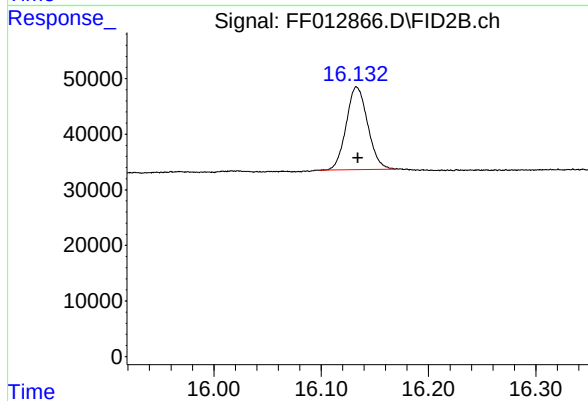

#16 n-Octacosane (C28)


R.T.: 16.133 min
Delta R.T.: -0.001 min
Response: 206969
Conc: 1.68 ug/ml

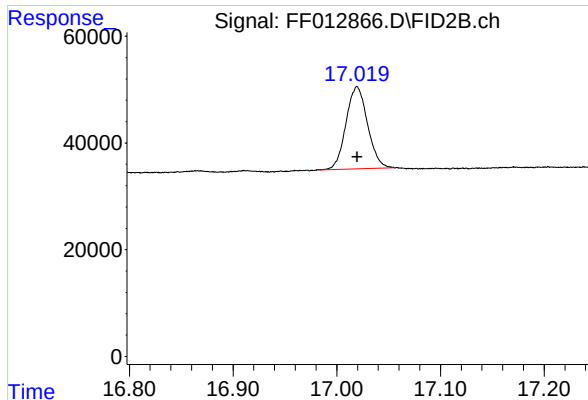

#17 n-Tricontane (C30)


R.T.: 17.020 min
Delta R.T.: 0.000 min
Response: 221750
Conc: 1.80 ug/ml

Instrument :
FID_F
ClientSampleId :

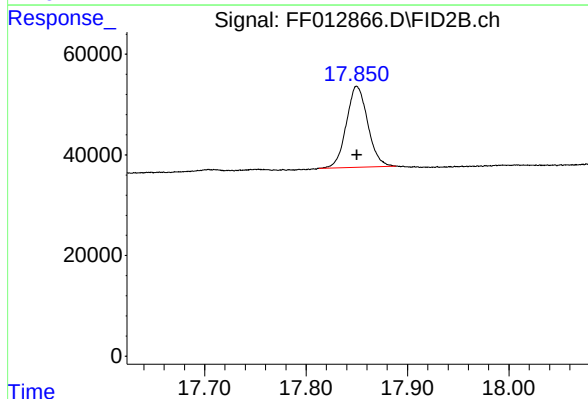


#18 n-Dotriacontane (C32)

R.T.: 17.850 min
Delta R.T.: 0.000 min
Response: 234283
Conc: 1.94 ug/ml

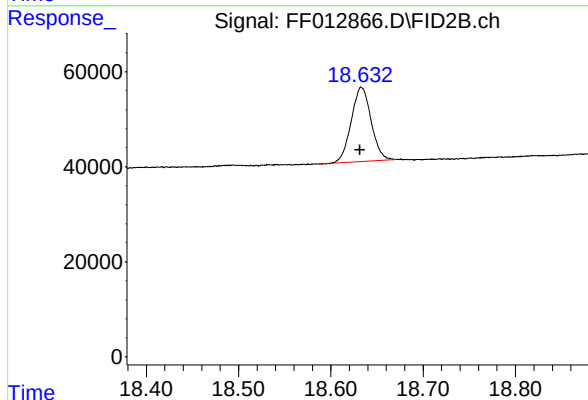

#19 n-Tetatriacontane (C34)

R.T.: 18.633 min
Delta R.T.: 0.001 min
Response: 233448
Conc: 2.00 ug/ml

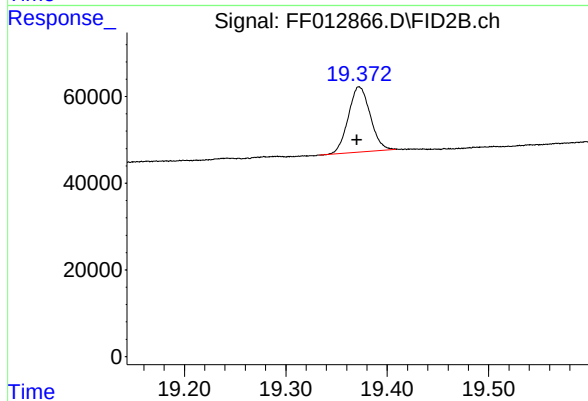

#20 n-Hexatriacontane (C36)

R.T.: 19.372 min
Delta R.T.: 0.002 min
Response: 224631
Conc: 1.99 ug/ml