

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061321\
 Data File : FF008599.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jun 2021 10:19
 Operator : DD\AJ
 Sample : M2673-02
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 14 07:19:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.768	2194091	20.823 ug/ml
Target Compounds			
8) N-DOCOSANE	13.862	78561	0.625 ug/ml
12) N-OCTACOSANE	16.995f	178030	1.501 ug/ml
14) N-DOTRIACONTANE	18.657	131577	1.093 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061321\
Data File : FF008599.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2021 10:19
Operator : DD\AJ
Sample : M2673-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 07:19:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

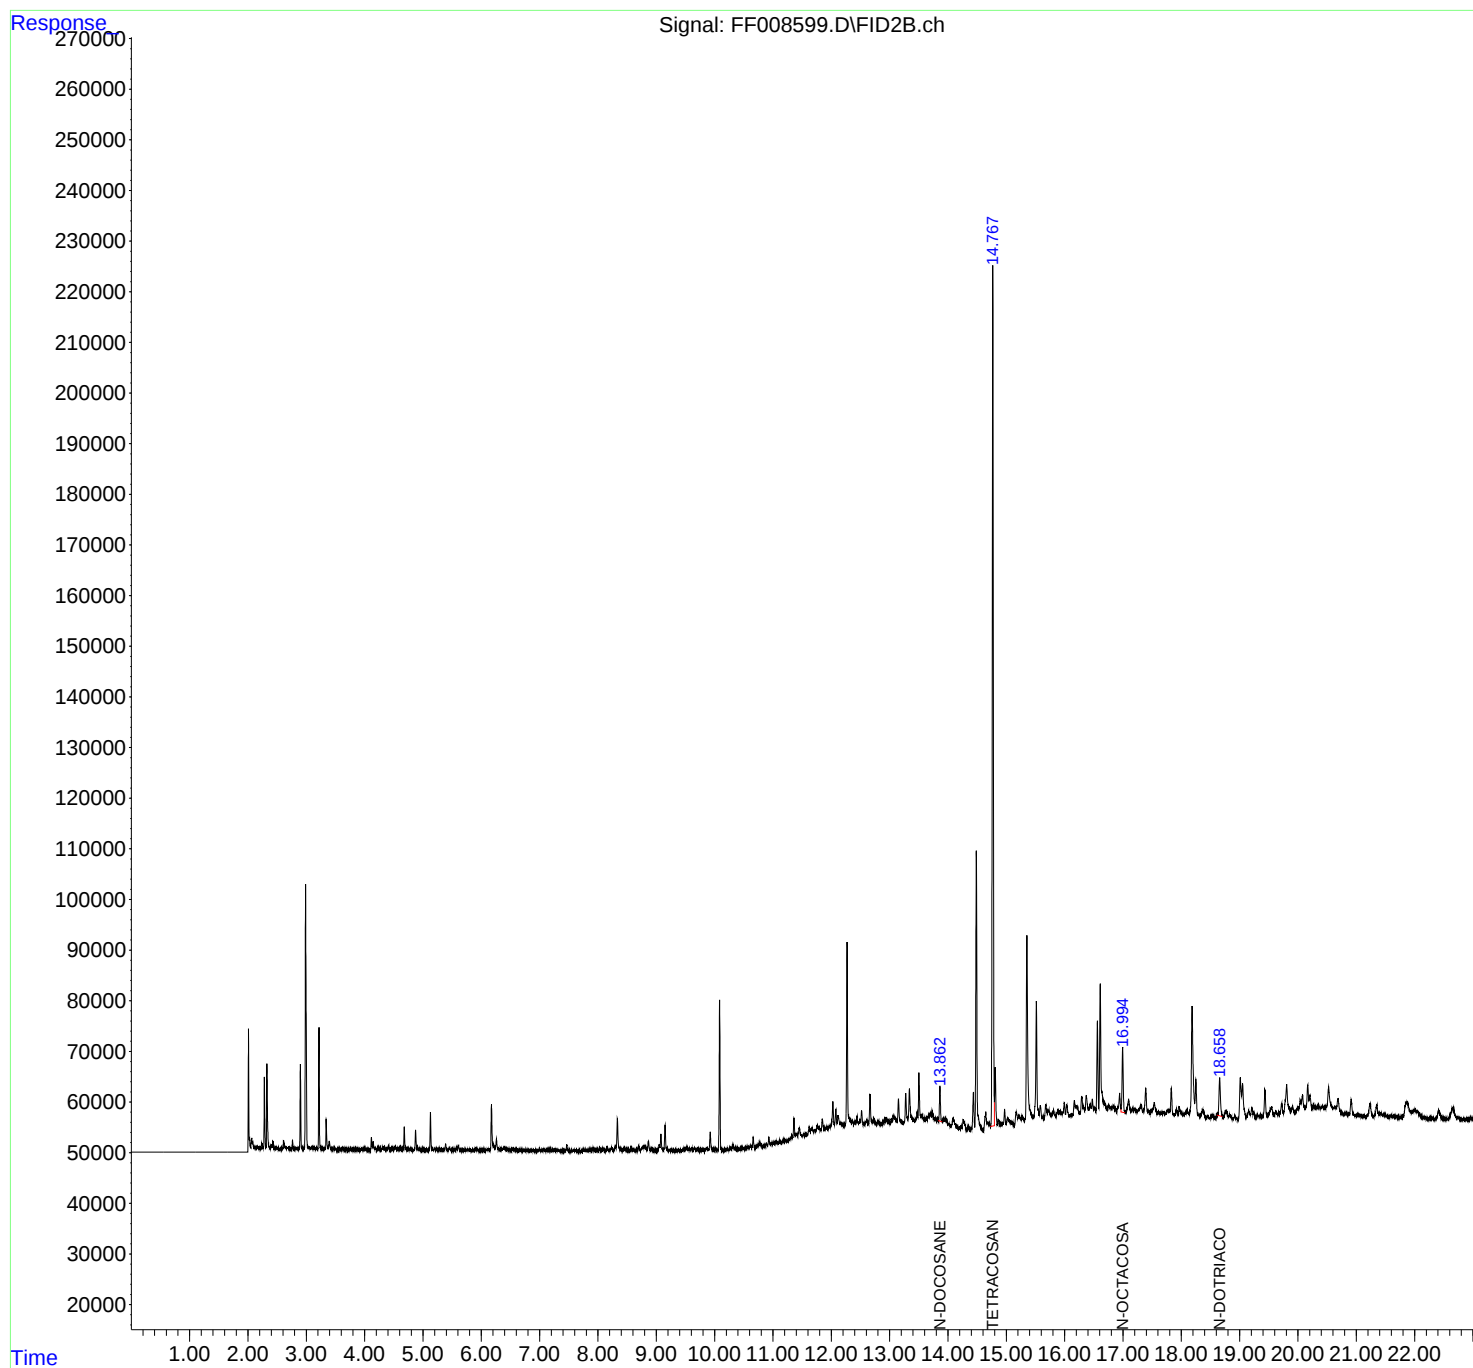


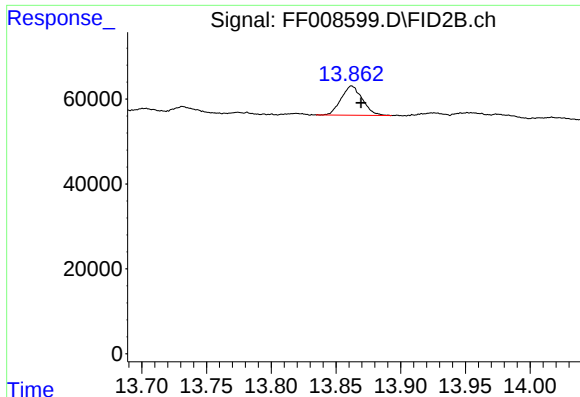

#8 N-DOCOSANE


R.T.: 13.862 min
Delta R.T.: -0.007 min
Response: 78561
Conc: 0.62 ug/ml

Instrument :
FID_F
ClientSampleId :

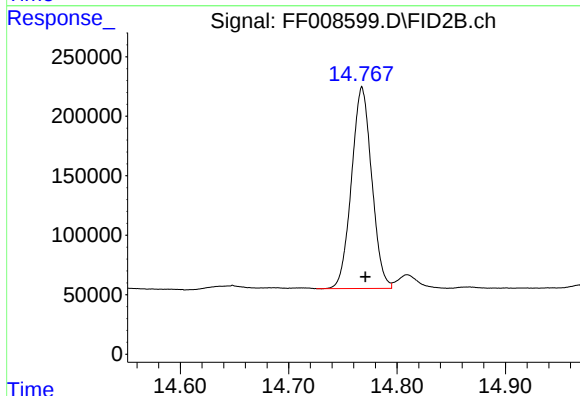


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.768 min
Delta R.T.: -0.003 min
Response: 2194091
Conc: 20.82 ug/ml

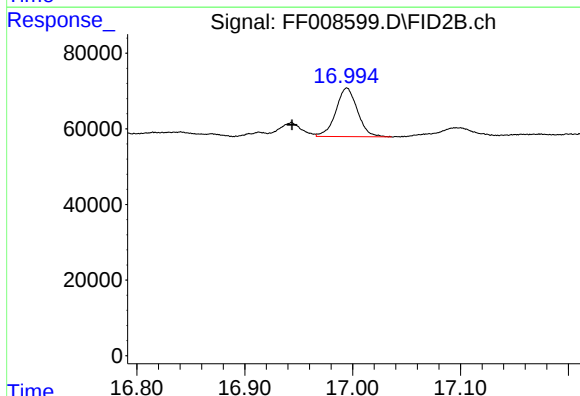

#12 N-OCTACOSANE

R.T.: 16.995 min
Delta R.T.: 0.051 min
Response: 178030
Conc: 1.50 ug/ml

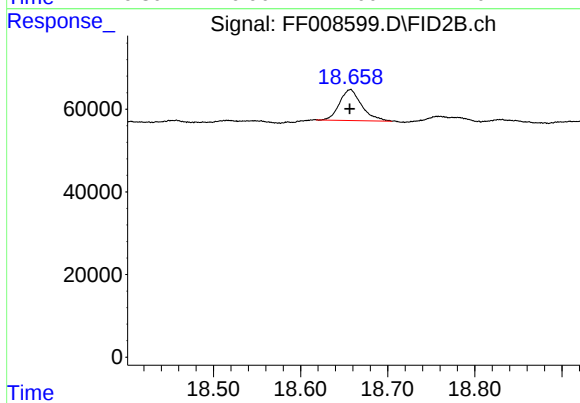

#14 N-DOTRIACONTANE

R.T.: 18.657 min
Delta R.T.: 0.000 min
Response: 131577
Conc: 1.09 ug/ml