

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061321\
 Data File : FF008603.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jun 2021 12:23
 Operator : DD\AJ
 Sample : M2639-03
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 14 07:20:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.772	2229223	21.157 ug/ml
Target Compounds			
3) N-DODECANE	6.507	69503	0.557 ug/ml
4) N-TETRADECANE	8.331	138653	1.090 ug/ml
5) N-HEXADECANE	9.948	369749	2.925 ug/ml
6) N-OCTADECANE	11.375	205678	1.623 ug/ml
7) N-EICOSANE	12.667	375252	2.939 ug/ml
8) N-DOCOSANE	13.869	322916	2.569 ug/ml
10) N-TETRACOSANE	14.978	4357407	35.560 ug/ml
11) N-HEXACOSANE	16.008	88152	0.735 ug/ml
12) N-OCTACOSANE	16.948	269486	2.272 ug/ml
13) N-TRIACONTANE	17.836	1597576	13.489 ug/ml
14) N-DOTRIACONTANE	18.660	803197	6.674 ug/ml
15) N-TETRATRIACONTANE	19.442	1349112	12.287 ug/ml
16) N-HEXATRIACONTANE	20.176	1609959	14.520 ug/ml
17) N-OCTATRIACONTANE	20.924	233053	2.297 ug/ml
18) N-TETRACONTANE	21.855	380310	3.600 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061321\
Data File : FF008603.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2021 12:23
Operator : DD\AJ
Sample : M2639-03
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 07:20:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

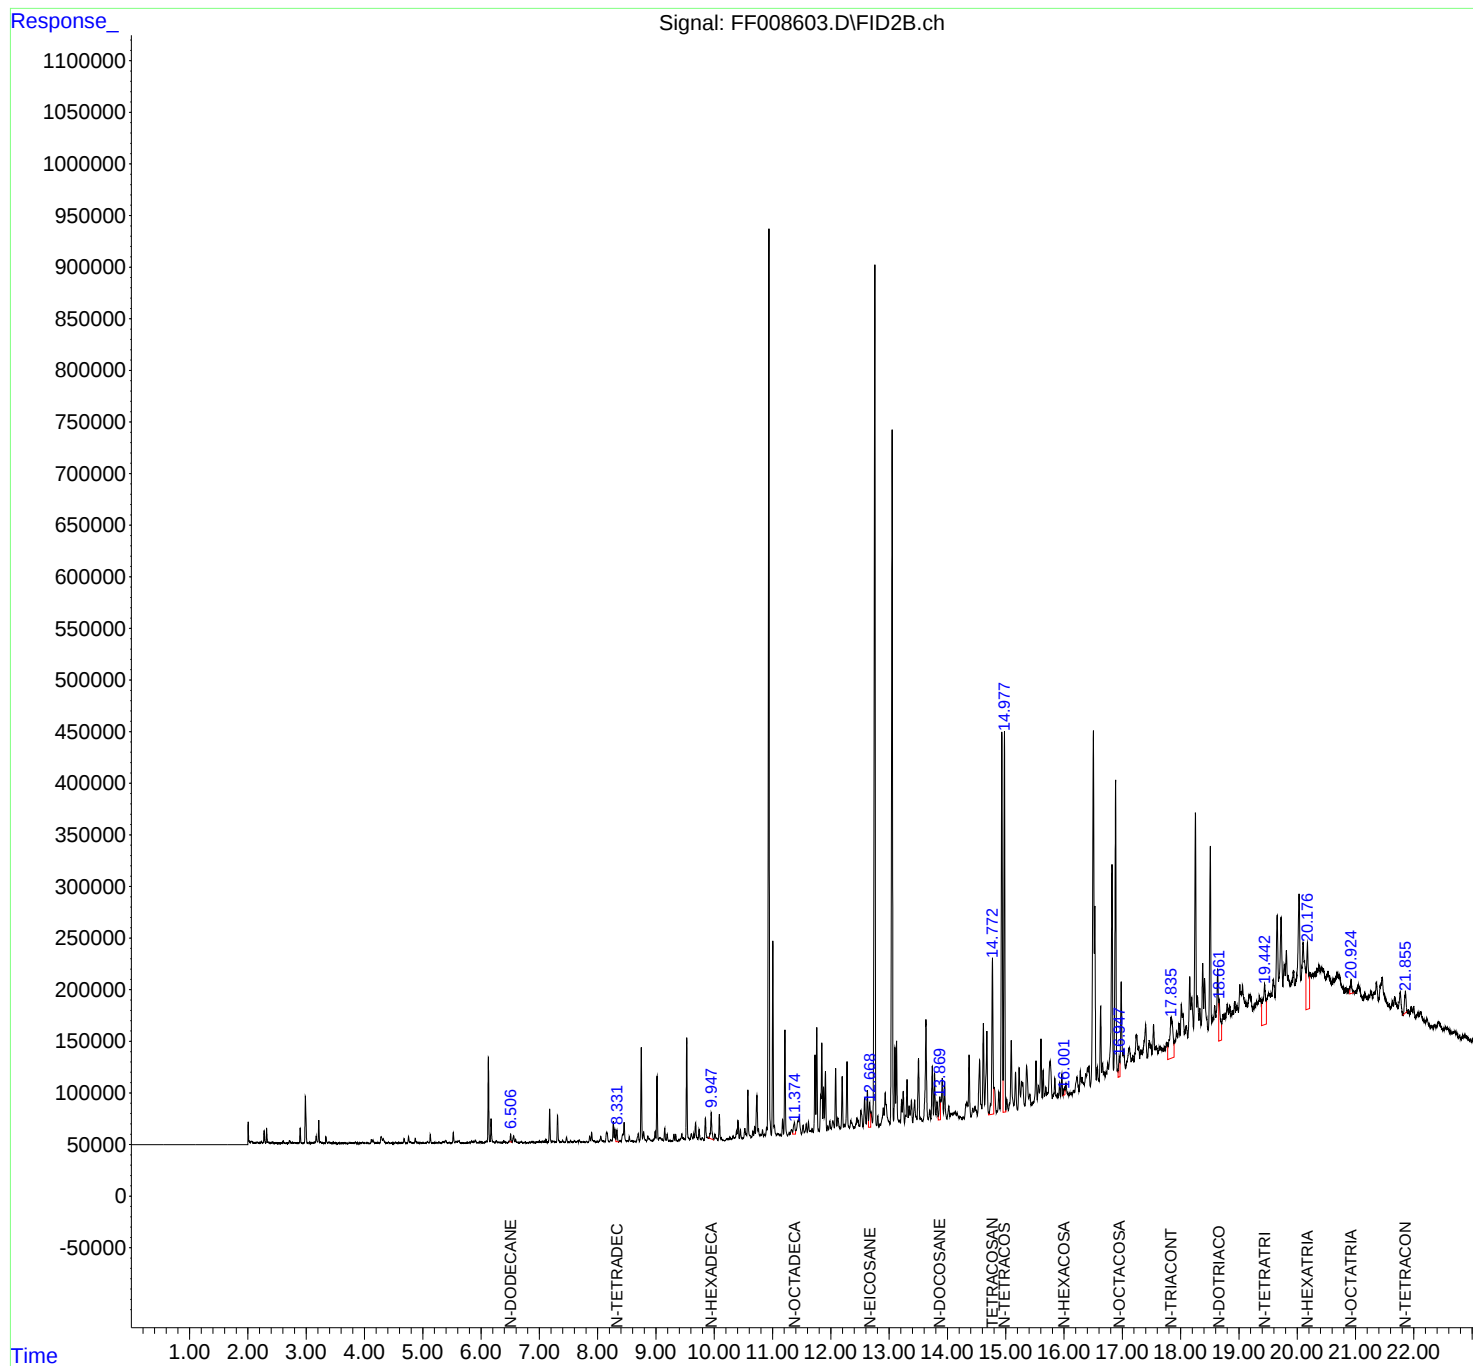


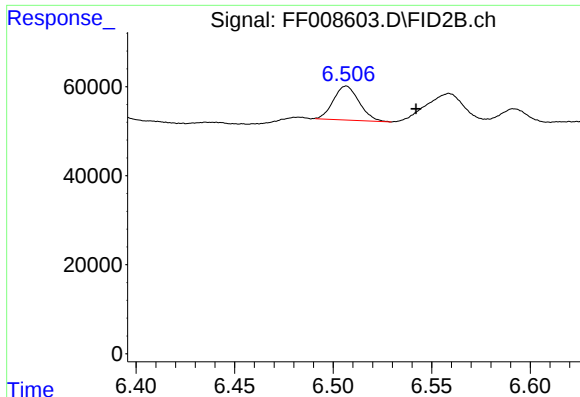

#3 N-DODECANE


R.T.: 6.507 min
Delta R.T.: -0.035 min
Response: 69503
Conc: 0.56 ug/ml

Instrument :
FID_F
ClientSampleId :

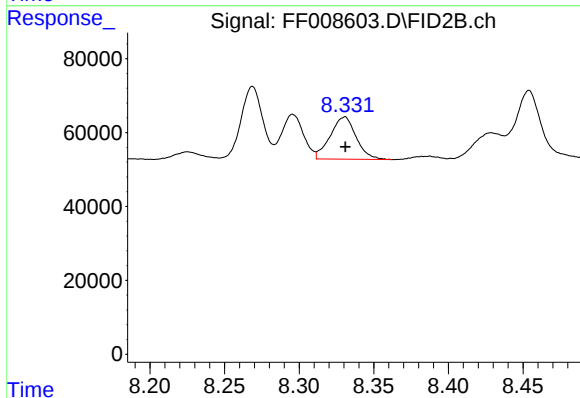


#4 N-TETRADECANE

R.T.: 8.331 min
Delta R.T.: 0.000 min
Response: 138653
Conc: 1.09 ug/ml

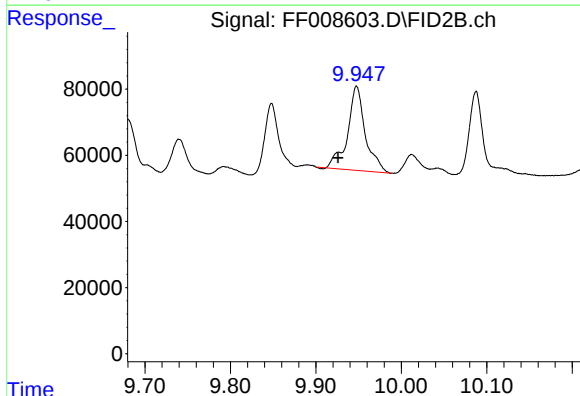


#5 N-HEXADECANE

R.T.: 9.948 min
Delta R.T.: 0.022 min
Response: 369749
Conc: 2.93 ug/ml

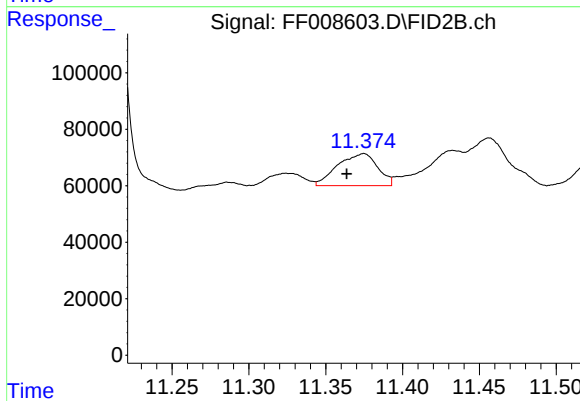

#6 N-OCTADECANE


R.T.: 11.375 min
Delta R.T.: 0.011 min
Response: 205678
Conc: 1.62 ug/ml

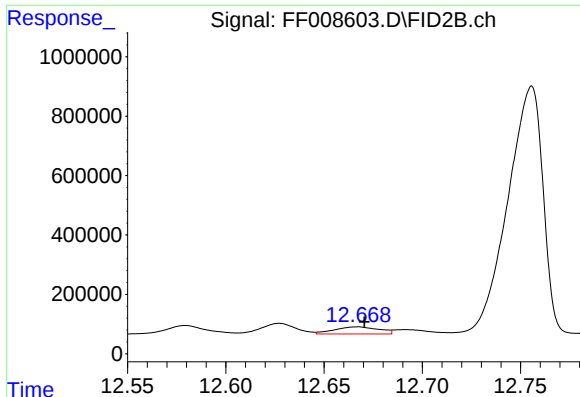

#7 N-EICOSANE


R.T.: 12.667 min
Delta R.T.: -0.003 min
Response: 375252
Conc: 2.94 ug/ml

Instrument :
FID_F
ClientSampleId :

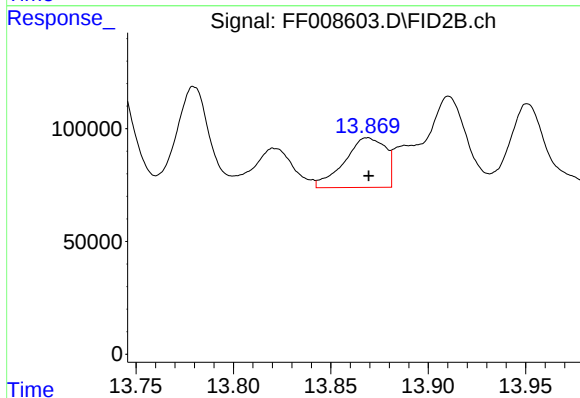


#8 N-DOCOSANE

R.T.: 13.869 min
Delta R.T.: 0.000 min
Response: 322916
Conc: 2.57 ug/ml

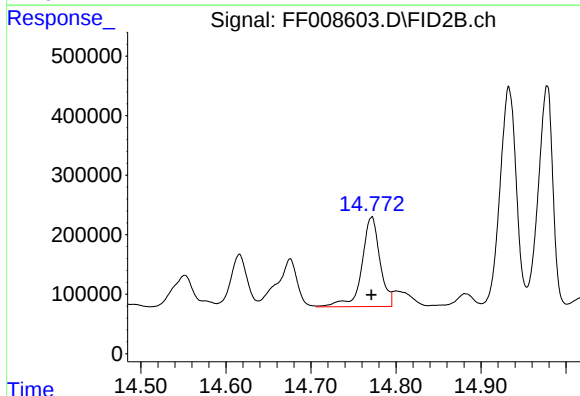


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.772 min
Delta R.T.: 0.000 min
Response: 2229223
Conc: 21.16 ug/ml

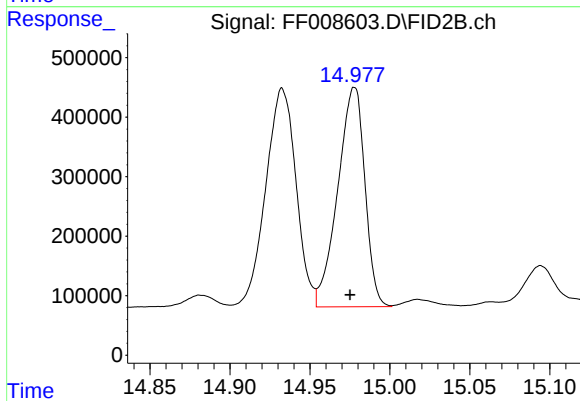

#10 N-TETRACOSANE


R.T.: 14.978 min
Delta R.T.: 0.003 min
Response: 4357407
Conc: 35.56 ug/ml

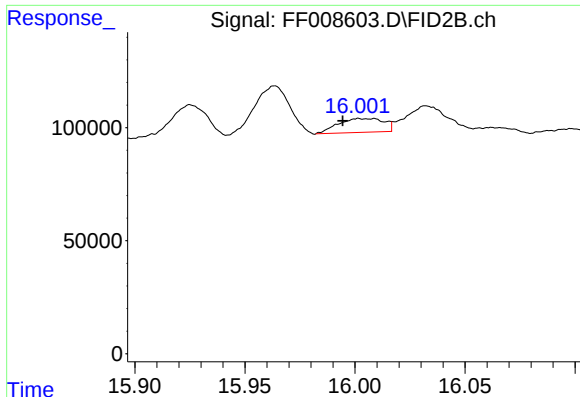

#11 N-HEXACOSANE


R.T.: 16.008 min
Delta R.T.: 0.014 min
Response: 88152
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :

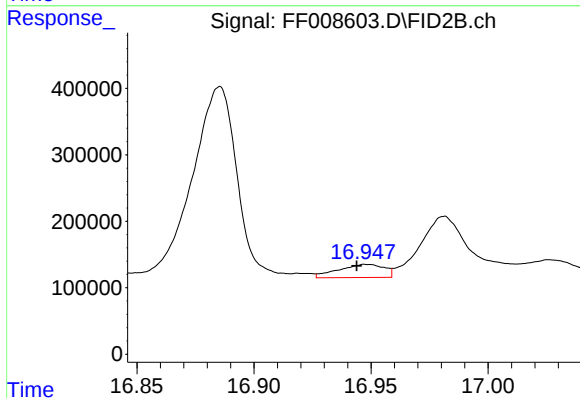


#12 N-OCTACOSANE

R.T.: 16.948 min
Delta R.T.: 0.004 min
Response: 269486
Conc: 2.27 ug/ml

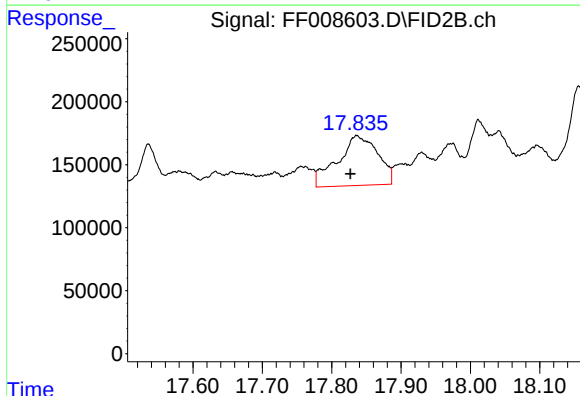


#13 N-TRIACONTANE

R.T.: 17.836 min
Delta R.T.: 0.009 min
Response: 1597576
Conc: 13.49 ug/ml

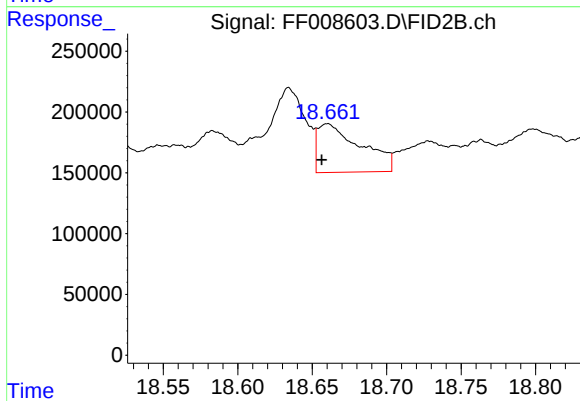

#14 N-DOTRIACONTANE


R.T.: 18.660 min
Delta R.T.: 0.004 min
Response: 803197
Conc: 6.67 ug/ml

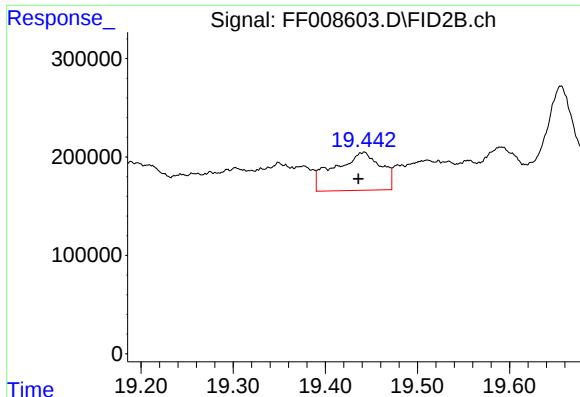

#15 N-TETRATRIACONTANE


R.T.: 19.442 min
Delta R.T.: 0.006 min
Response: 1349112
Conc: 12.29 ug/ml

Instrument :
FID_F
ClientSampleId :

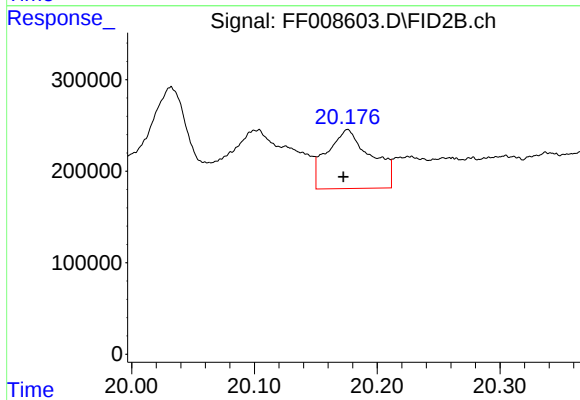


#16 N-HEXATRIACONTANE

R.T.: 20.176 min
Delta R.T.: 0.004 min
Response: 1609959
Conc: 14.52 ug/ml

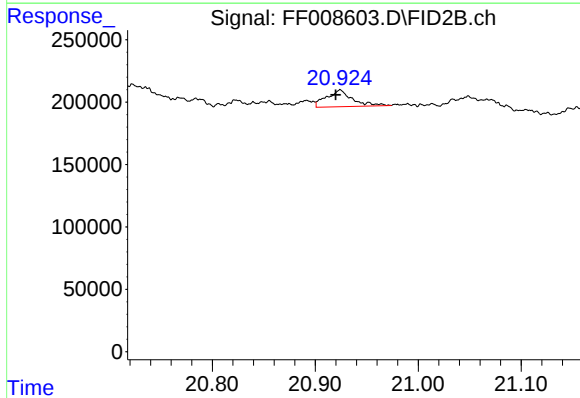

#17 N-OCTATRIACONTANE

R.T.: 20.924 min
Delta R.T.: 0.004 min
Response: 233053
Conc: 2.30 ug/ml

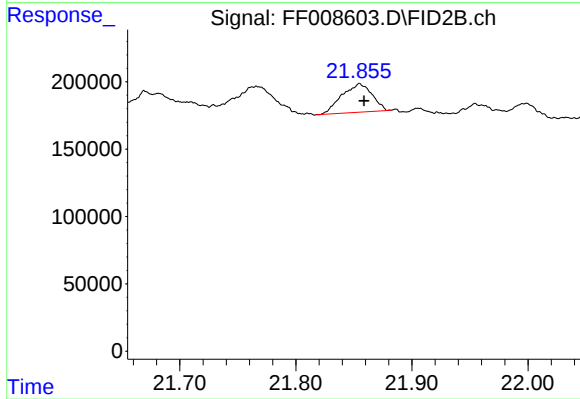

#18 N-TETRACONTANE

R.T.: 21.855 min
Delta R.T.: -0.004 min
Response: 380310
Conc: 3.60 ug/ml